
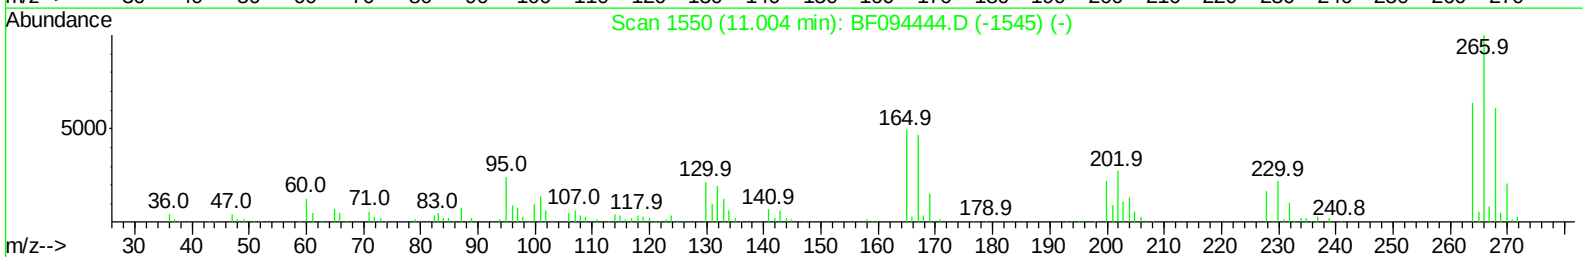
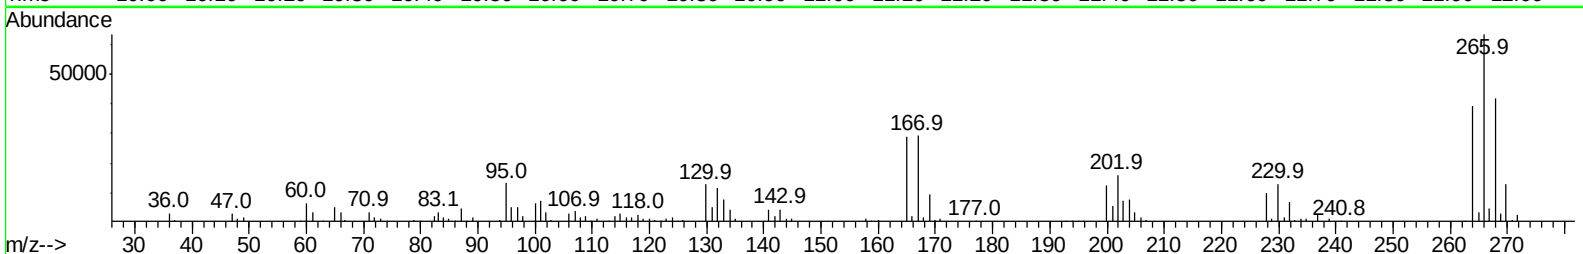


Data Path : Z:\HPCHEM1\BNA F\Data\BF042117\
Data File : BF094558.D
Acq On : 21 Apr 2017 10:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 18:57:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

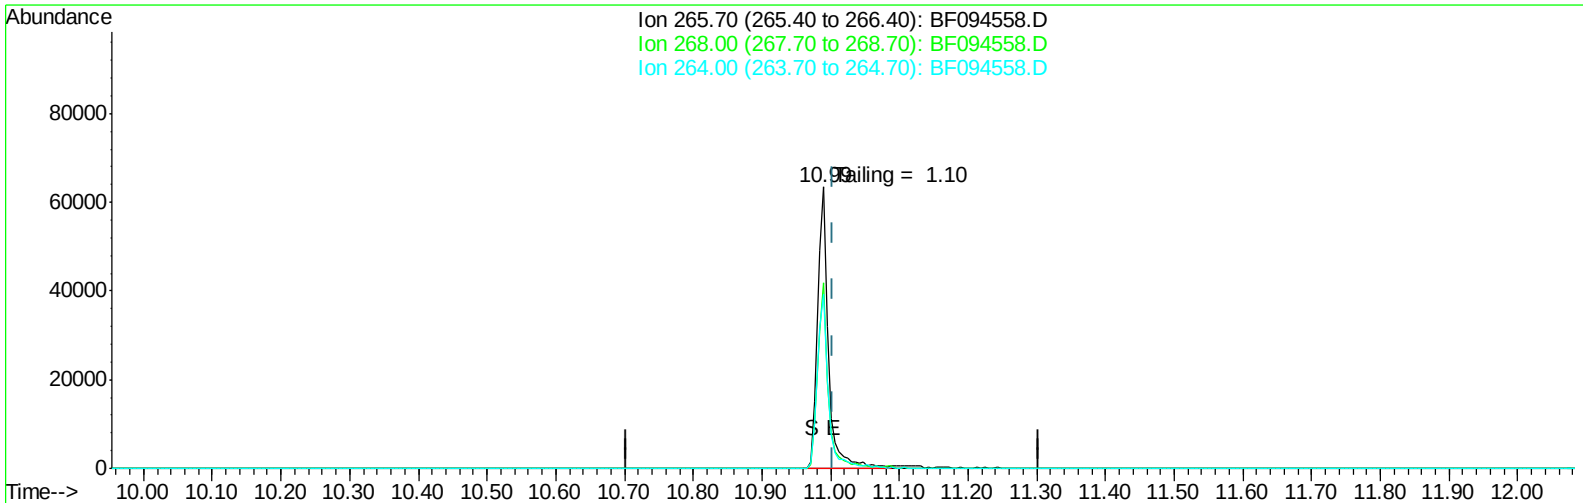

TIC: BF094558.D

(69) Pentachlorophenol (C)




10.989min (-0.015) 0.00ng

response 69257

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.00
264.00	64.60	61.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF042117\
Data File : BF094558.D
Acq On : 21 Apr 2017 10:33
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 18:57:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

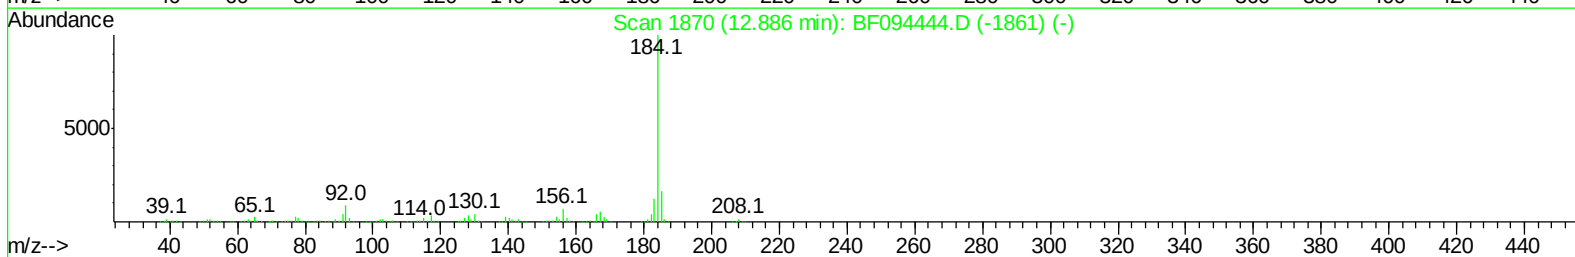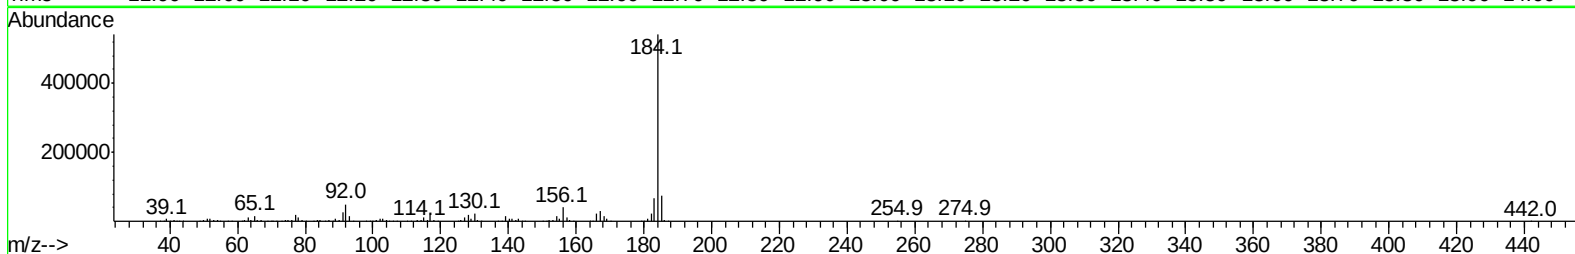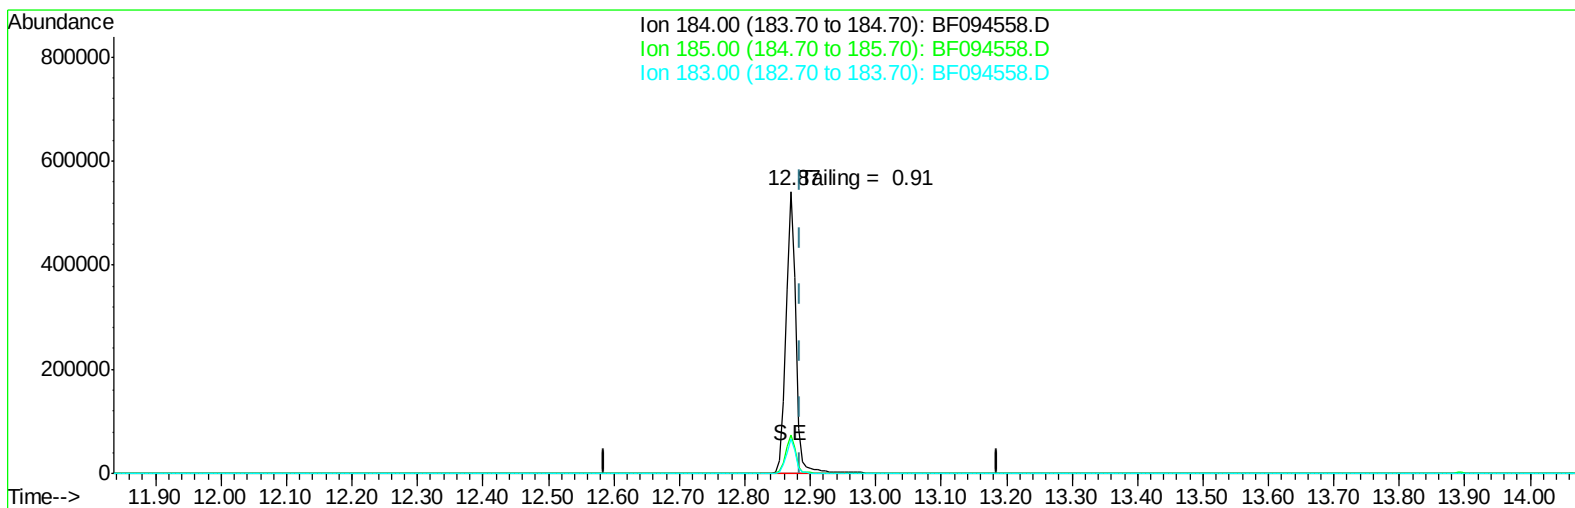

TIC: BF094558.D

(76) Benzidine

12.871min (-0.015) 0.00ng

response 572854

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.81#
183.00	12.20	12.17
0.00	0.00	0.00