
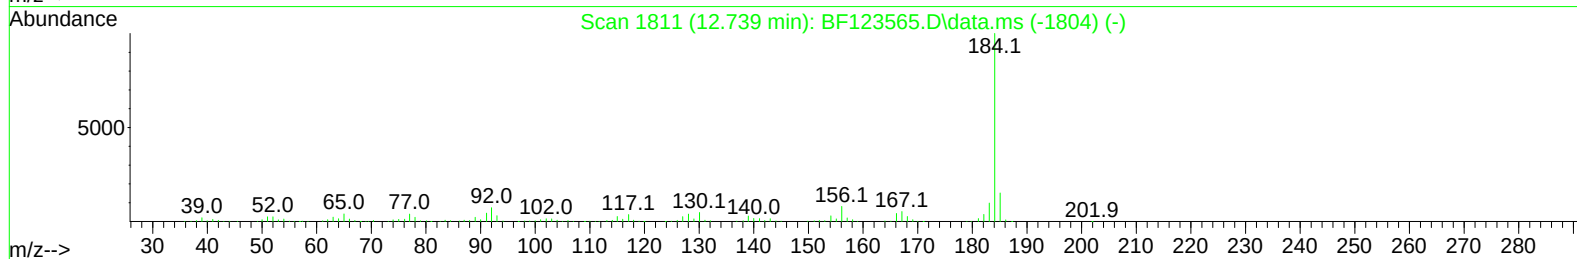
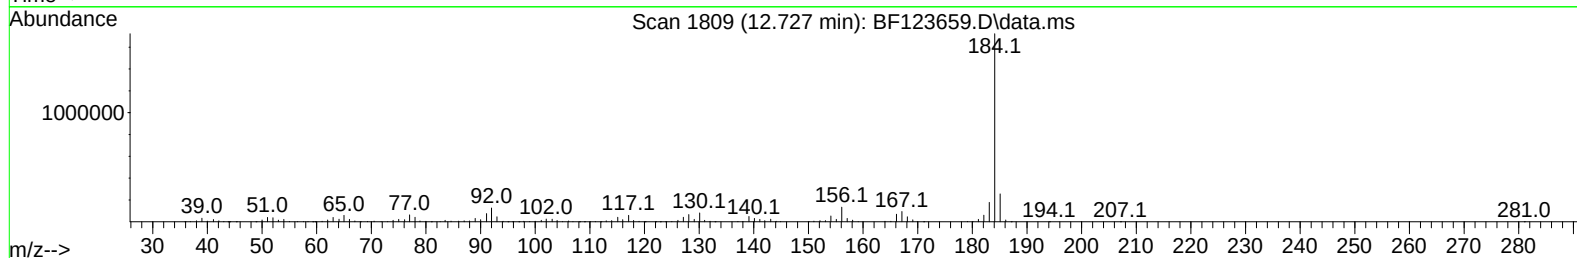


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042121\
Data File : BF123659.D
Acq On : 21 Apr 2021 10:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 11:59:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

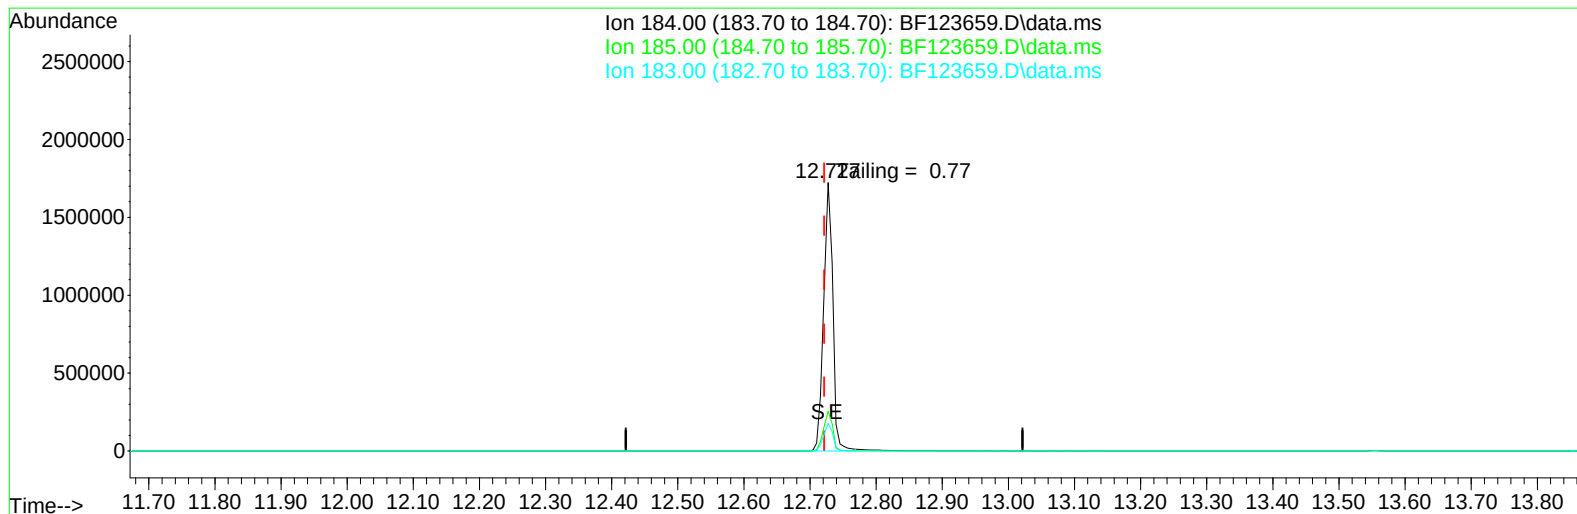

TIC: BF123659.D\data.ms

(77) Benzidine




12.727min (+ 0.006) 42053.20 ng

response 1685022

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.80
183.00	9.80	10.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042121\
Data File : BF123659.D
Acq On : 21 Apr 2021 10:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 21 11:59:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

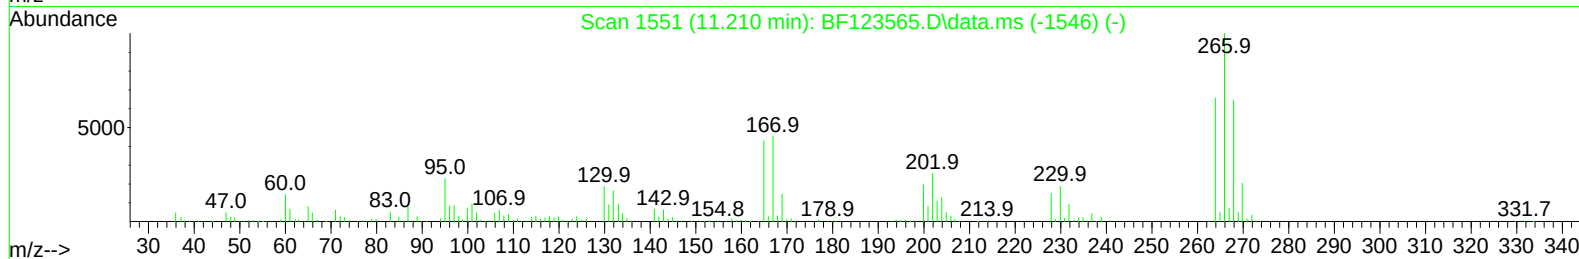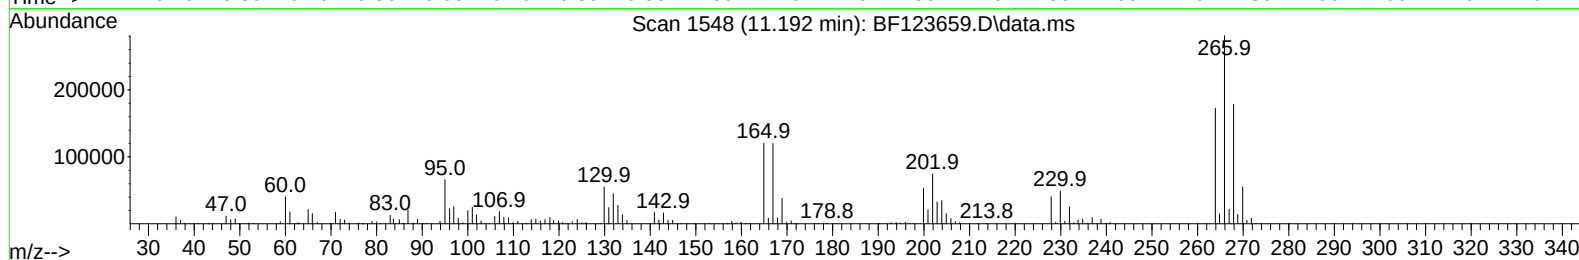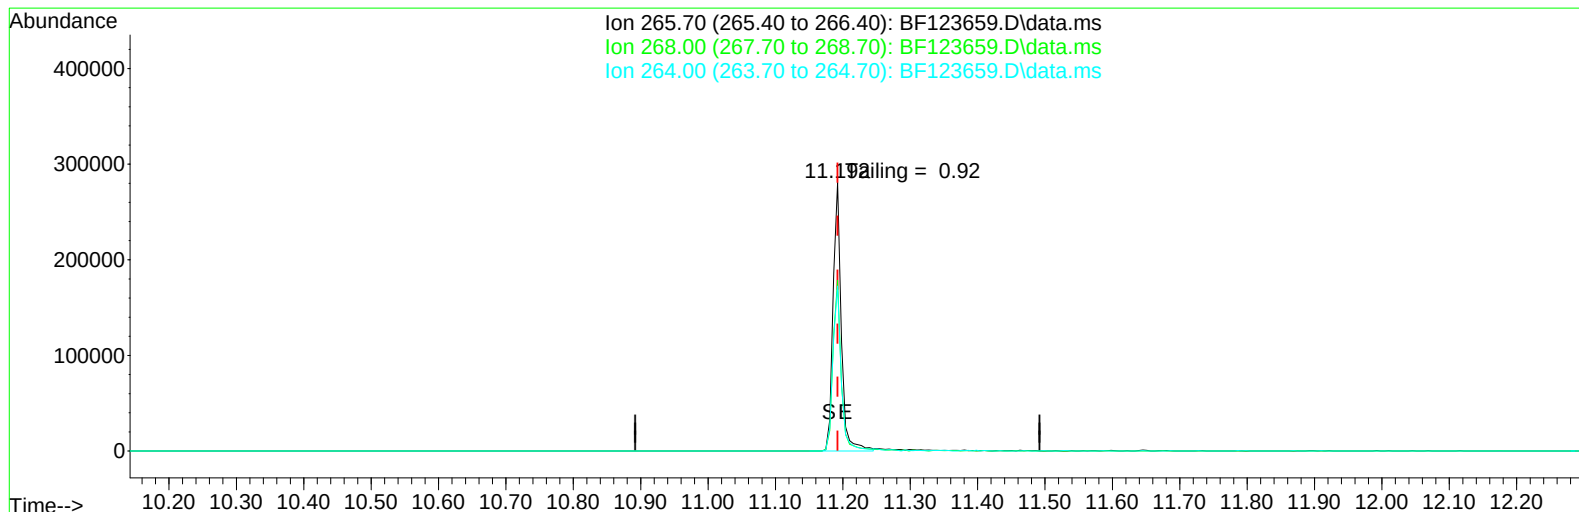

TIC: BF123659.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.000) 102193.50 ng

response 244718

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.52
264.00	65.70	61.47
0.00	0.00	0.00