
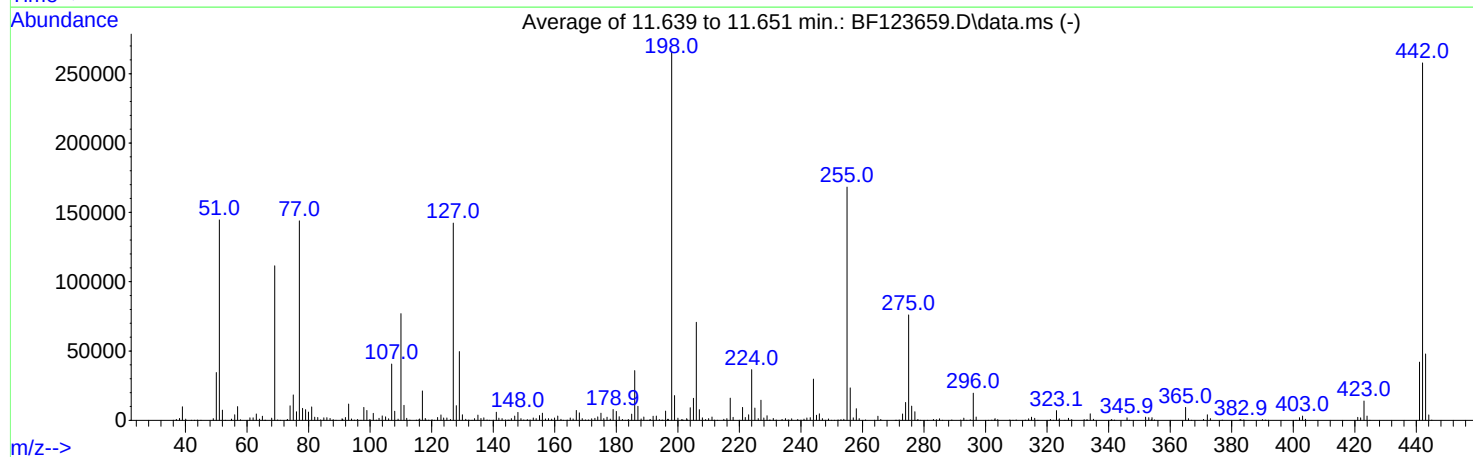


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042121\
 Data File : BF123659.D
 Acq On : 21 Apr 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 20 15:49:40 2021

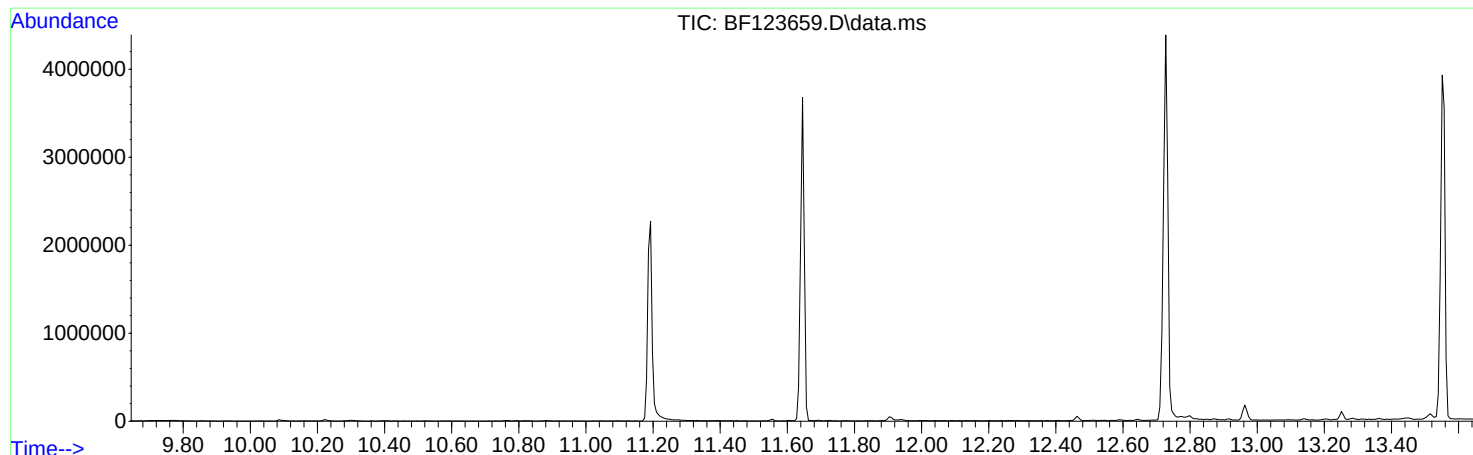




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	144608	PASS
68	69	0.00	2	1.4	1590	PASS
69	198	0.00	100	42.0	111507	PASS
70	69	0.00	2	0.3	383	PASS
127	198	10	80	53.7	142339	PASS
197	198	0.00	2	0.3	856	PASS
198	198	100	100	100.0	265301	PASS
199	198	5	9	6.7	17871	PASS
275	198	10	60	28.7	76075	PASS
365	198	1	100	3.5	9319	PASS
441	198	0.01	100	15.8	42003	PASS
442	442	50	100	100.0	257779	PASS
443	442	15	24	18.6	47939	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042121\
Data File : BF123659.D
Acq On : 21 Apr 2021 10:33
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 21 11:59:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 15:49:40 2021
Response via : Initial Calibration

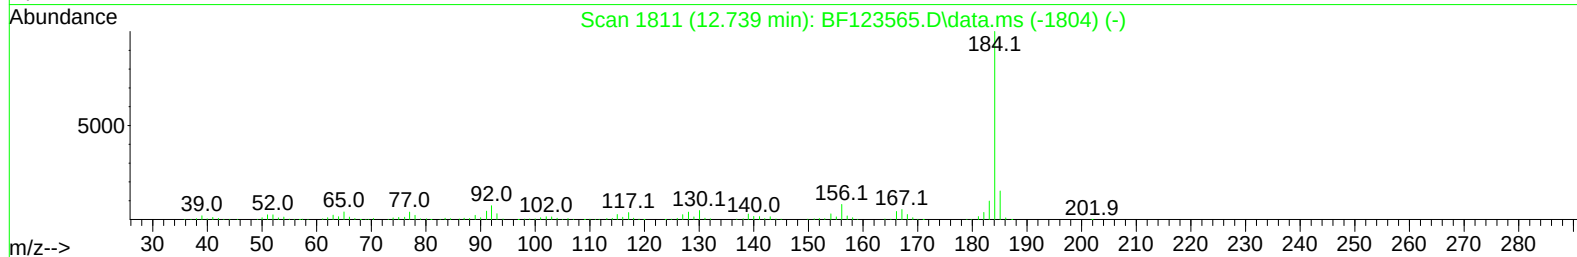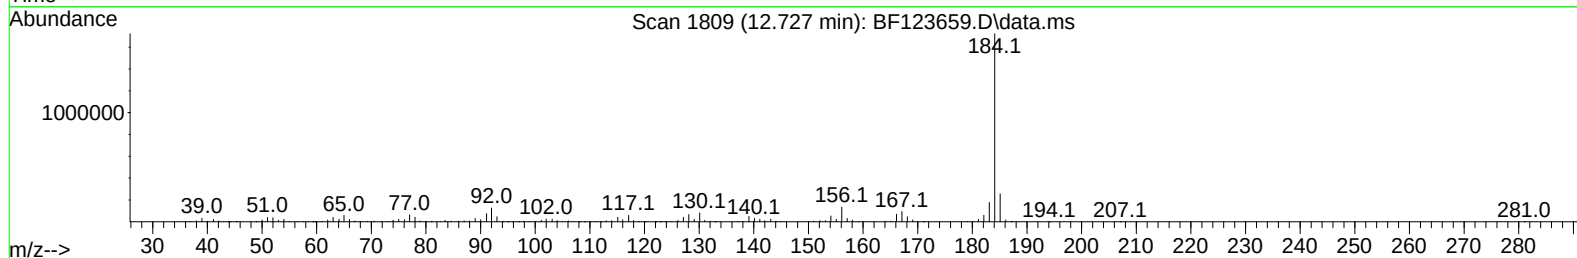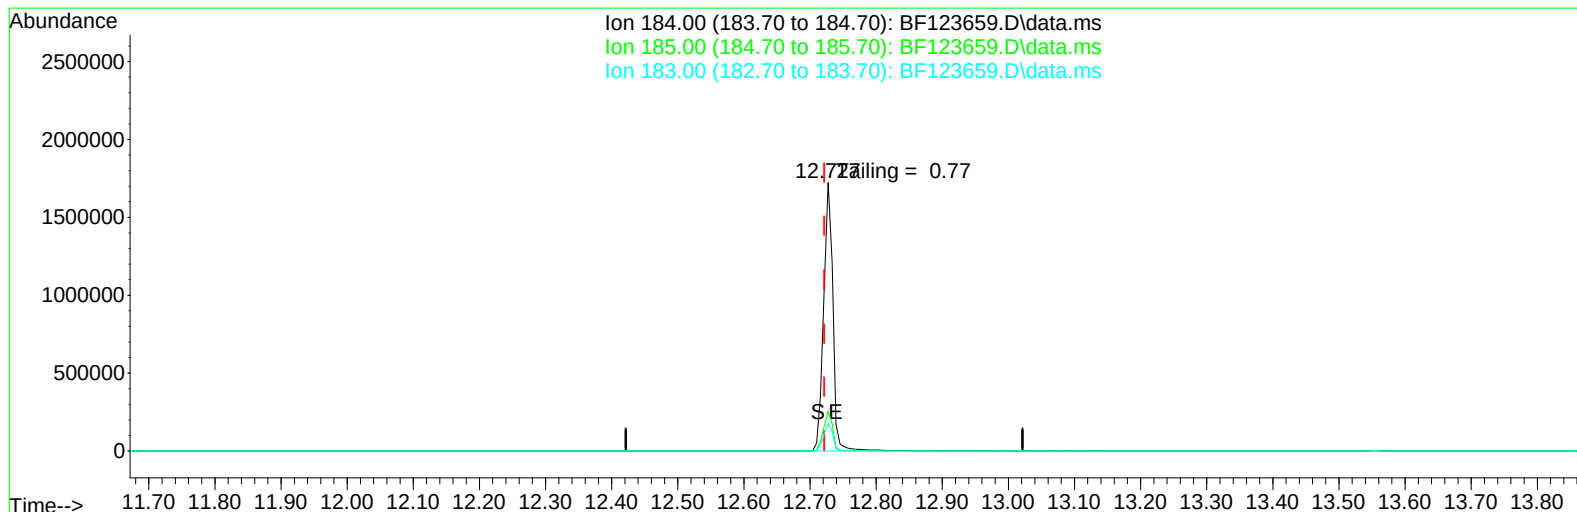

TIC: BF123659.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 42053.20 ng




response 1685022

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.80
183.00	9.80	10.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042121\
 Data File : BF123659.D
 Acq On : 21 Apr 2021 10:33
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 21 11:59:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 15:49:40 2021
 Response via : Initial Calibration

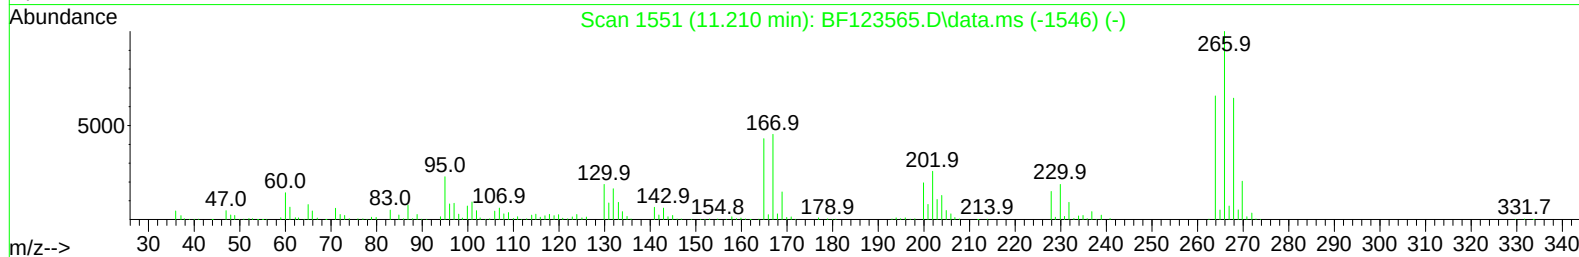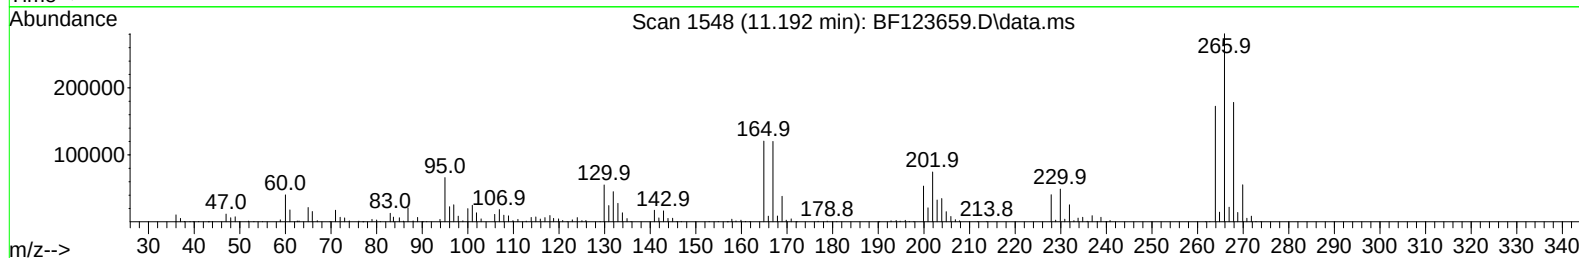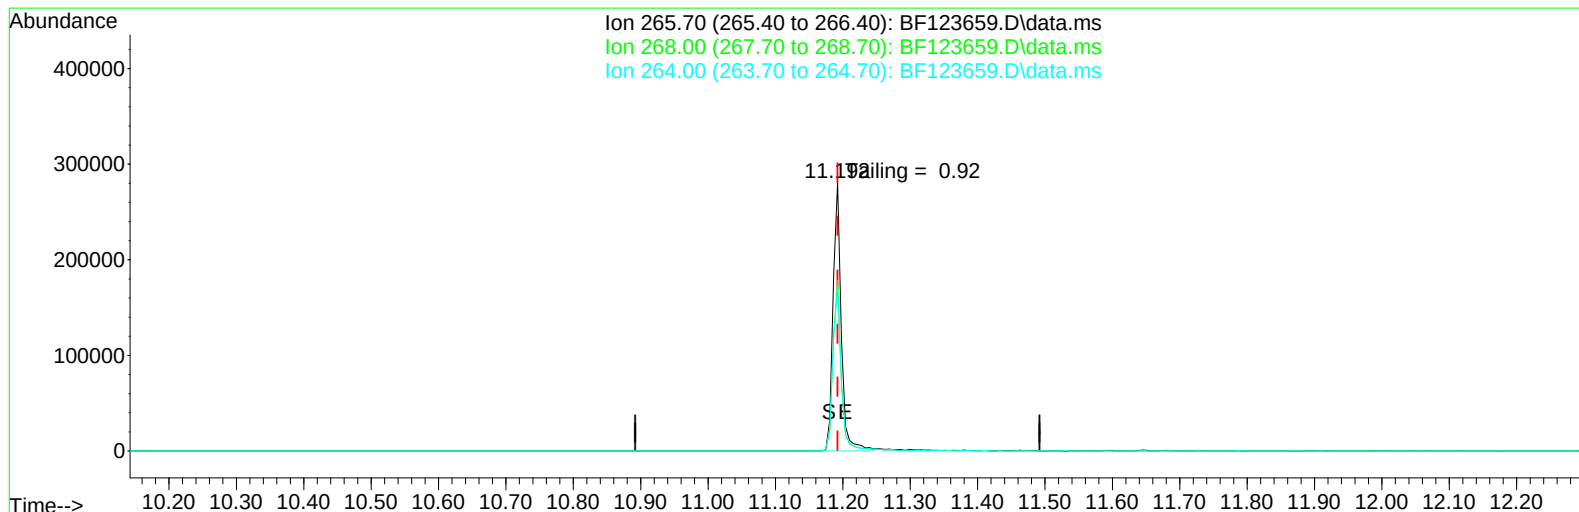

TIC: BF123659.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.000) 102193.50 ng

response 244718

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.52
264.00	65.70	61.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/21/2021	BNA_F	<u>BF123659.D</u>
Compound Name	Response	Retention Time
DDT	662314	13.55
DDD	13517	13.25
DDE	1775	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15292	677606	2.26

Instrument :
BNA_F
ClientSampleId :
DFTPP