

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042215\
 Data File : BF078730.D
 Acq On : 22 Apr 2015 22:40
 Operator : TP/IZ
 Sample : PB82930BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB82930BL

Quant Time: Apr 23 01:15:23 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 23 00:55:17 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.78	152	24619	20.00	ng	-0.01
21) Naphthalene-d8	7.94	136	99625	20.00	ng	-0.01
38) Acenaphthene-d10	11.13	164	51007	20.00	ng	0.00
63) Phenanthrene-d10	13.86	188	105062	20.00	ng	0.00
75) Chrysene-d12	17.74	240	114754	20.00	ng	0.00
86) Perylene-d12	19.42	264	114181	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	3.80	112	181376	121.47	ng	0.00
7) Phenol-d6	5.29	99	230160	123.00	ng	0.00
23) Nitrobenzene-d5	6.72	82	130705	79.52	ng	-0.01
41) 2,4,6-Tribromophenol	12.61	330	57992	137.09	ng	0.00
44) 2-Fluorobiphenyl	9.96	172	286886	80.40	ng	0.00
78) Terphenyl-d14	16.40	244	367009	72.27	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042215\
Data File : BF078730.D
Acq On : 22 Apr 2015 22:40
Operator : TP/IZ
Sample : PB82930BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB82930BL

Quant Time: Apr 23 01:15:23 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 00:55:17 2015
Response via : Initial Calibration

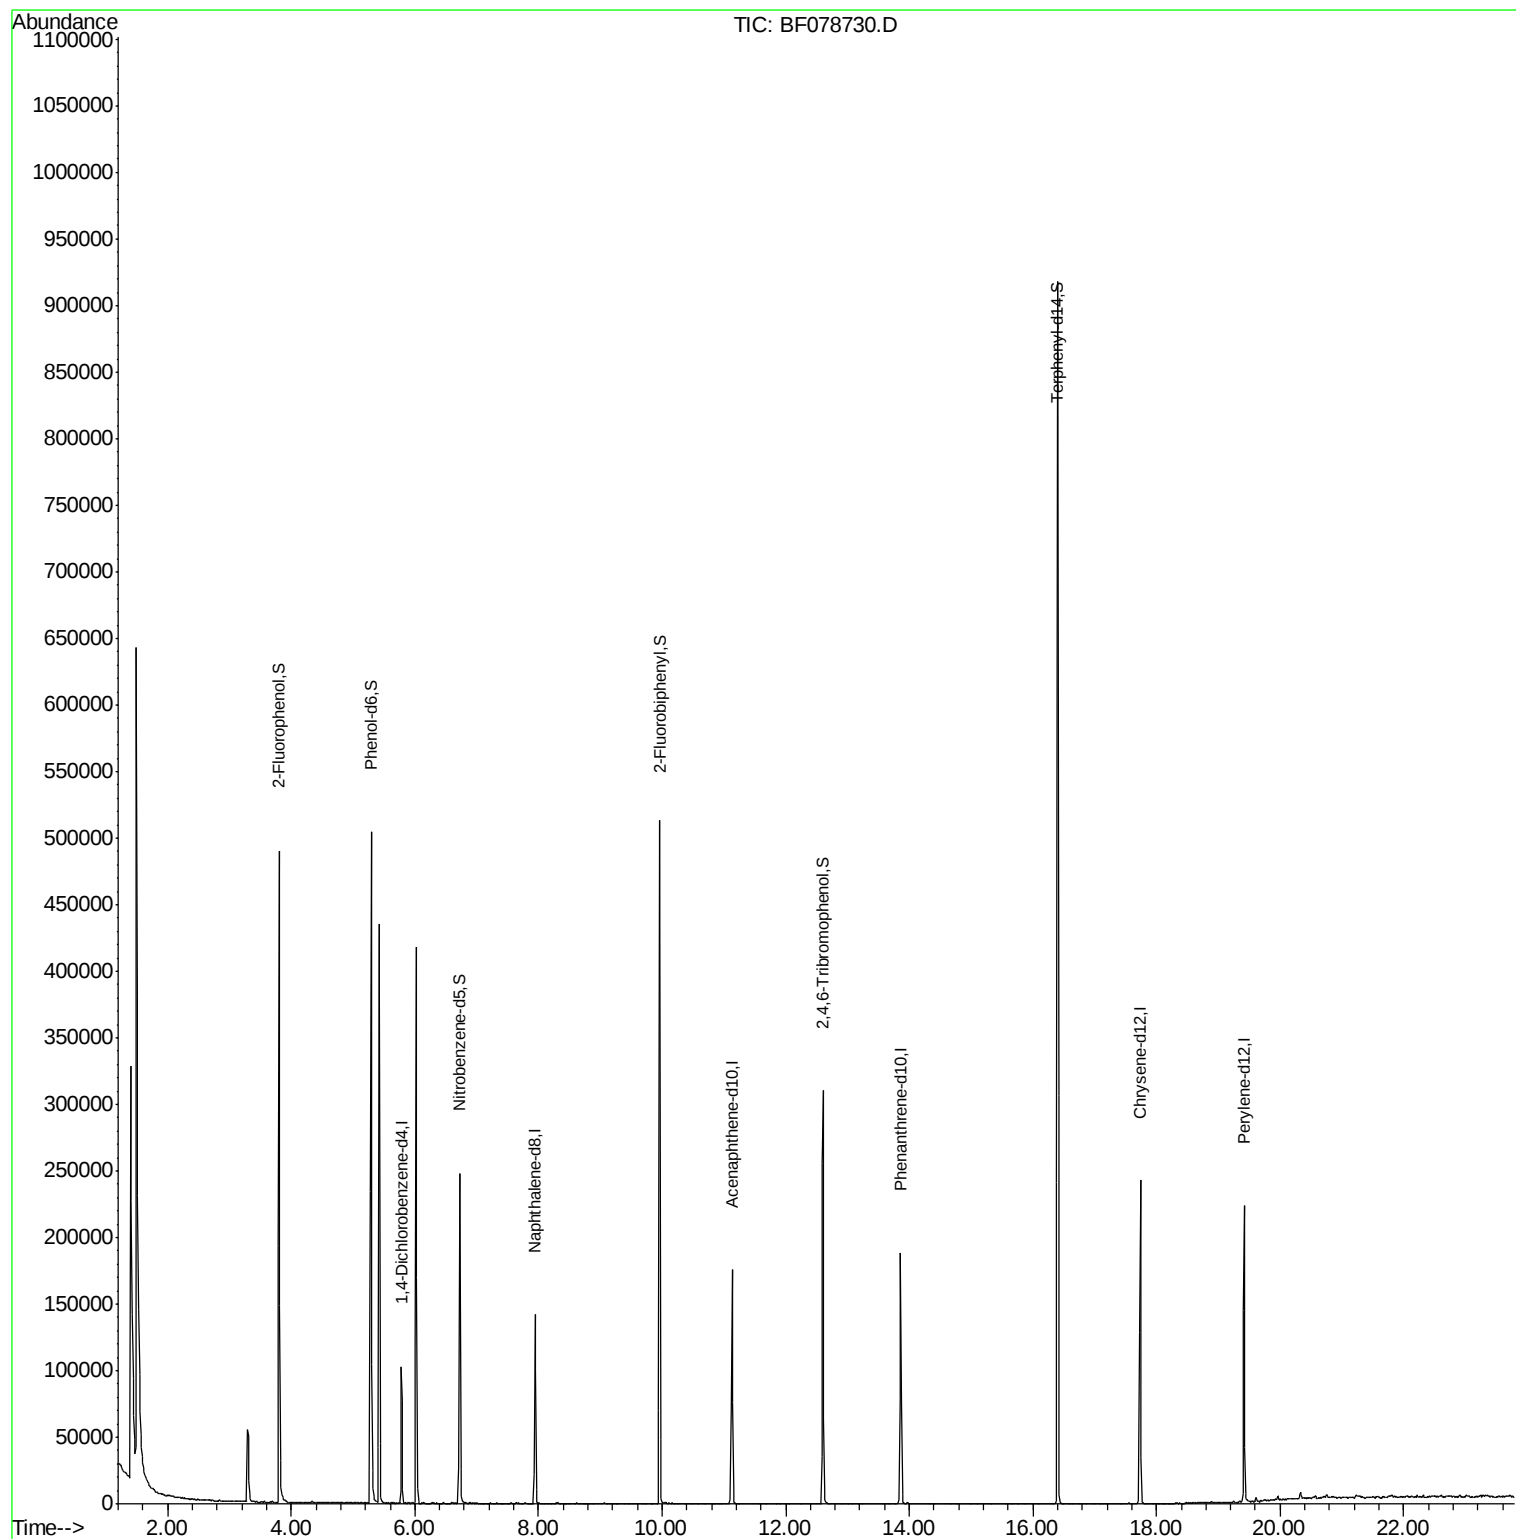

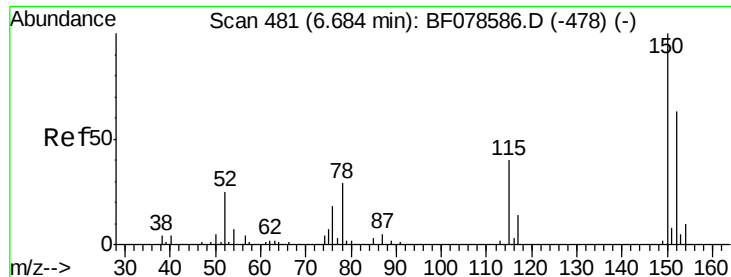


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.78 min Scan# 402
Delta R.T. -0.01 min
Lab File: BF078730.D
Acq: 22 Apr 2015 22:40

Instrument :
BNA_F
ClientSampleId :
PB82930BL

Tgt Ion:152 Resp: 24619
Ion Ratio Lower Upper
152 100
150 166.2 125.9 188.9
115 67.9 52.7 79.1

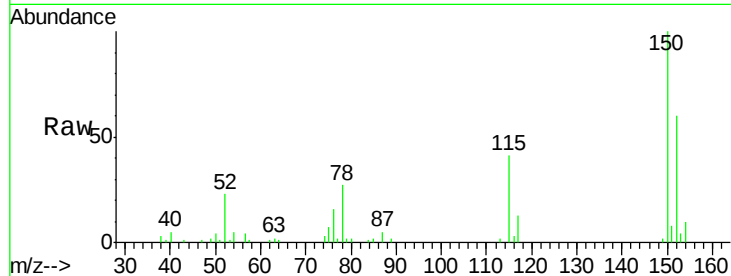


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

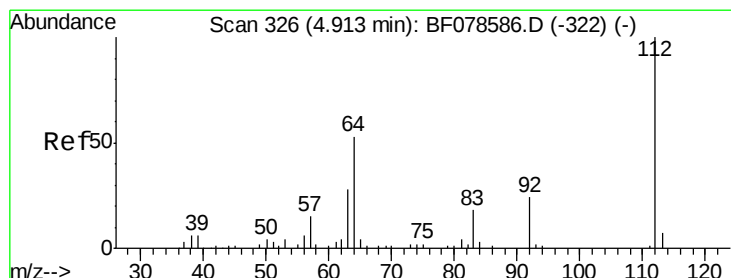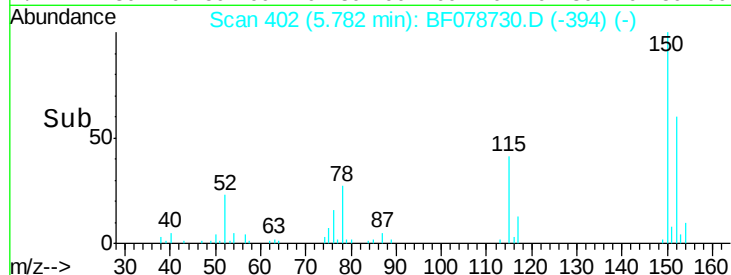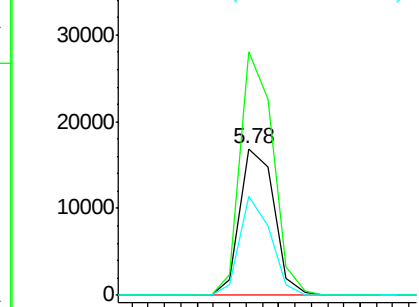



#5


2-Fluorophenol
Concen: 121.47 ng
RT: 3.80 min Scan# 229
Delta R.T. 0.00 min
Lab File: BF078730.D
Acq: 22 Apr 2015 22:40

Tgt Ion:112 Resp: 181376
Ion Ratio Lower Upper
112 100
64 55.0 39.9 59.9
63 28.9 20.2 30.4

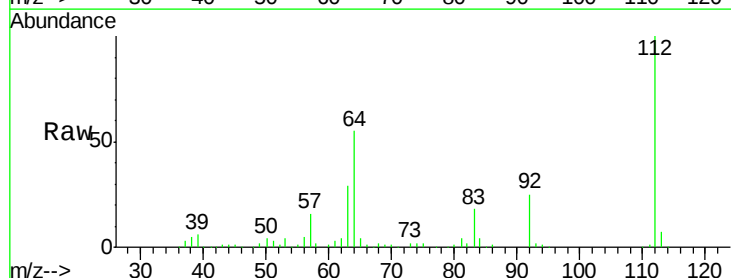

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

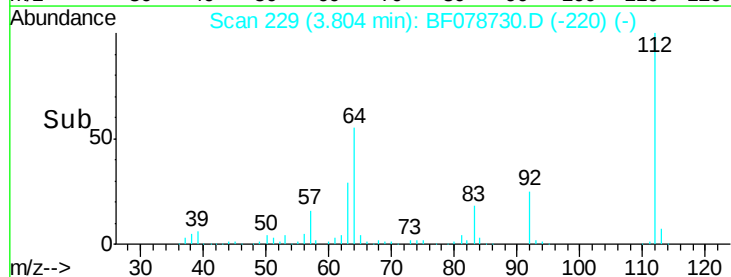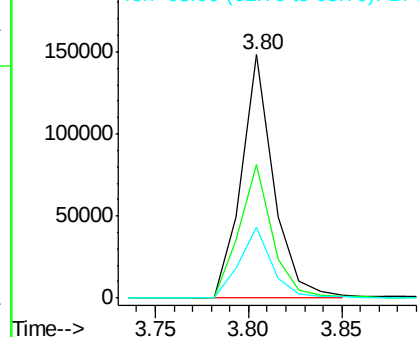

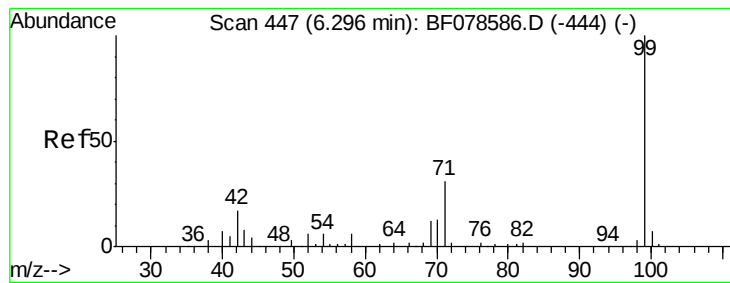

#7

Phenol-d6

Concen: 123.00 ng

RT: 5.29 min Scan# 359

Delta R.T. 0.00 min

Lab File: BF078730.D

Acq: 22 Apr 2015 22:40

Instrument :

BNA_F

ClientSampleId :

PB82930BL


Tgt Ion: 99 Resp: 230160

Ion Ratio Lower Upper

99 100

42 16.4 14.8 22.2




71 32.7 26.6 39.8

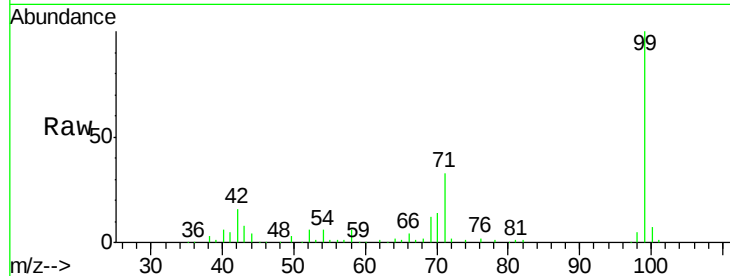

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

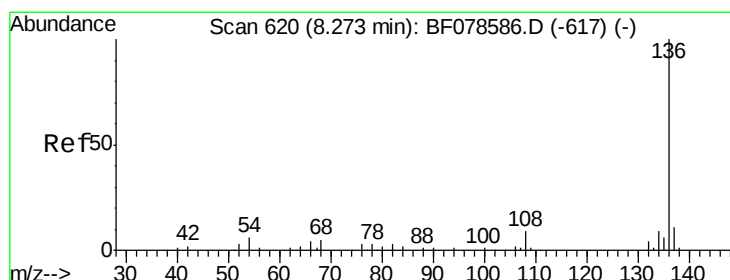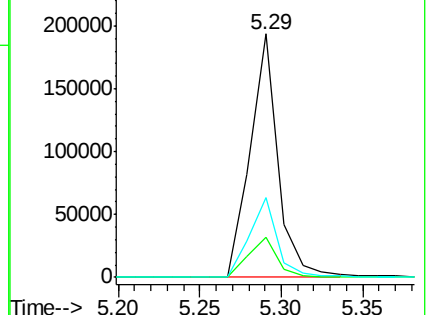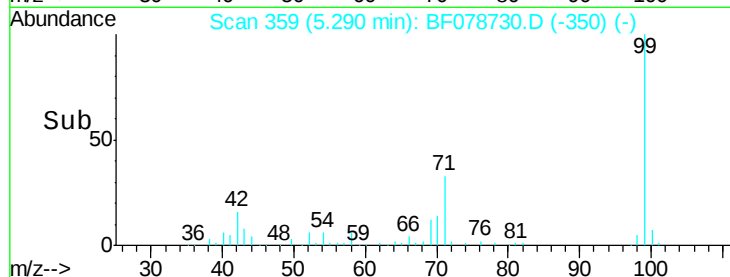

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.94 min Scan# 591

Delta R.T. -0.01 min

Lab File: BF078730.D

Acq: 22 Apr 2015 22:40

Tgt Ion: 136 Resp: 99625


Ion Ratio Lower Upper

136 100

137 10.8 9.0 13.4

54 8.2 7.0 10.6

68 6.0 5.4 8.2


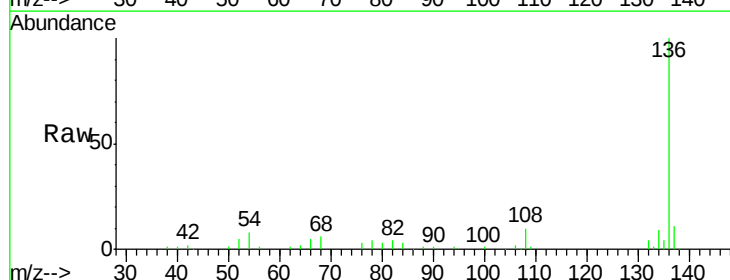


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

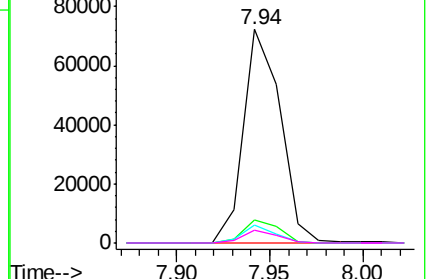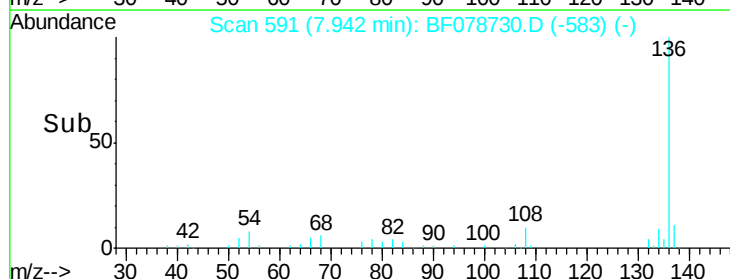







#23
Nitrobenzene-d5
Concen: 79.52 ng
RT: 6.72 min Scan# 484
Delta R.T. -0.01 min
Lab File: BF078730.D
Acq: 22 Apr 2015 22:40

Instrument :
BNA_F
ClientSampleId :
PB82930BL

Tgt Ion	Ratio	Lower	Upper
82	100		
128	41.0	31.8	47.8
54	52.8	41.5	62.3

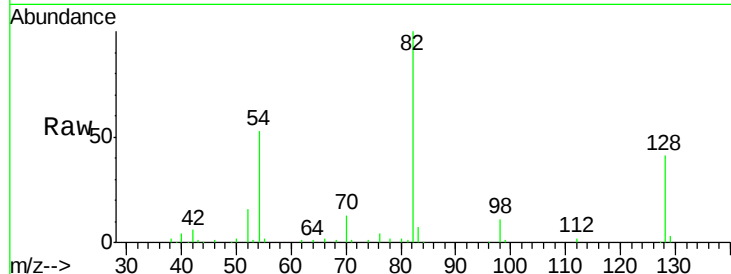


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

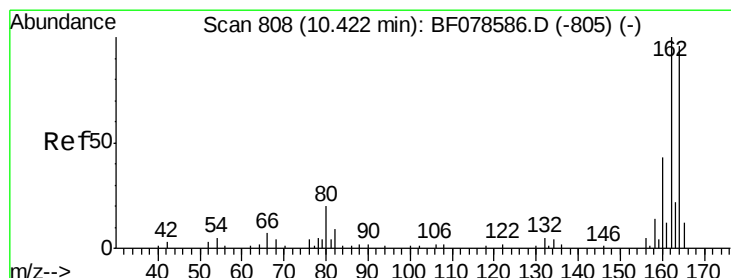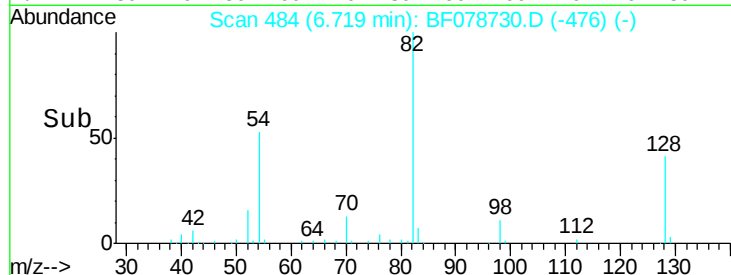
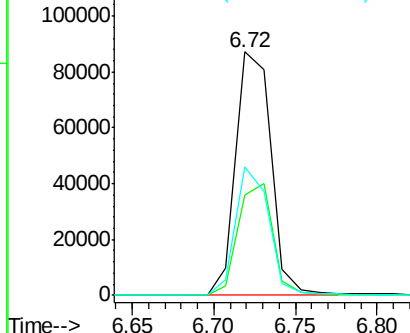


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 11.13 min Scan# 870
Delta R.T. 0.00 min
Lab File: BF078730.D
Acq: 22 Apr 2015 22:40

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.8	82.2	123.2
160	45.5	34.7	52.1

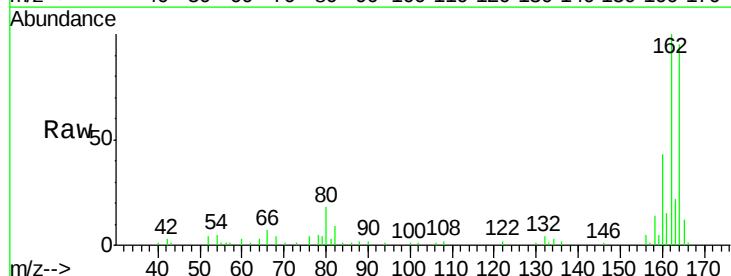

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

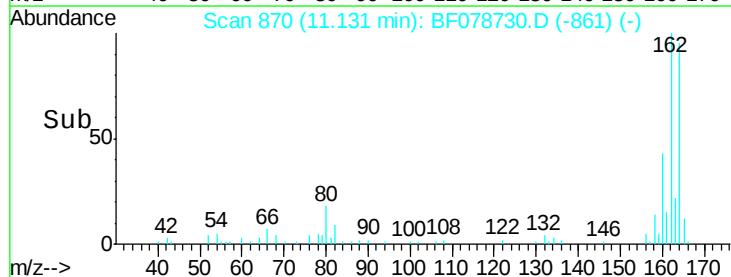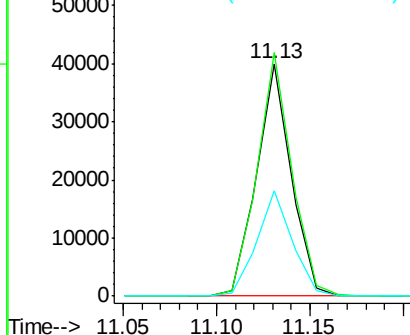







#41
 2,4,6-Tribromophenol
 Concen: 137.09 ng
 RT: 12.61 min Scan# 999
 Delta R.T. 0.00 min
 Lab File: BF078730.D
 Acq: 22 Apr 2015 22:40

Instrument :
 BNA_F
 ClientSampleId :
 PB82930BL

Tgt Ion:330 Resp: 57992
 Ion Ratio Lower Upper
 330 100
 332 96.2 78.6 117.8
 141 38.9 31.2 46.8

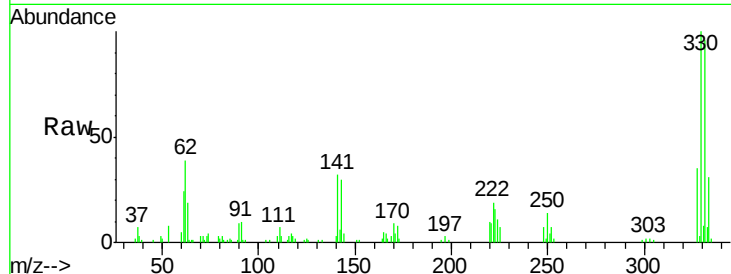


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

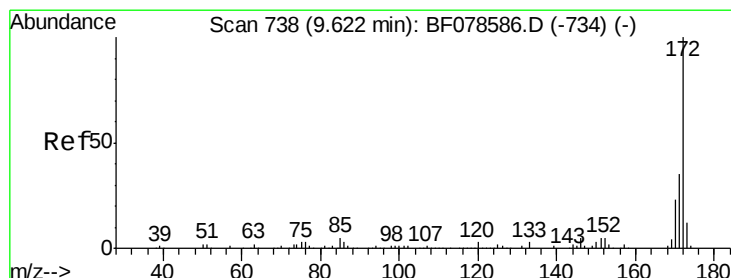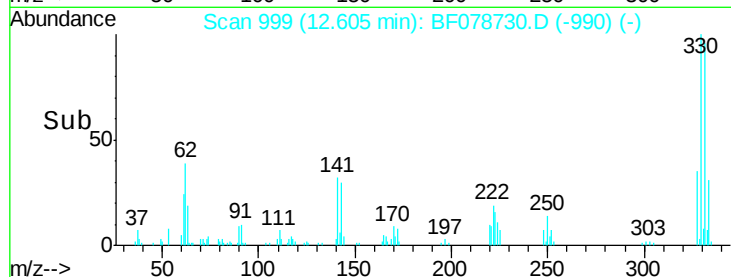
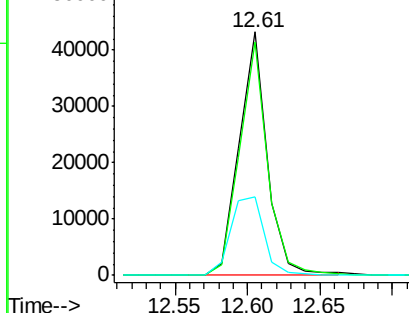


#44
 2-Fluorobiphenyl
 Concen: 80.40 ng
 RT: 9.96 min Scan# 768
 Delta R.T. 0.00 min
 Lab File: BF078730.D
 Acq: 22 Apr 2015 22:40

Tgt Ion:172 Resp: 286886
 Ion Ratio Lower Upper
 172 100
 171 34.8 28.6 42.8
 170 23.1 18.5 27.7

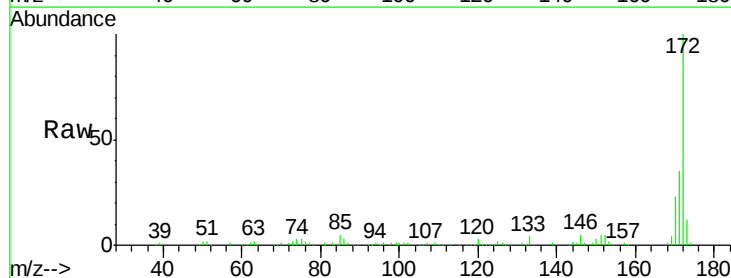

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



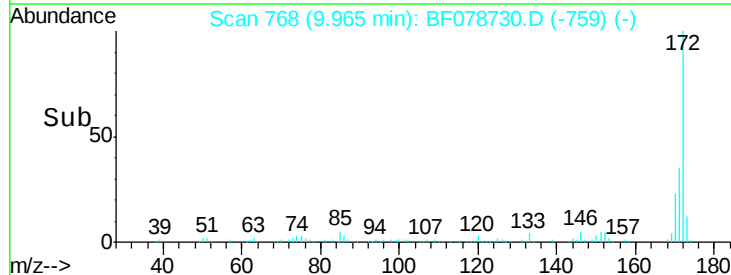
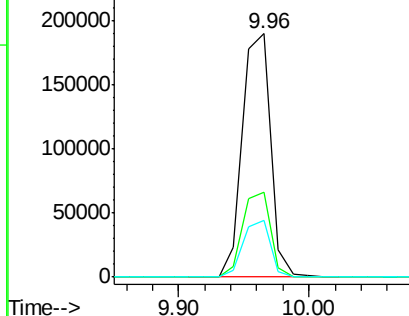




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 13.86 min Scan# 1109
 Delta R.T. 0.00 min
 Lab File: BF078730.D
 Acq: 22 Apr 2015 22:40




Instrument :
 BNA_F
 ClientSampleId :
 PB82930BL


Tgt Ion:188 Resp: 105062
 Ion Ratio Lower Upper
 188 100
 94 8.9 9.0 13.4#
 80 9.8 9.5 14.3

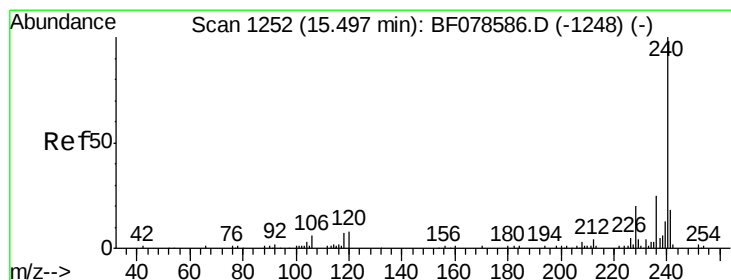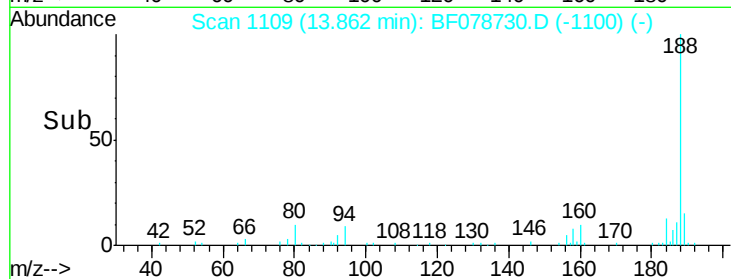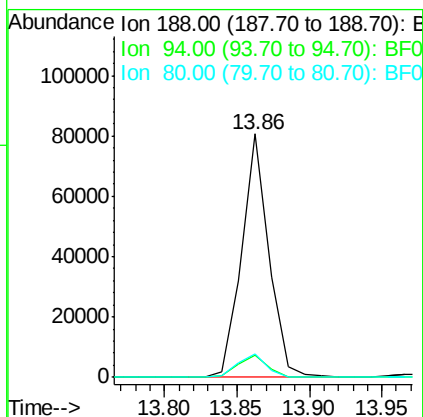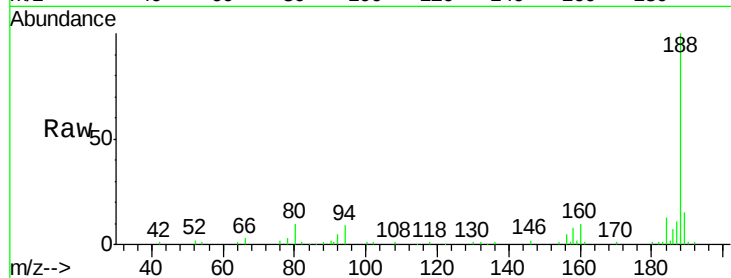

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 17.74 min Scan# 1448
 Delta R.T. 0.00 min
 Lab File: BF078730.D
 Acq: 22 Apr 2015 22:40

Tgt Ion:240 Resp: 114754
 Ion Ratio Lower Upper
 240 100
 120 10.0 7.1 10.7
 236 24.8 21.4 32.2


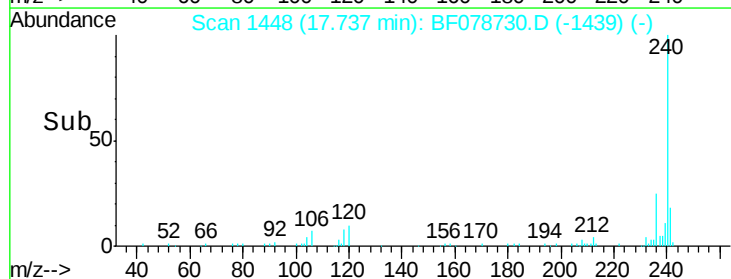
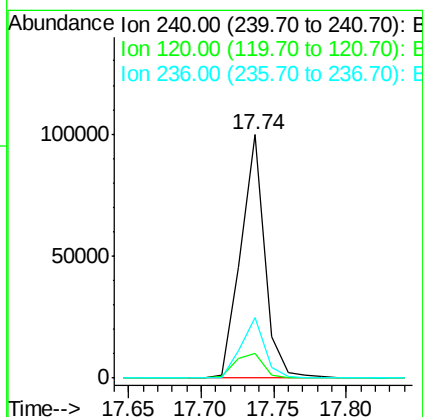
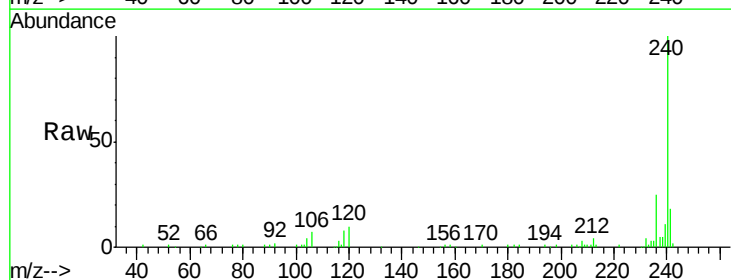


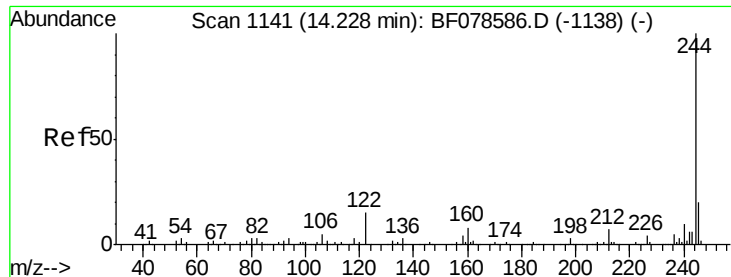

#78
 Terphenyl-d14
 Concen: 72.27 ng
 RT: 16.40 min Scan# 1331
 Delta R.T. 0.00 min
 Lab File: BF078730.D
 Acq: 22 Apr 2015 22:40

Instrument :
 BNA_F
 ClientSampleId :
 PB82930BL

Tgt Ion:244 Resp: 367009
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.0 7.4
 122 12.4 7.1 10.7#

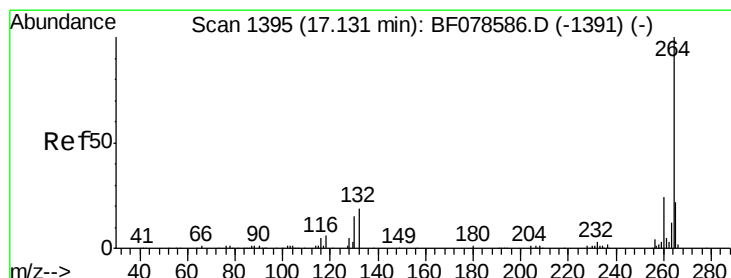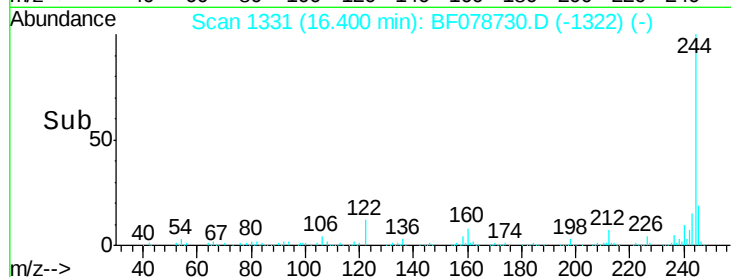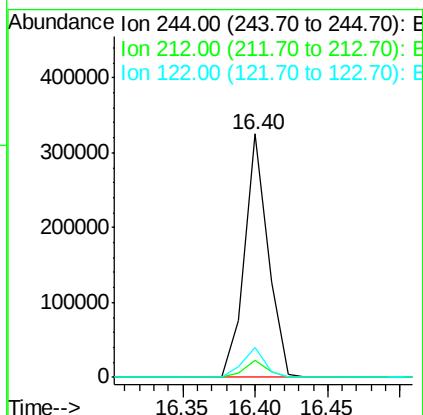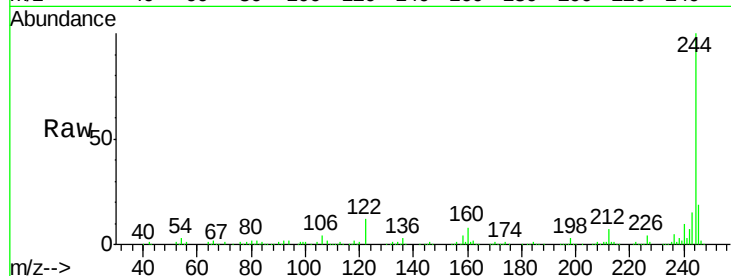

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 19.42 min Scan# 1595
 Delta R.T. -0.01 min
 Lab File: BF078730.D
 Acq: 22 Apr 2015 22:40

Tgt Ion:264 Resp: 114181
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.6 27.8
 265 22.0 17.0 25.6

