
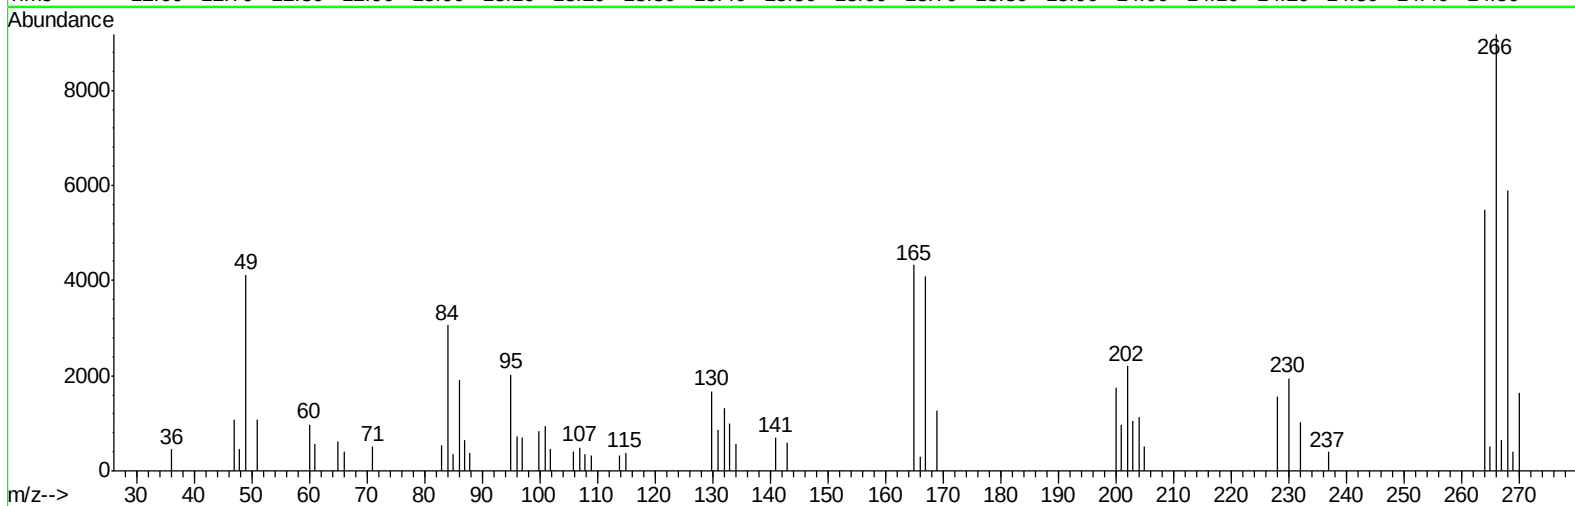


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042215\
Data File : BF078718.D
Acq On : 22 Apr 2015 15:12
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 07:19:58 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 00:55:17 2015
Response via : Initial Calibration

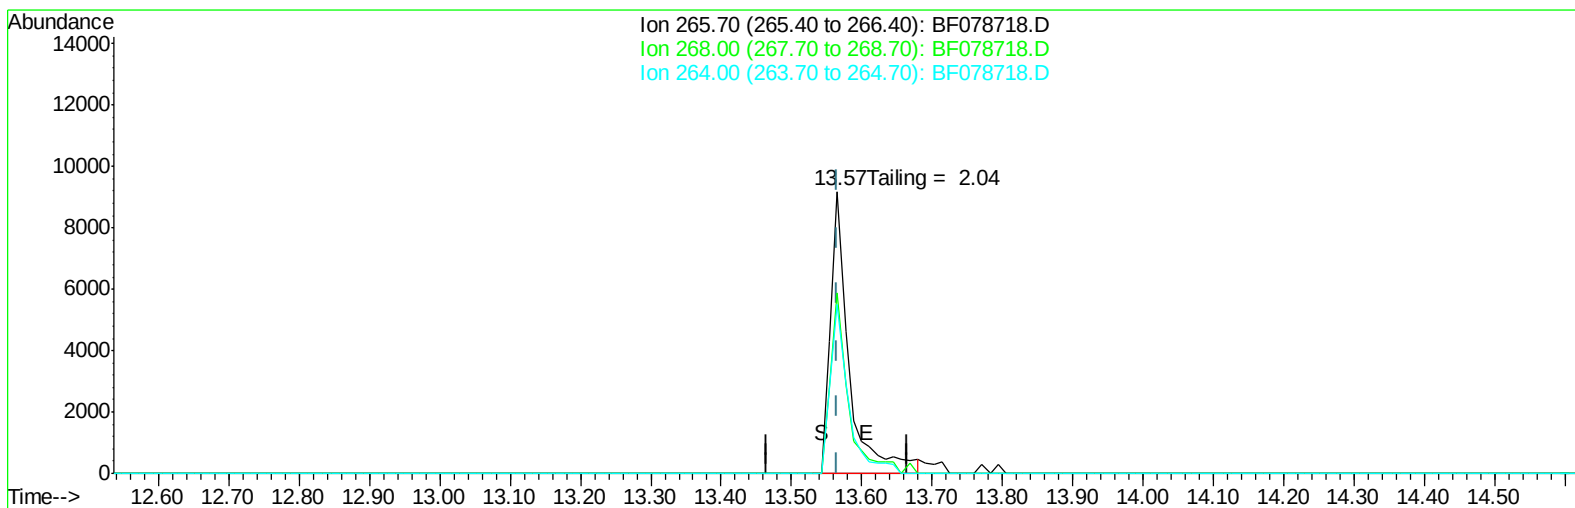

TIC: BF078718.D

(69) Pentachlorophenol (C)



13.565min (+0.000) 0.00ng

response 15293

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	64.33
264.00	62.50	59.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042215\
Data File : BF078718.D
Acq On : 22 Apr 2015 15:12
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 07:19:58 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 00:55:17 2015
Response via : Initial Calibration

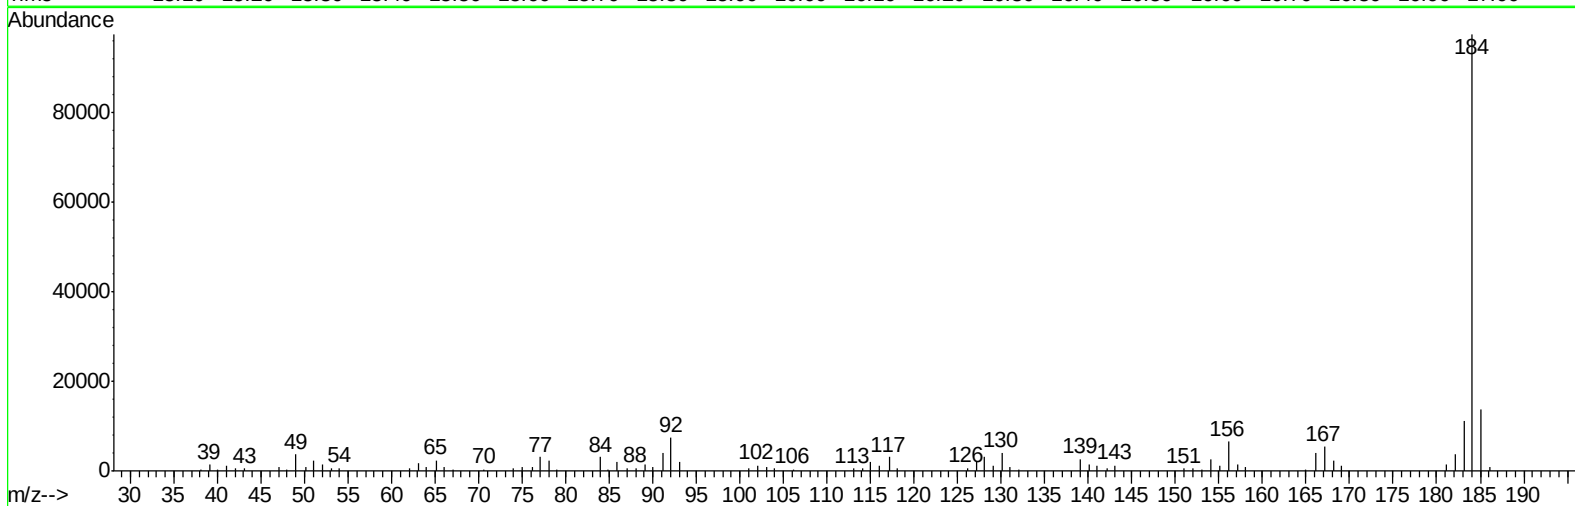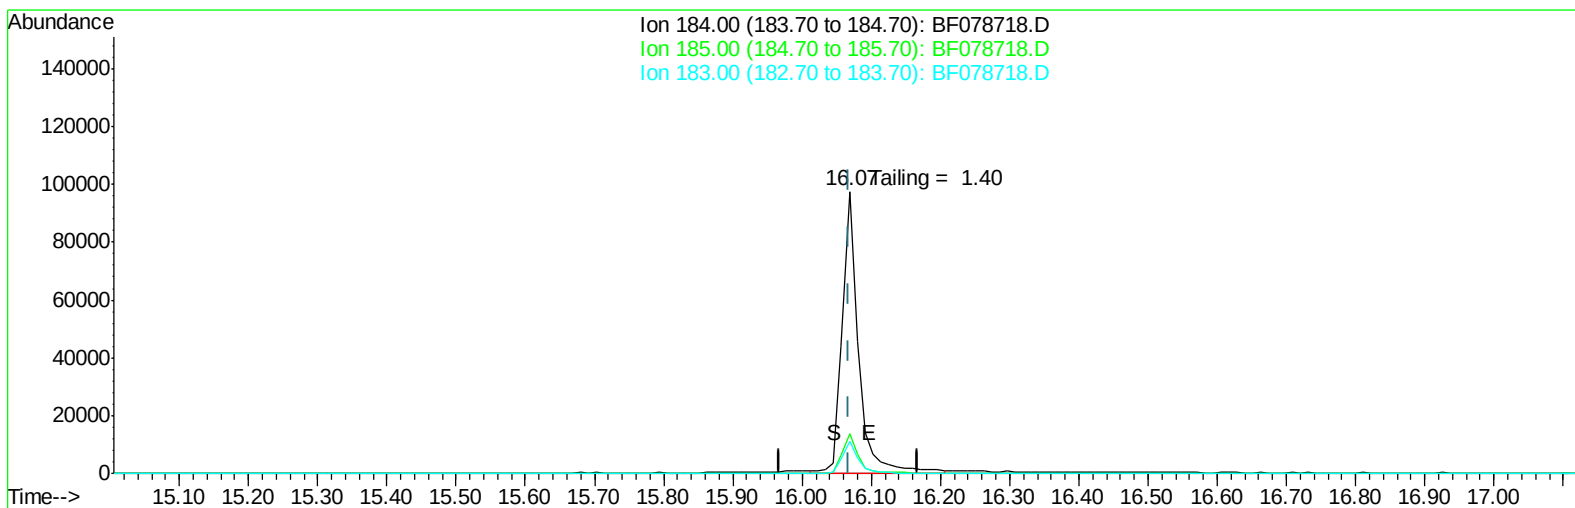

TIC: BF078718.D

(76) Benzidine

16.068min (+0.000) 17895.52ng

response 146773

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.18
183.00	11.90	11.36
0.00	0.00	0.00