


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042215\
 Data File : BF078718.D
 Acq On : 22 Apr 2015 15:12
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

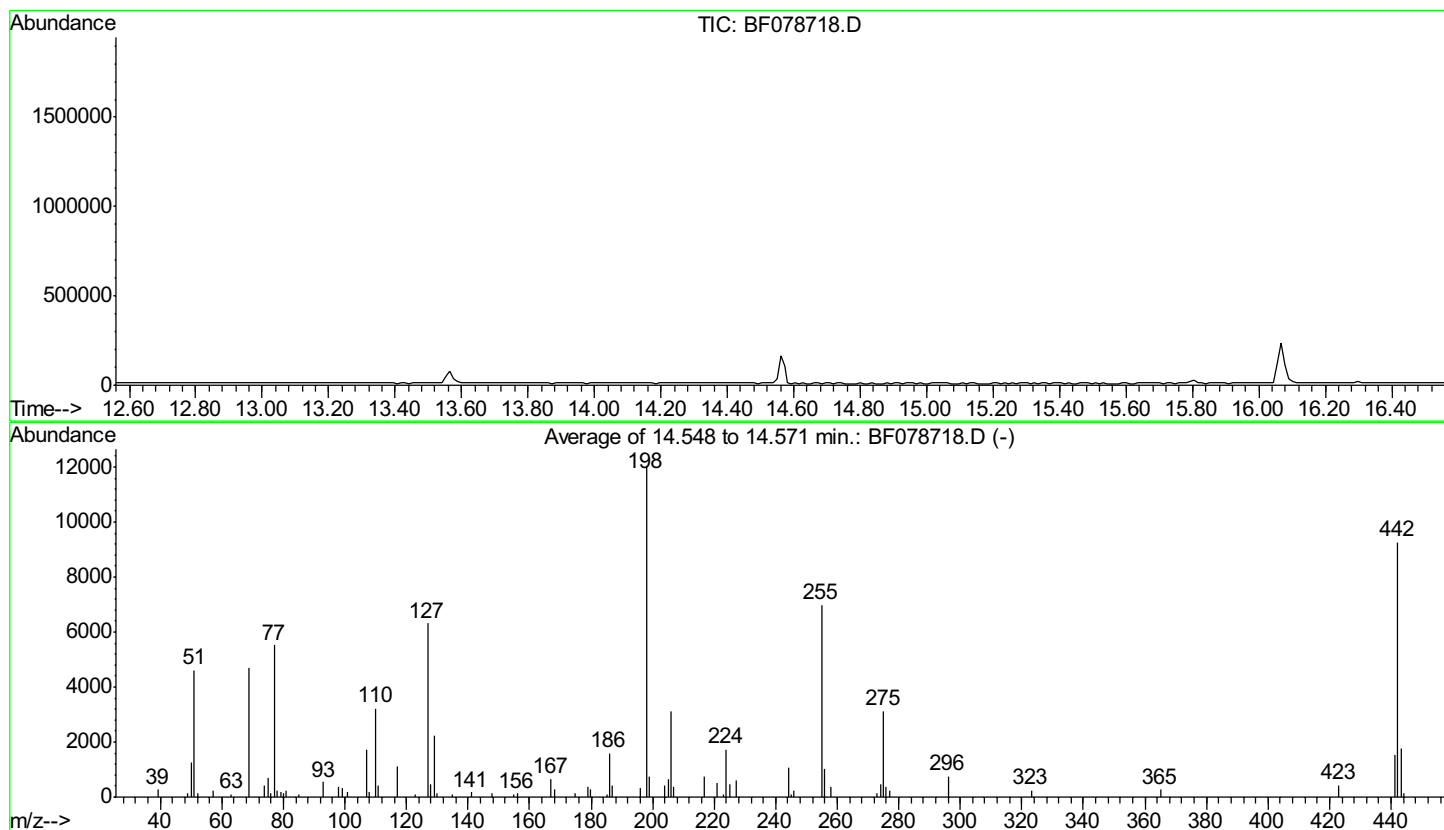

AutoFind: Scans 1169, 1170, 1171; Background Corrected with Scan 1166

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	38.4	4623	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.9	4680	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	6308	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12046	PASS
199	198	5	9	6.3	760	PASS
275	198	10	60	26.0	3130	PASS
365	198	1	100	2.3	275	PASS
441	442	0.01	24	16.3	1513	PASS
442	198	50	100	77.0	9274	PASS
443	442	15	24	18.9	1750	PASS