


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042215\
 Data File : BF078736.D
 Acq On : 23 Apr 2015 3:21
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:58:34 2015

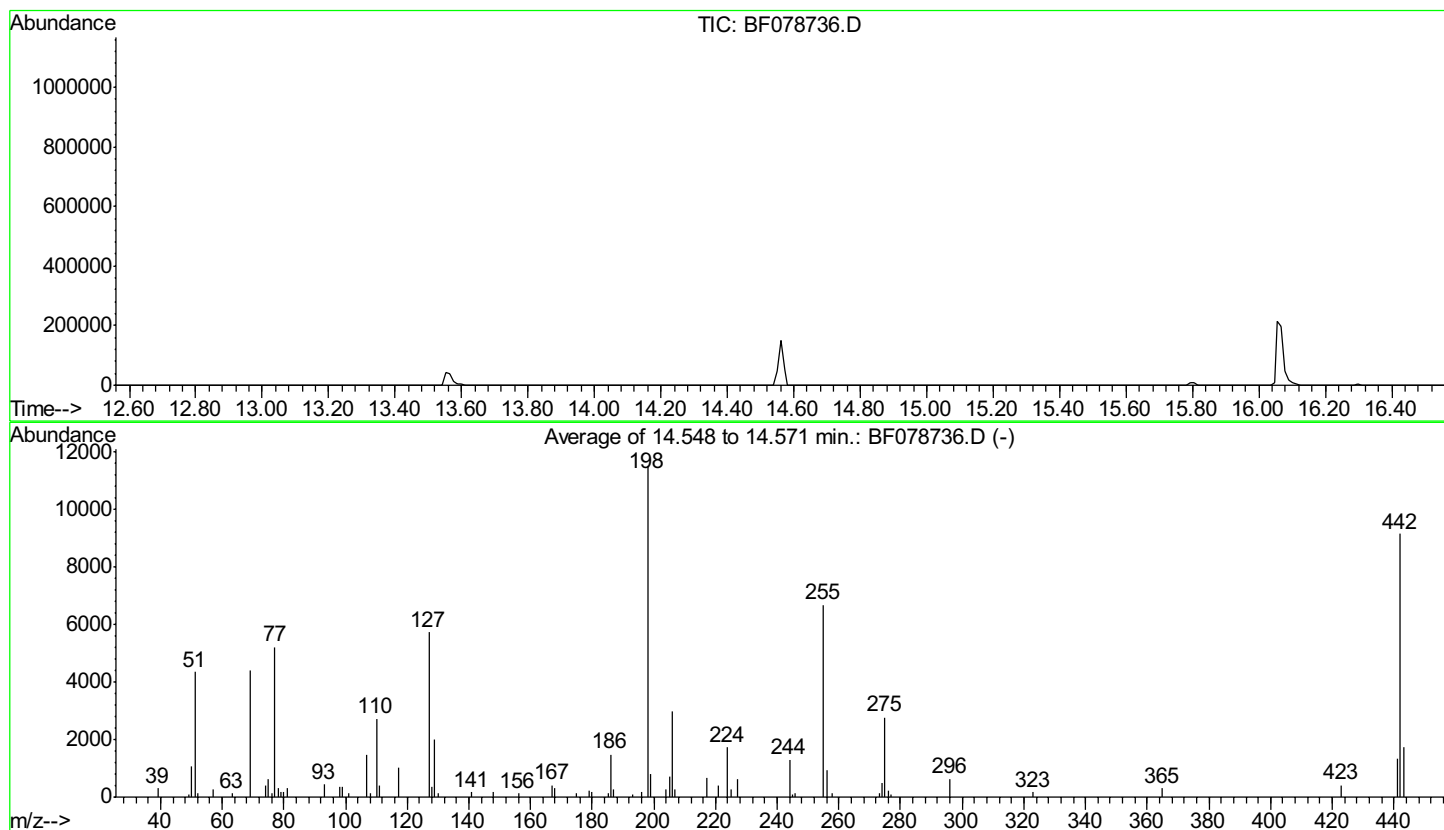

AutoFind: Scans 1169, 1170, 1171; Background Corrected with Scan 1166

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	37.7	4333	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	4381	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	5711	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11494	PASS
199	198	5	9	7.0	799	PASS
275	198	10	60	24.1	2774	PASS
365	198	1	100	2.5	292	PASS
441	442	0.01	24	14.4	1316	PASS
442	198	50	100	79.5	9140	PASS
443	442	15	24	18.7	1712	PASS