
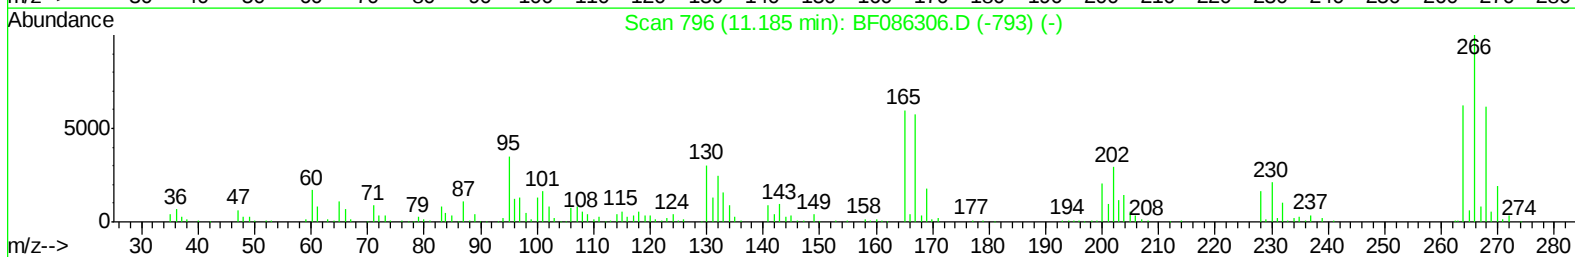
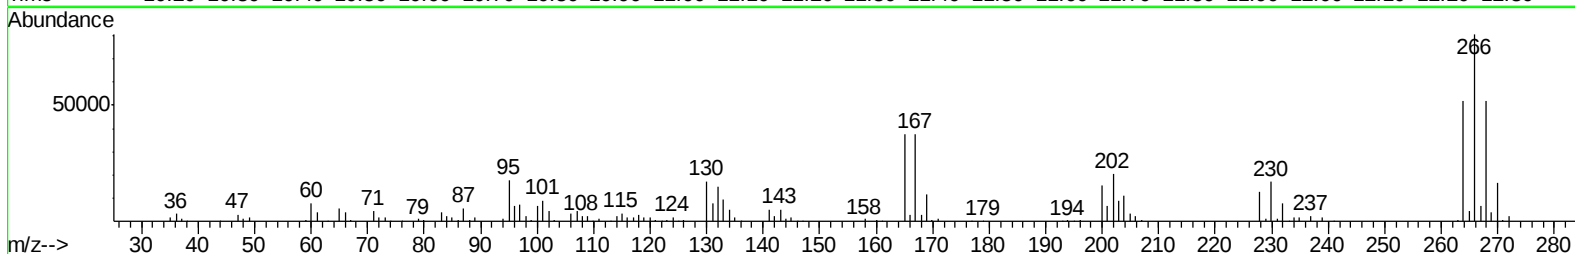


Data Path : Z:\HPCHEM1\BNA_F\Data\BF042216\
Data File : BF086361.D
Acq On : 23 Apr 2016 00:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 07:44:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 23 00:24:02 2016
Response via : Initial Calibration

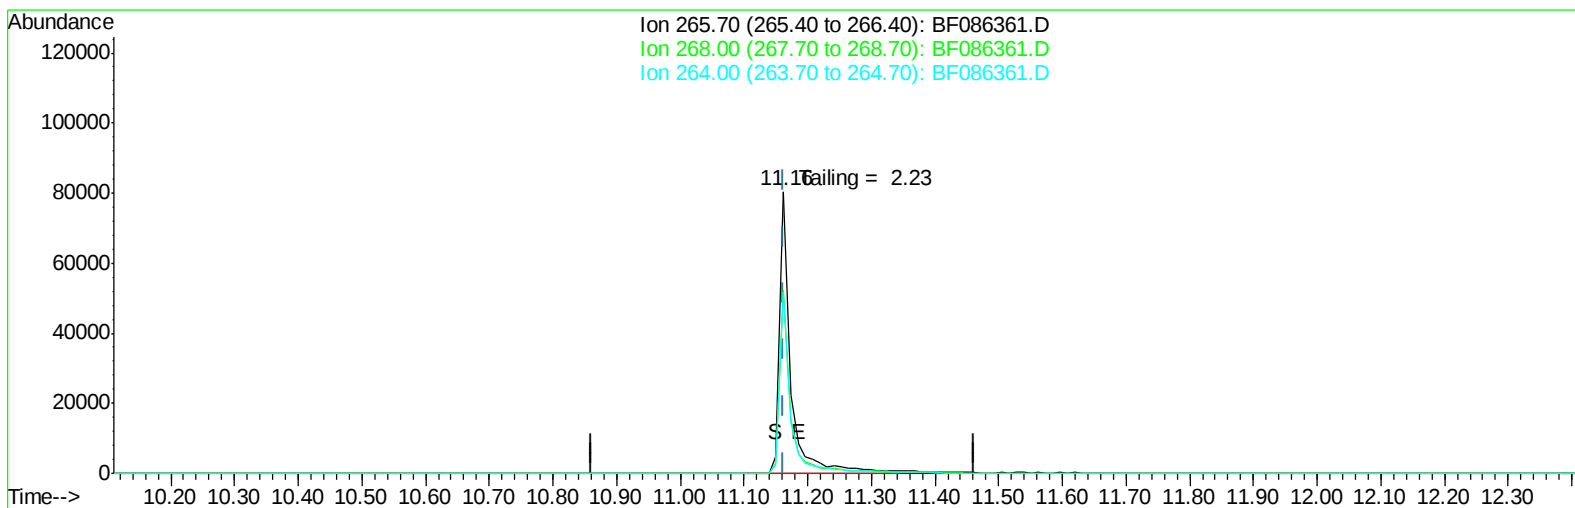

TIC: BF086361.D

(69) Pentachlorophenol (C)




11.162min (-0.000) 0.00ng

response 99380

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.85
264.00	66.10	64.74
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF042216\
Data File : BF086361.D
Acq On : 23 Apr 2016 00:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 07:44:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 23 00:24:02 2016
Response via : Initial Calibration

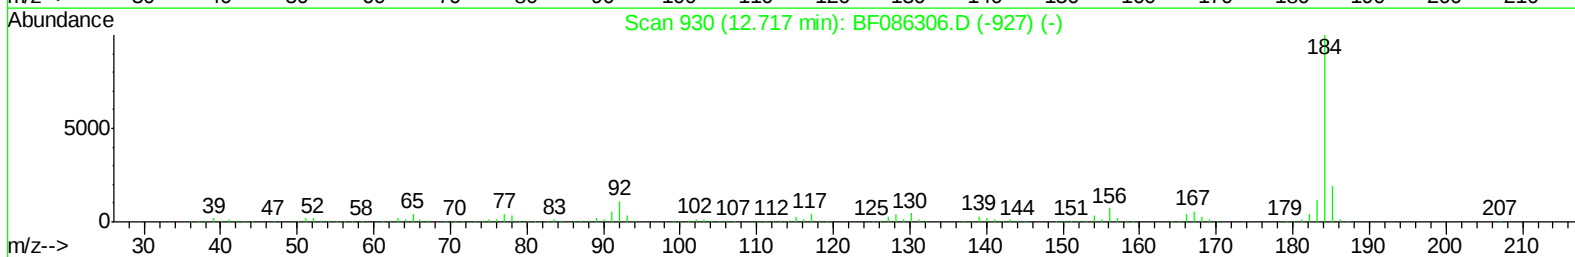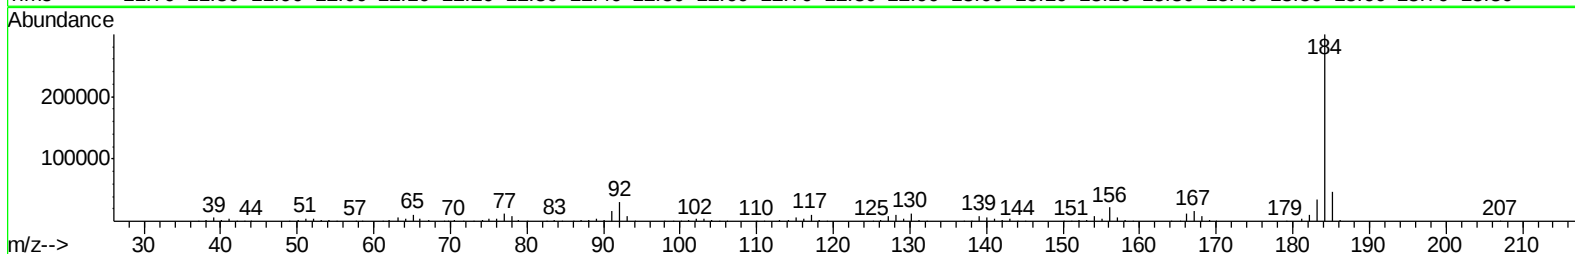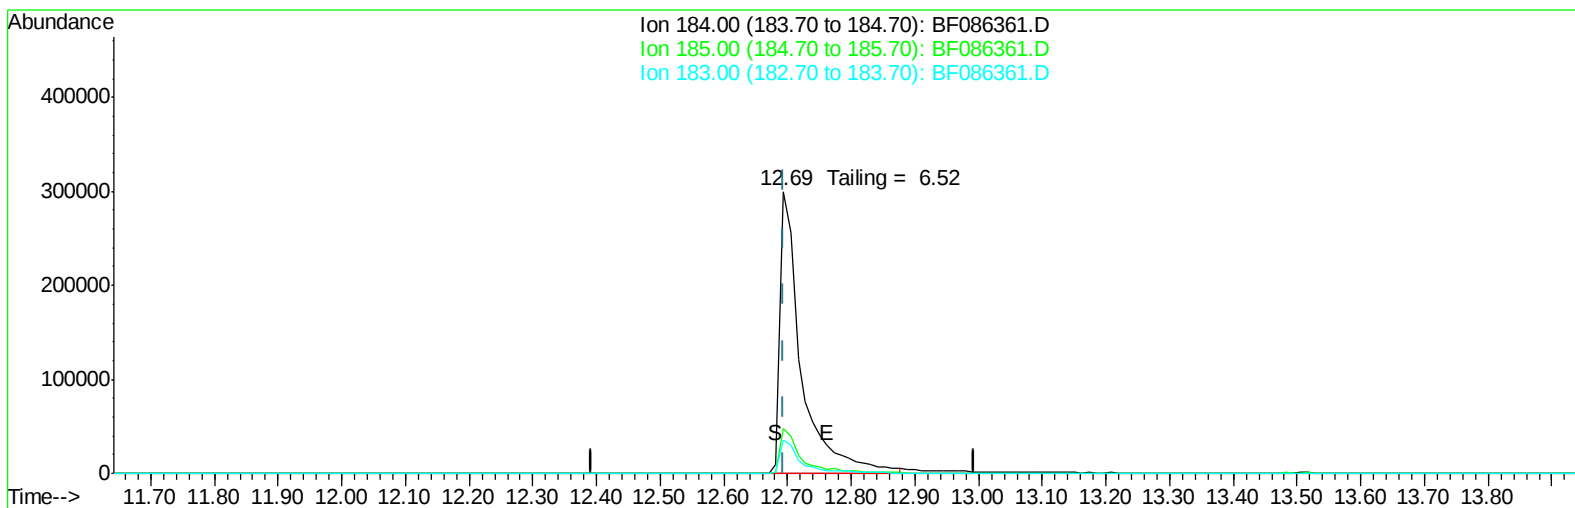

TIC: BF086361.D

(76) Benzidine

12.694min (-0.000) 0.00ng

response 699387

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	16.13
183.00	12.20	11.74
0.00	0.00	0.00