

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042216\
 Data File : BF086367.D
 Acq On : 23 Apr 2016 3:23
 Operator : UM/SJ
 Sample : PB89989BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB89989BL

Quant Time: Apr 25 08:03:44 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 23 00:24:02 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	169950	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	715953	20.00	ng	-0.01
38) Acenaphthene-d10	9.87	164	331965	20.00	ng	-0.01
63) Phenanthrene-d10	11.36	188	693368	20.00	ng	-0.01
75) Chrysene-d12	13.99	240	608190	20.00	ng	-0.01
86) Perylene-d12	15.40	264	530256	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	1072854	109.02	ng	0.01
7) Phenol-d6	6.46	99	1492476	111.56	ng	-0.01
23) Nitrobenzene-d5	7.40	82	908956	75.21	ng	-0.01
41) 2,4,6-Tribromophenol	10.66	330	350857	116.76	ng	-0.01
44) 2-Fluorobiphenyl	9.21	172	1649747	84.81	ng	0.00
78) Terphenyl-d14	12.95	244	1578334	64.48	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042216\
Data File : BF086367.D
Acq On : 23 Apr 2016 3:23
Operator : UM/SJ
Sample : PB89989BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89989BL

Quant Time: Apr 25 08:03:44 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 23 00:24:02 2016
Response via : Initial Calibration

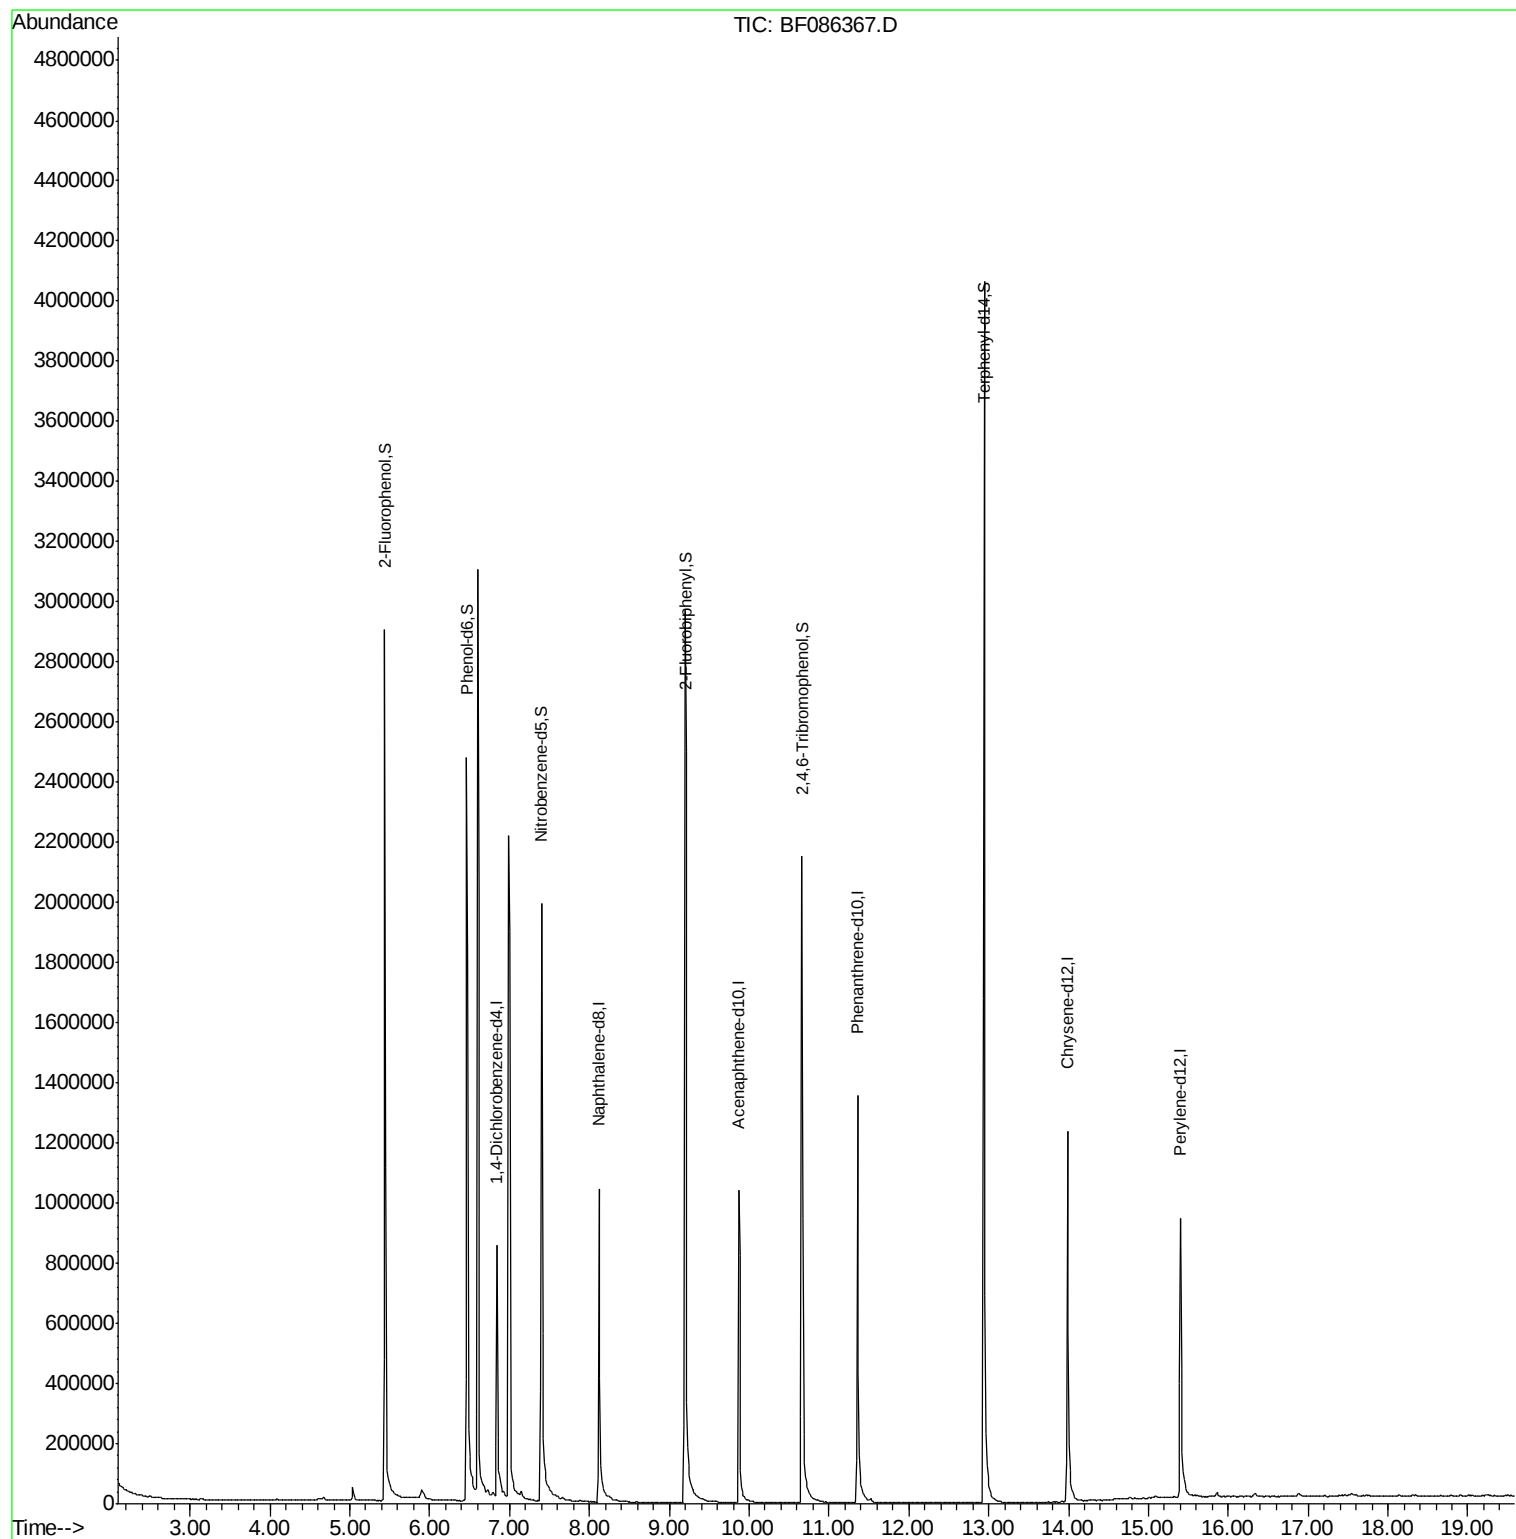

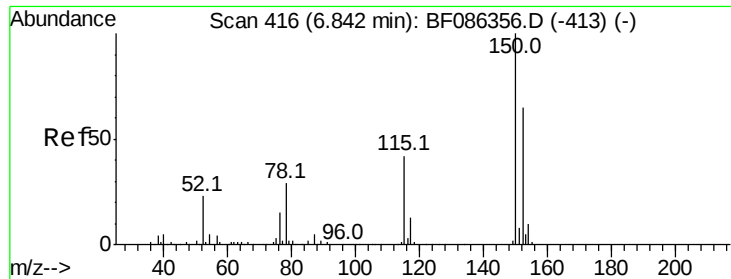

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.84 min Scan# 416

Delta R.T. -0.00 min

Lab File: BF086367.D

Acq: 23 Apr 2016 3:23

Instrument :

BNA_F

ClientSampleId :

PB89989BL


Tot Ion:152 Resp: 169950

Ion Ratio Lower Upper

152 100

150 154.0 125.8 188.6




115 58.5 51.5 77.3

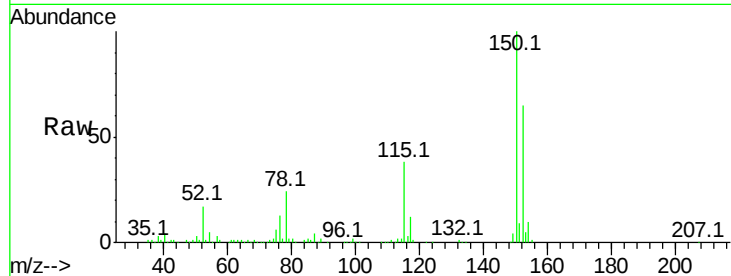

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

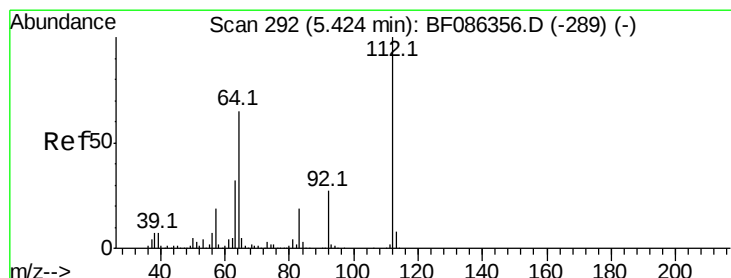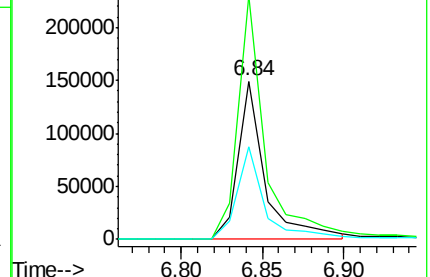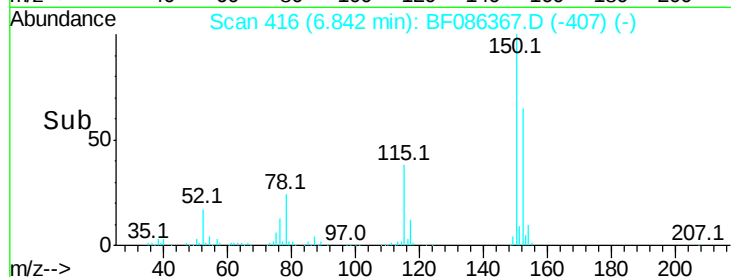

#5

2-Fluorophenol

Concen: 109.02 ng

RT: 5.44 min Scan# 293

Delta R.T. 0.01 min

Lab File: BF086367.D

Acq: 23 Apr 2016 3:23


Tgt Ion:112 Resp: 1072854

Ion Ratio Lower Upper

112 100

64 61.5 52.1 78.1



63 32.3 25.7 38.5

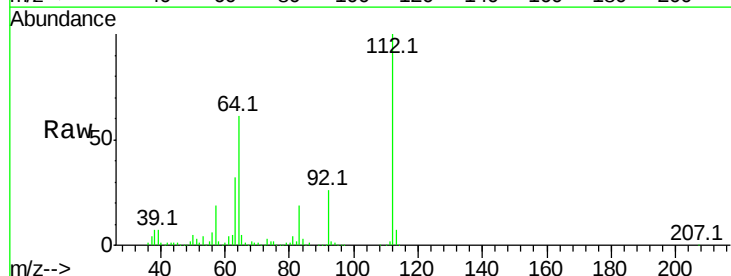


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

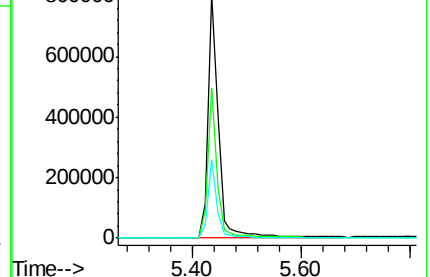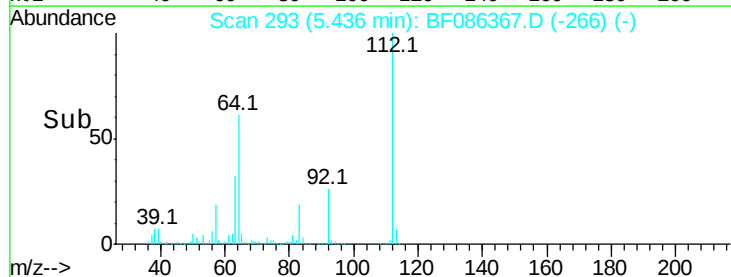

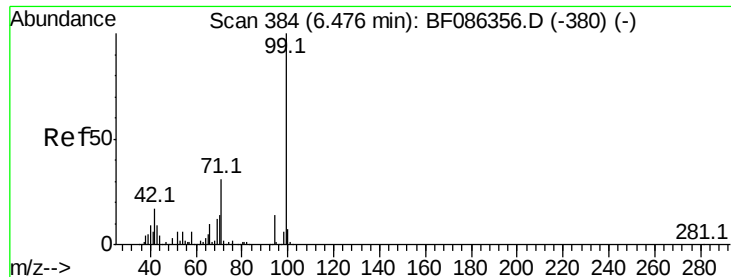

#7

Phenol-d6

Concen: 111.56 ng

RT: 6.46 min Scan# 383

Delta R.T. -0.01 min

Lab File: BF086367.D

Acq: 23 Apr 2016 3:23

Instrument :





BNA_F

ClientSampleId :

PB89989BL

Tot Ion: 99 Resp: 1492476

Ion	Ratio	Lower	Upper
99	100		
42	20.6	13.6	20.4#
71	33.6	24.6	36.8

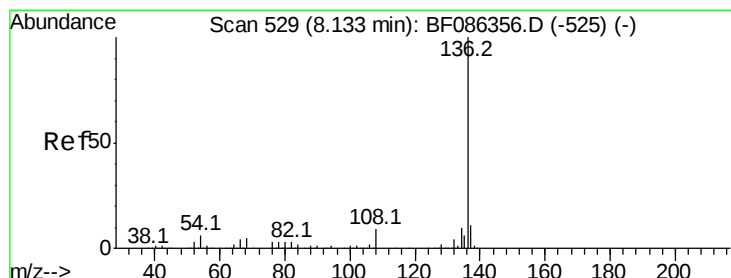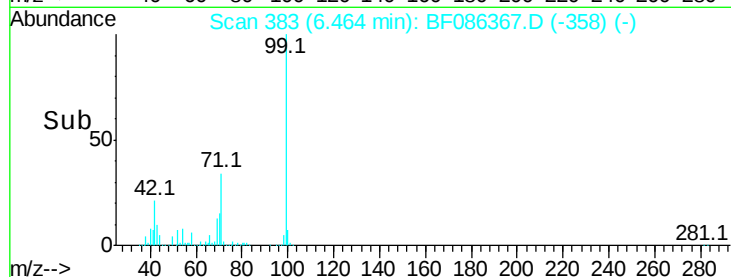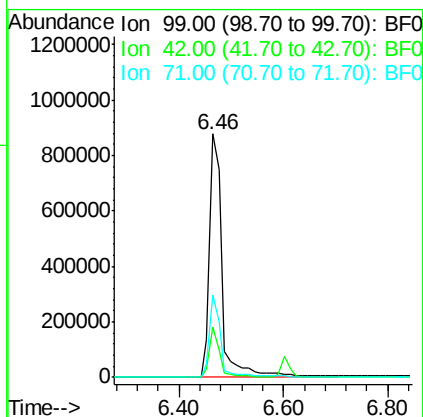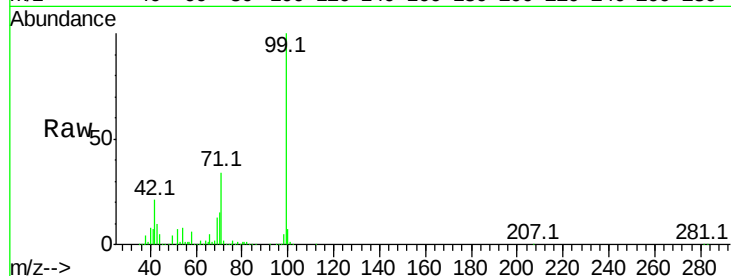

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.12 min Scan# 528




Delta R.T. -0.01 min


Lab File: BF086367.D

Acq: 23 Apr 2016 3:23

Tgt Ion: 136 Resp: 715953

Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.8	13.2
54	8.5	5.0	7.4#
68	7.1	4.4	6.6#


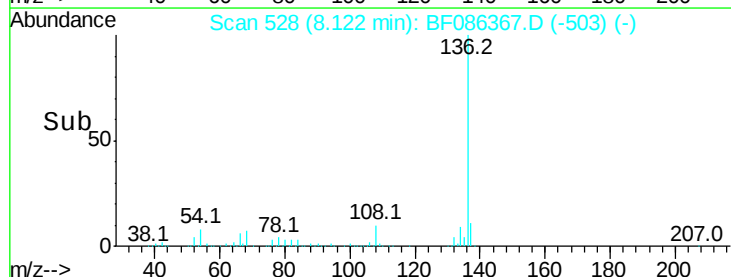
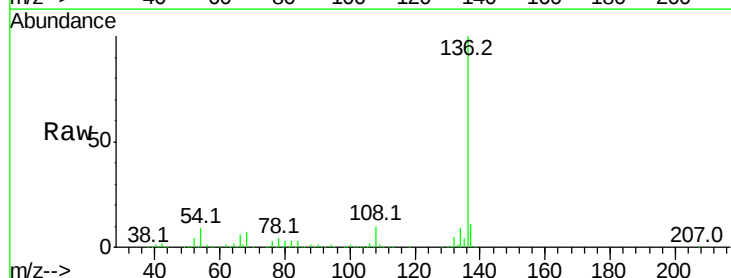
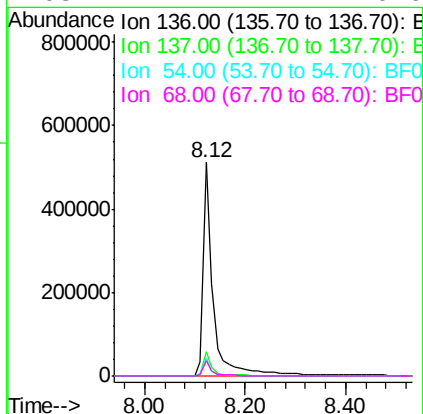


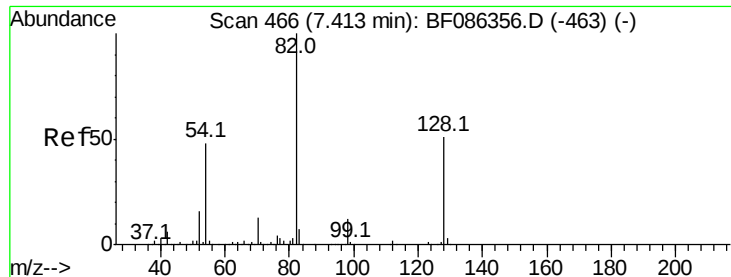

#23
 Nitrobenzene-d5
 Concen: 75.21 ng
 RT: 7.40 min Scan# 465
 Delta R.T. -0.01 min
 Lab File: BF086367.D
 Acq: 23 Apr 2016 3:23




Instrument :
 BNA_F
 ClientSampleID :
 PB89989BL


Tot Ion	82	Resp	908956
Ion Ratio	Lower	Upper	
82	100		
128	43.7	40.6	61.0
54	50.7	38.1	57.1

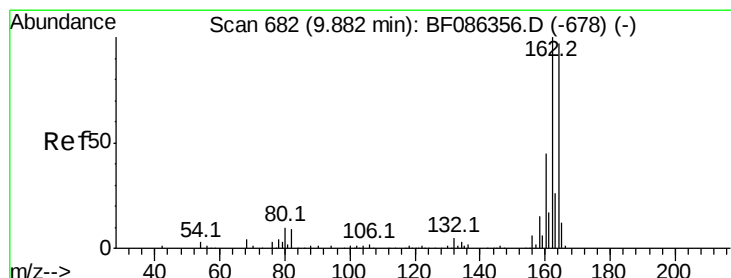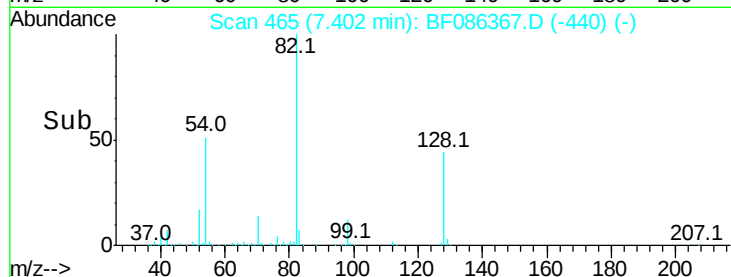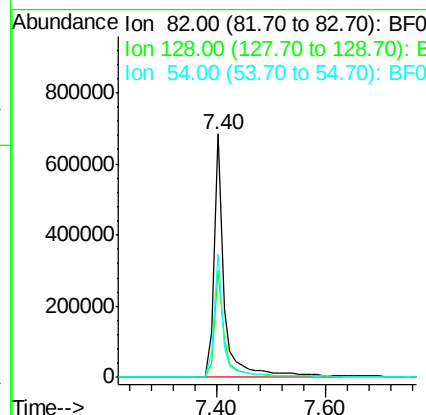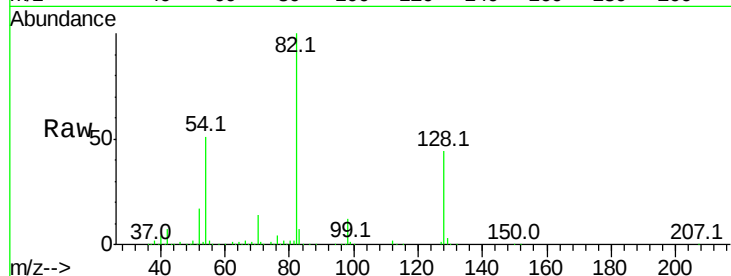

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.87 min Scan# 681
 Delta R.T. -0.01 min
 Lab File: BF086367.D
 Acq: 23 Apr 2016 3:23

Tgt Ion	164	Resp	331965
Ion Ratio	Lower	Upper	
164	100		
162	102.1	82.8	124.2
160	46.3	36.9	55.3

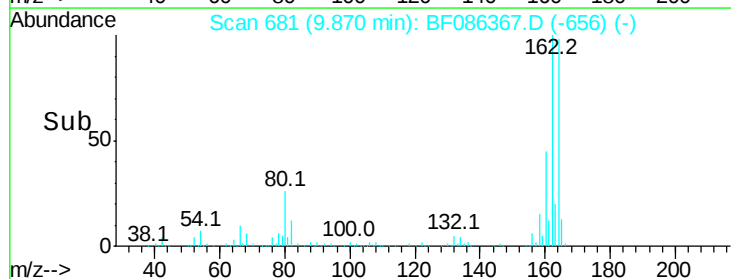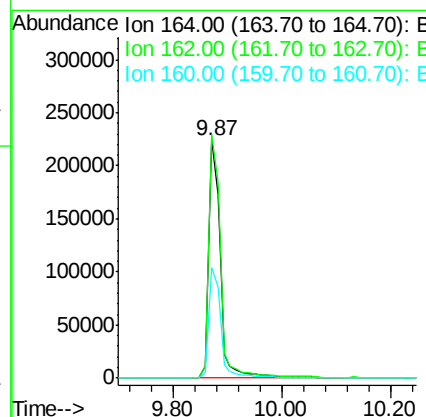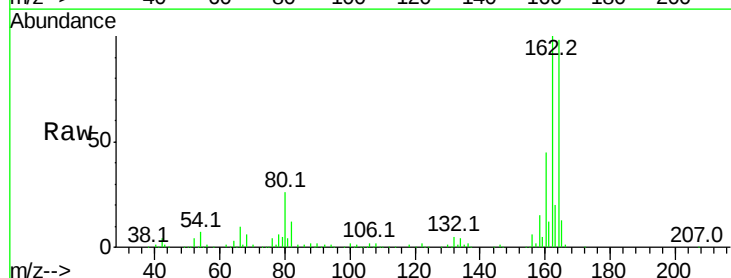


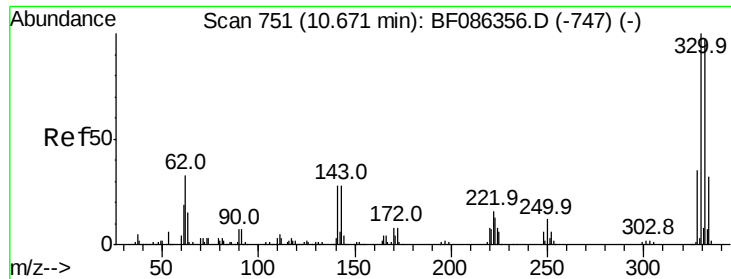




#41
 2,4,6-Tribromophenol
 Concen: 116.76 ng
 RT: 10.66 min Scan# 750
 Delta R.T. -0.01 min
 Lab File: BF086367.D
 Acq: 23 Apr 2016 3:23

Instrument :
 BNA_F
 ClientSampleId :
 PB89989BL

Tot Ion:330 Resp: 350857
 Ion Ratio Lower Upper
 330 100
 332 94.9 79.0 118.4
 141 39.0 31.2 46.8

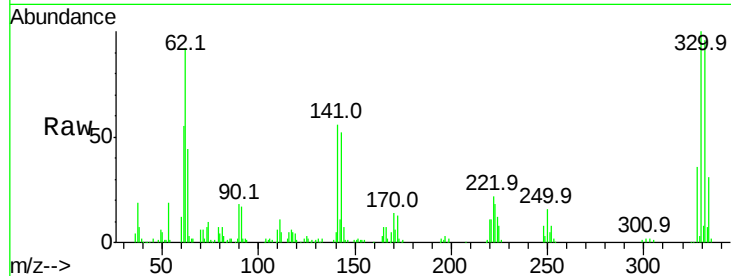


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

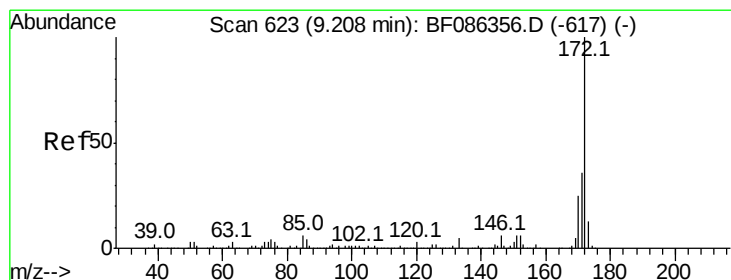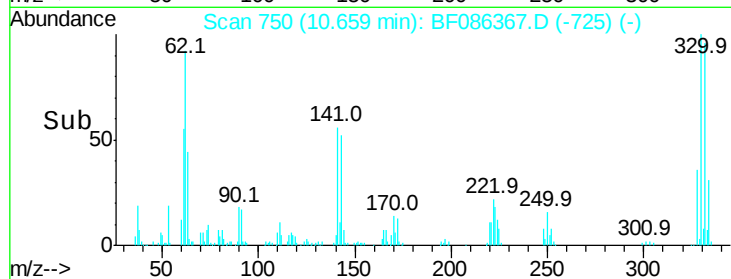
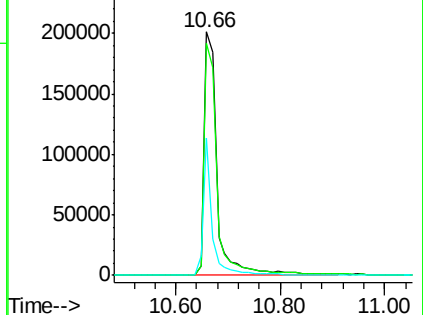



#44
 2-Fluorobiphenyl
 Concen: 84.81 ng
 RT: 9.21 min Scan# 623
 Delta R.T. -0.00 min
 Lab File: BF086367.D
 Acq: 23 Apr 2016 3:23

Tgt Ion:172 Resp: 1649747
 Ion Ratio Lower Upper
 172 100
 171 35.1 29.0 43.6
 170 24.1 19.8 29.8

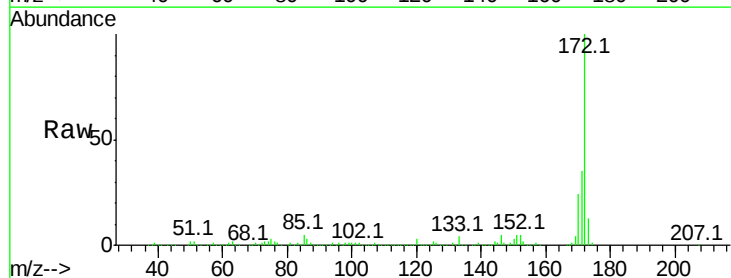

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

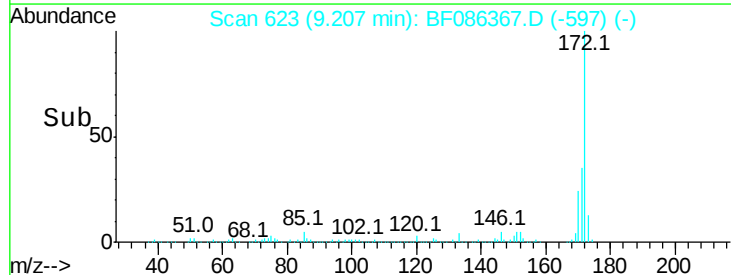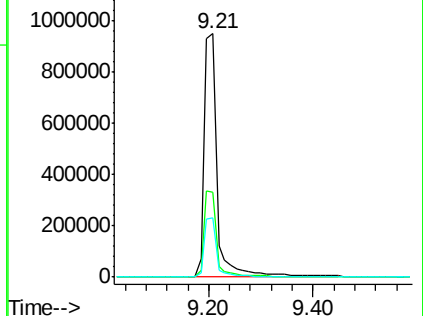

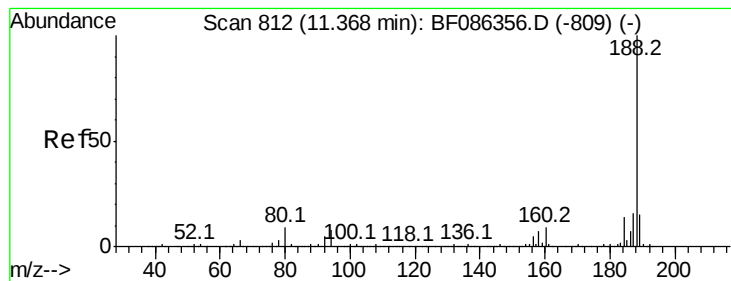

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.36 min Scan# 811

Delta R.T. -0.01 min

Lab File: BF086367.D

Acq: 23 Apr 2016 3:23

Instrument :

BNA_F

ClientSampleId :

PB89989BL


Tot Ion:188 Resp: 693368

Ion Ratio Lower Upper

188 100

94 10.9 6.8 10.2#




80 11.7 7.1 10.7#

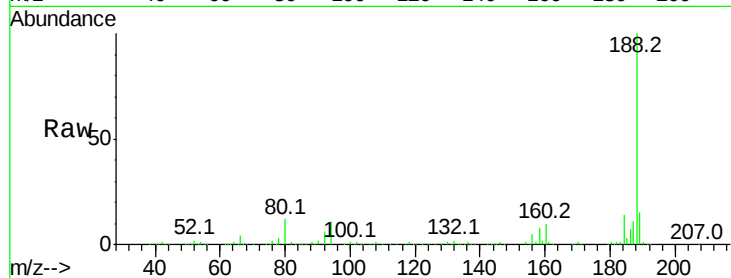

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

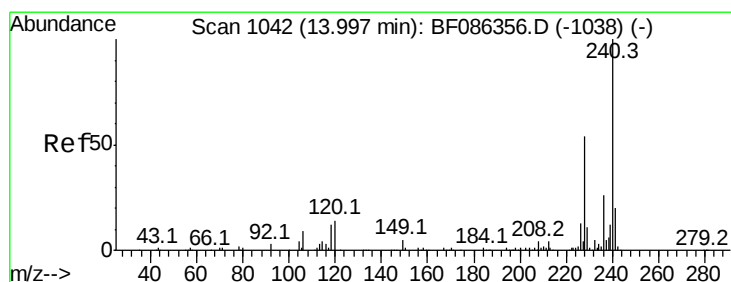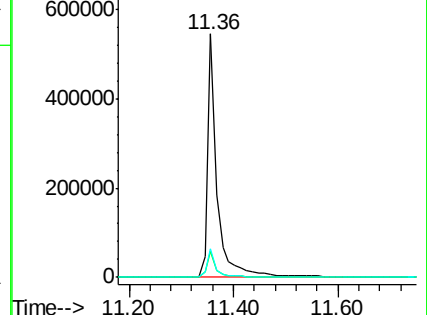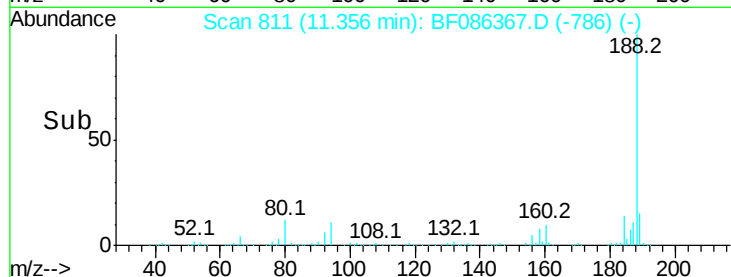

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.99 min Scan# 1041

Delta R.T. -0.01 min

Lab File: BF086367.D

Acq: 23 Apr 2016 3:23


Tgt Ion:240 Resp: 608190

Ion Ratio Lower Upper

240 100

120 15.5 11.2 16.8



236 25.5 21.2 31.8

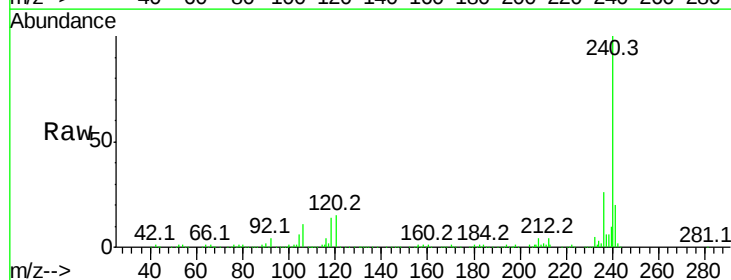


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



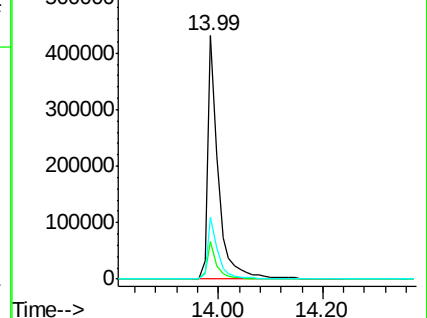
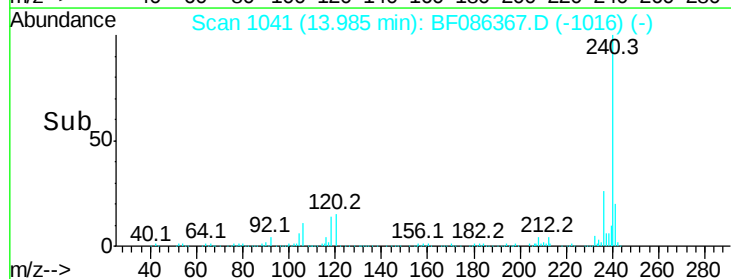


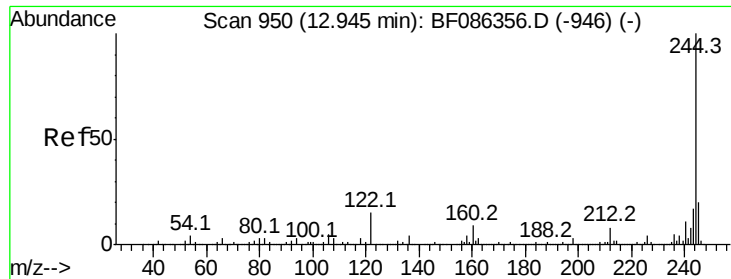

#78
 Terphenyl-d14
 Concen: 64.48 ng
 RT: 12.95 min Scan# 950
 Delta R.T. -0.00 min
 Lab File: BF086367.D
 Acq: 23 Apr 2016 3:23

Instrument :
 BNA_F
 ClientSampleId :
 PB89989BL

Tot Ion:244 Resp: 1578334
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.2 9.2
 122 13.2 12.0 18.0

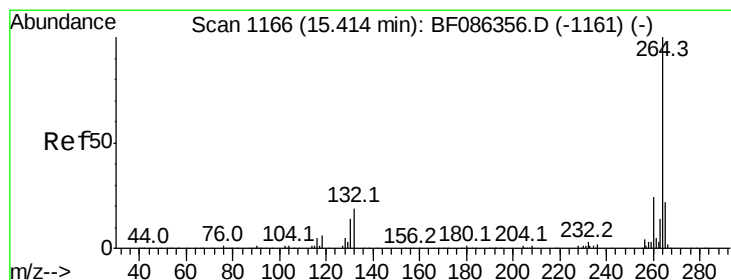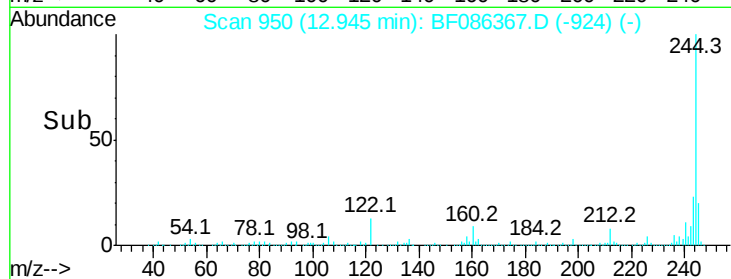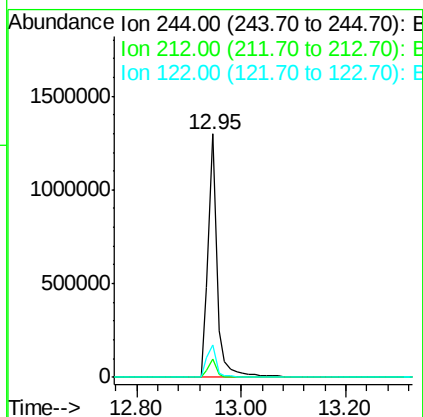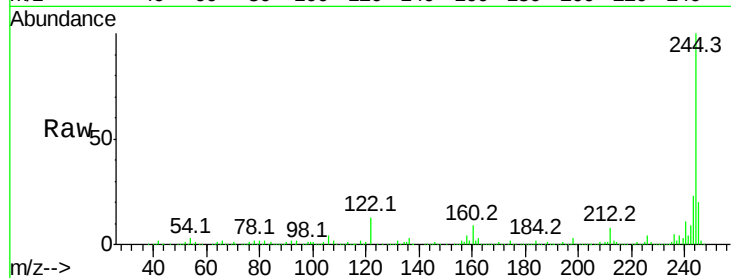

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.40 min Scan# 1165
 Delta R.T. -0.01 min
 Lab File: BF086367.D
 Acq: 23 Apr 2016 3:23

Tgt Ion:264 Resp: 530256
 Ion Ratio Lower Upper
 264 100
 260 24.6 19.5 29.3
 265 21.1 17.3 25.9

