

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
 Data File : BF086367.D
 Acq On : 23 Apr 2016 3:23
 Operator : UM/SJ
 Sample : PB89989BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB89989BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.036	255	258	266	rBV	44046	67961	1.39%	0.184%
2	5.436	290	293	296	rBV	2896001	3252275	66.32%	8.794%
3	5.904	330	334	345	rVB	31073	101314	2.07%	0.274%
4	6.464	380	383	386	rBV	2472274	3471284	70.78%	9.387%
5	6.602	393	395	398	rBV	3053313	3716649	75.78%	10.050%
6	6.842	414	416	422	rBV	832295	972641	19.83%	2.630%
7	6.990	427	429	432	rBV	2197819	3027441	61.73%	8.186%
8	7.150	441	443	451	rVB	29382	62905	1.28%	0.170%
9	7.402	462	465	485	rBV	1985450	2593477	52.88%	7.013%
10	8.122	526	528	547	rBV	1042700	1394084	28.43%	3.770%
11	9.196	620	622	625	rBV	2969912	4284619	87.37%	11.586%
12	9.870	679	681	684	rBV	1037507	1420552	28.97%	3.841%
13	10.659	747	750	770	rBV	2149730	2861358	58.34%	7.737%
14	11.356	809	811	824	rBV	1354099	1664917	33.95%	4.502%
15	12.945	947	950	973	rBV	4061892	4904217	100.00%	13.261%
16	13.985	1039	1041	1055	rBV	1233736	1672979	34.11%	4.524%
17	15.402	1162	1165	1179	rBV	928717	1512590	30.84%	4.090%


Sum of corrected areas: 36981263

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
Data File : BF086367.D
Acq On : 23 Apr 2016 3:23
Operator : UM/SJ
Sample : PB89989BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89989BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

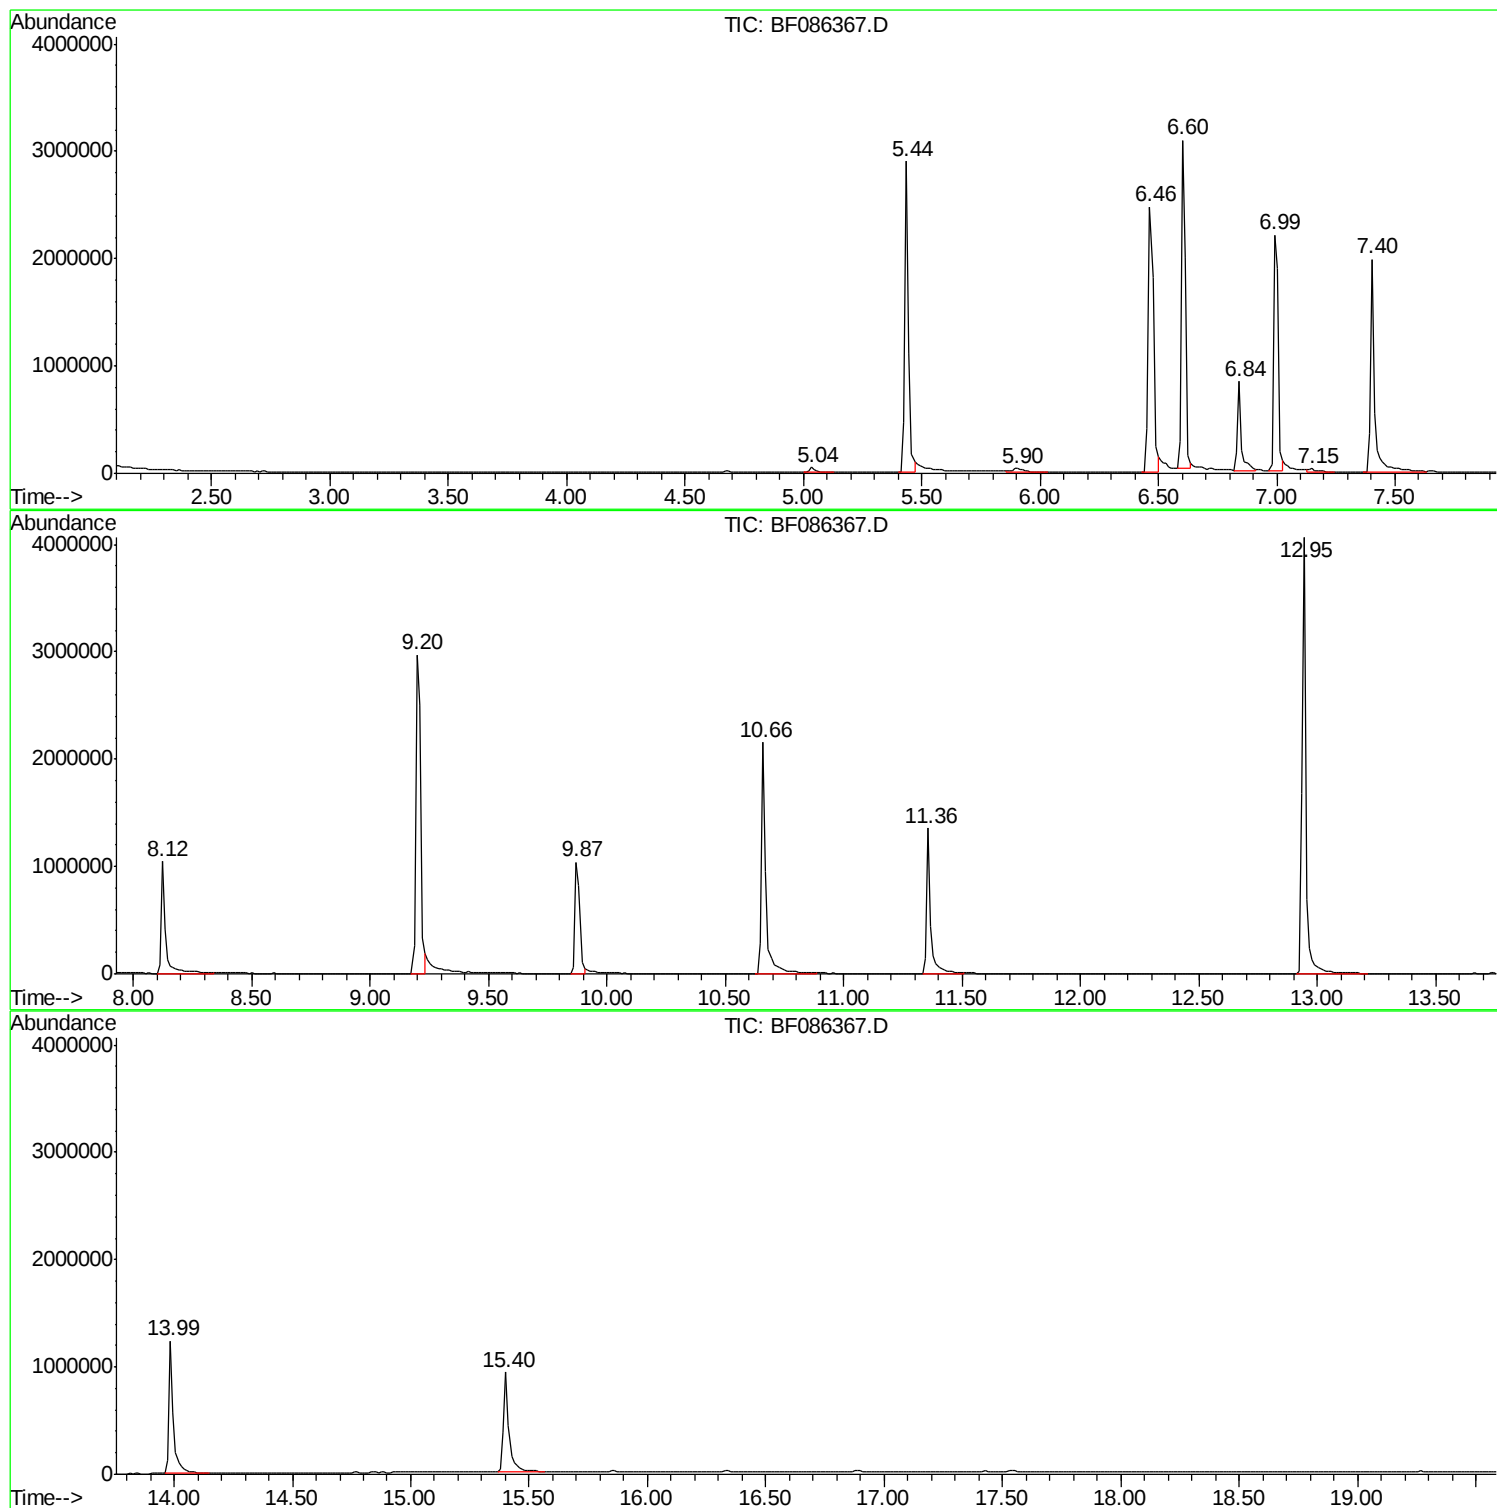

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
Data File : BF086367.D
Acq On : 23 Apr 2016 3:23
Operator : UM/SJ
Sample : PB89989BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89989BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
Data File : BF086367.D
Acq On : 23 Apr 2016 3:23
Operator : UM/SJ
Sample : PB89989BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB89989BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc