

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
 Data File : BF086373.D
 Acq On : 23 Apr 2016 6:19
 Operator : UM/SJ
 Sample : H2634-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-13

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.013	253	256	266	rBV	186462	292068	5.65%	0.858%
2	5.424	290	292	295	rBV	1346345	1778589	34.39%	5.223%
3	5.847	326	329	331	rBV	49442	68568	1.33%	0.201%
4	6.465	380	383	388	rBV	1088925	1241517	24.01%	3.646%
5	6.602	393	395	398	rBV	3218647	3322820	64.25%	9.758%
6	6.842	414	416	422	rBV	768457	940582	18.19%	2.762%
7	6.990	427	429	432	rBV	2233554	3230658	62.47%	9.487%
8	7.402	462	465	482	rBV	2167475	2883491	55.75%	8.468%
9	8.122	526	528	537	rBV	1025031	1275027	24.65%	3.744%
10	9.208	620	623	625	rBV	3326961	4953730	95.78%	14.548%
11	9.871	679	681	684	rBV	1053833	1375499	26.60%	4.039%
12	10.659	748	750	753	rBV	2378711	2972944	57.48%	8.731%
13	10.785	760	761	768	rVB	51909	75506	1.46%	0.222%
14	11.356	809	811	825	rBV	1308828	1612949	31.19%	4.737%
15	12.945	947	950	968	rBV	4323975	5171763	100.00%	15.188%
16	13.985	1039	1041	1053	rBV	1117193	1535305	29.69%	4.509%
17	15.403	1162	1165	1177	rBV	780794	1321069	25.54%	3.880%


Sum of corrected areas: 34052085

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
Data File : BF086373.D
Acq On : 23 Apr 2016 6:19
Operator : UM/SJ
Sample : H2634-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-13

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

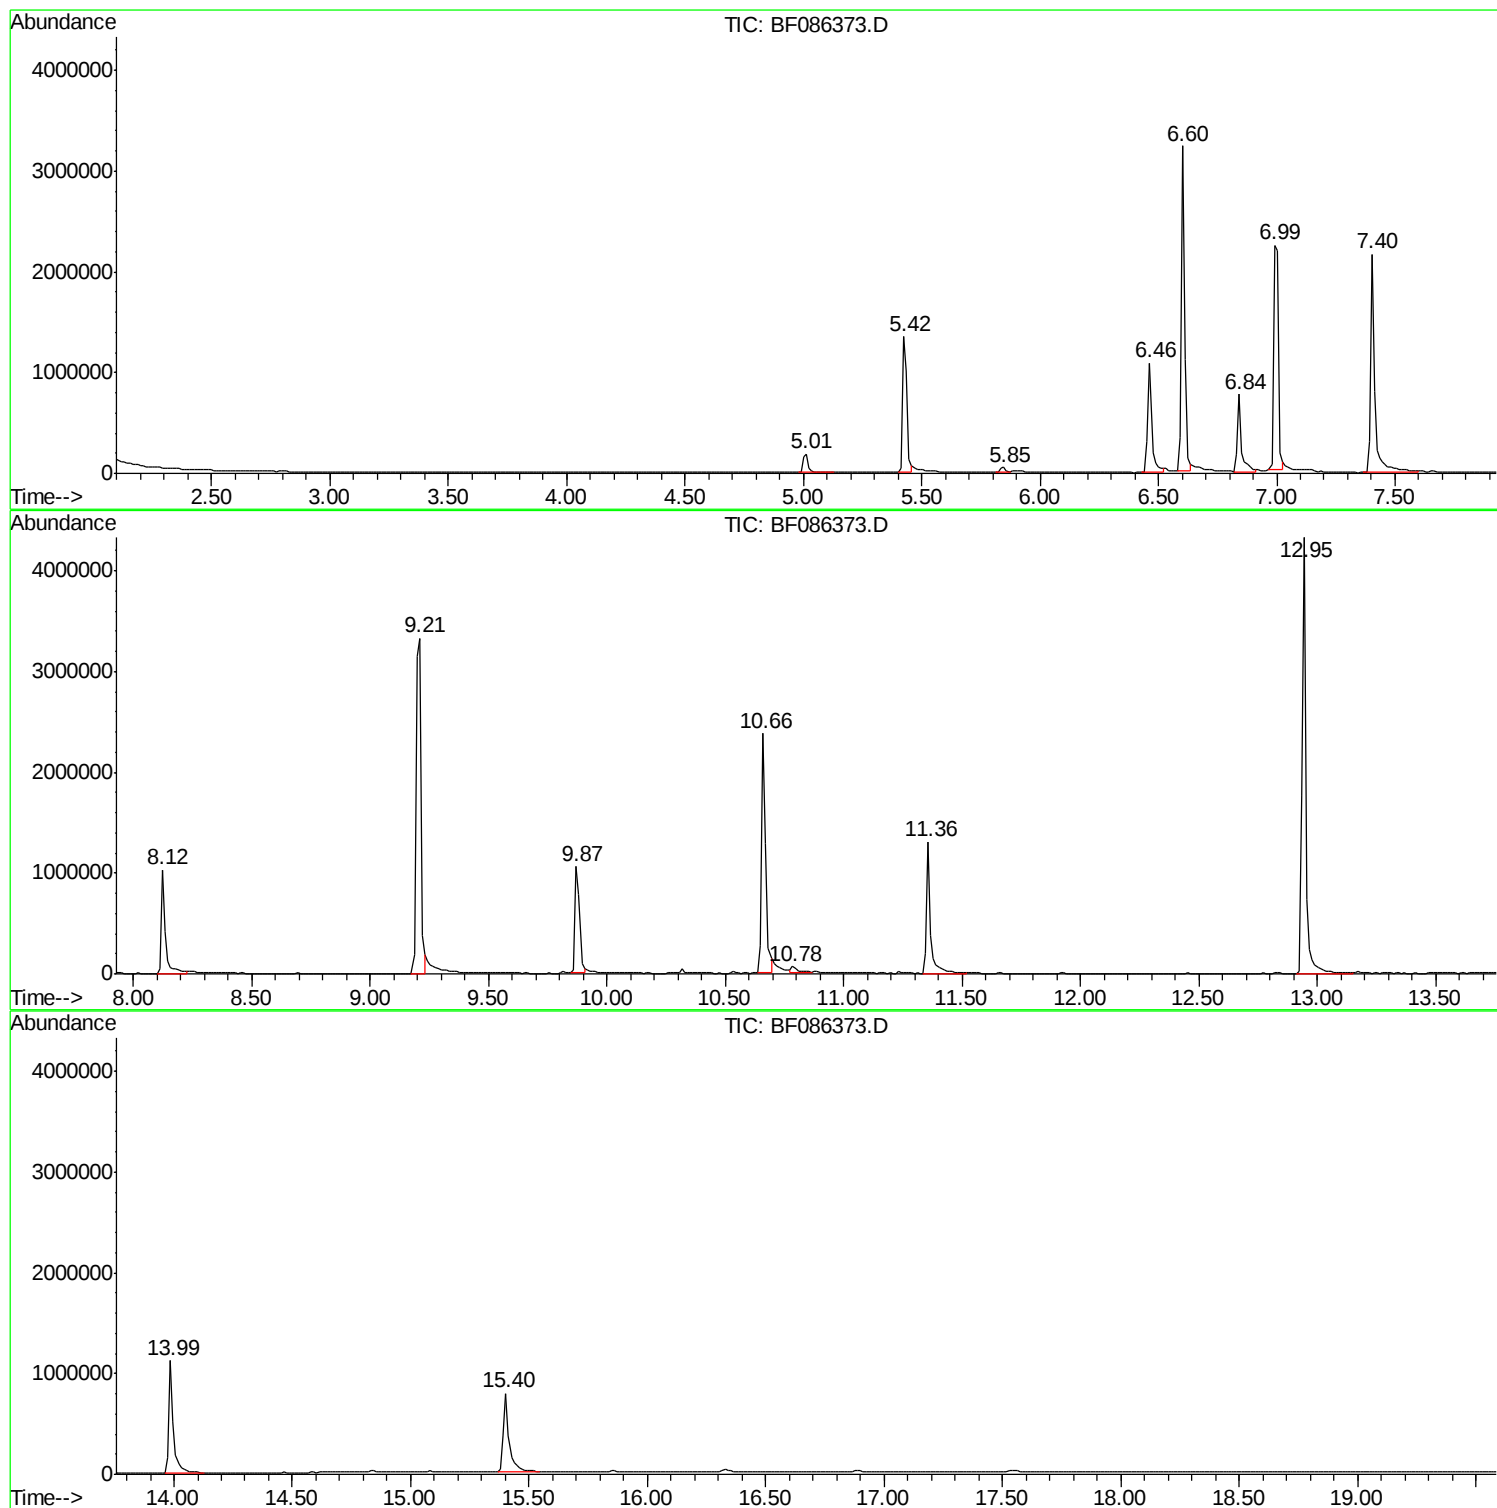

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
Data File : BF086373.D
Acq On : 23 Apr 2016 6:19
Operator : UM/SJ
Sample : H2634-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-13










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.01	6.21 ng	292068	1,4-Dichlorobenzene-d4	6.84

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45
2		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	17
3		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9
4		5-Hexen-2-one	98	C6H10O	000109-49-9	9
5		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9

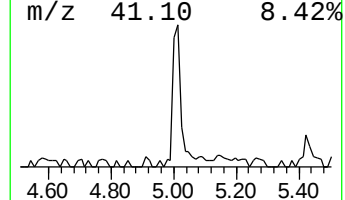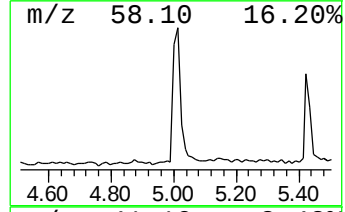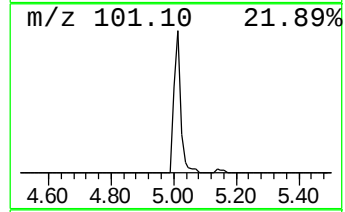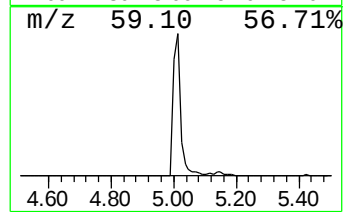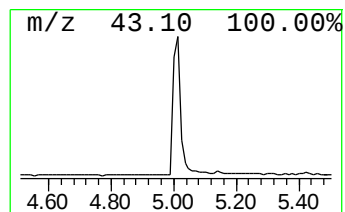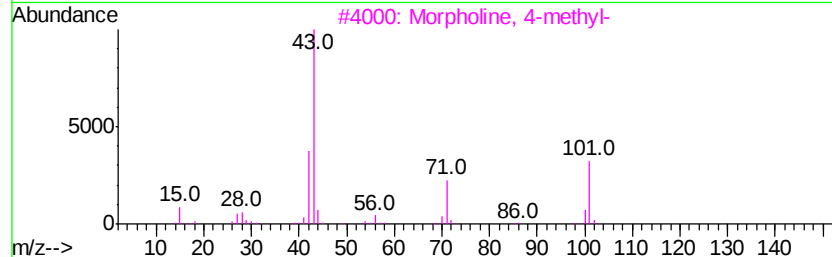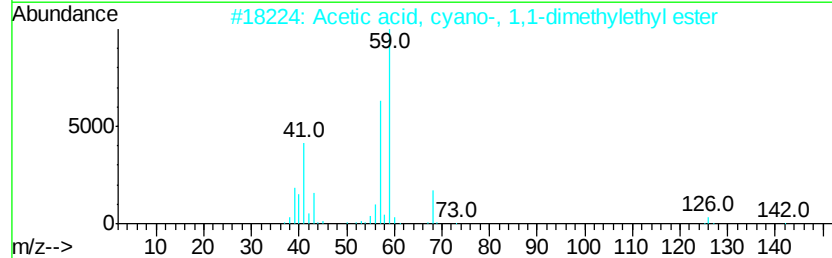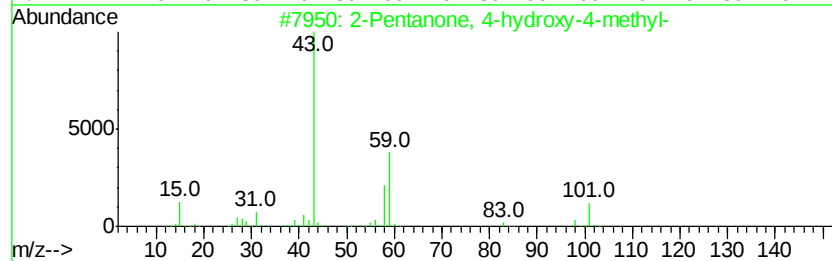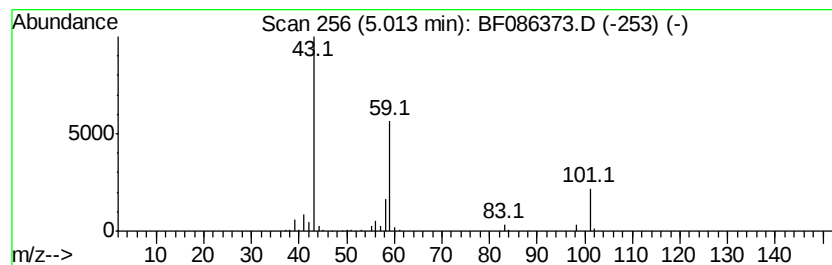

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
Data File : BF086373.D
Acq On : 23 Apr 2016 6:19
Operator : UM/SJ
Sample : H2634-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-13










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	70.65 ng	3322820	1,4-Dichlorobenzene-d4	6.84

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

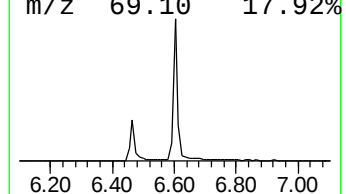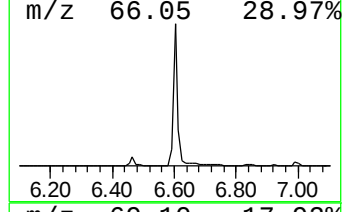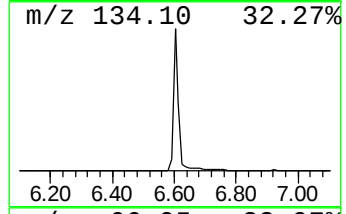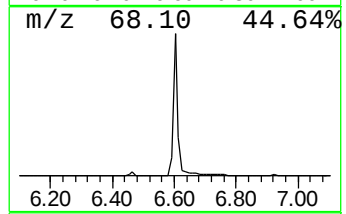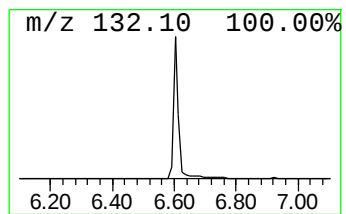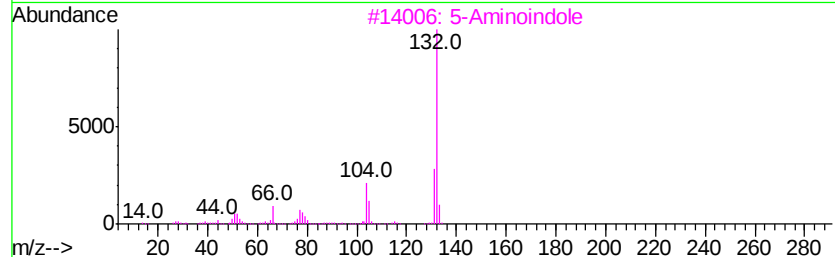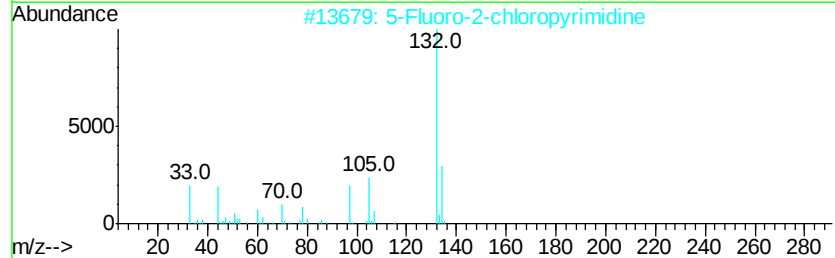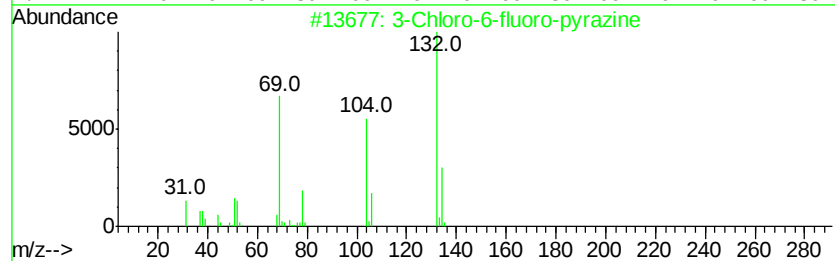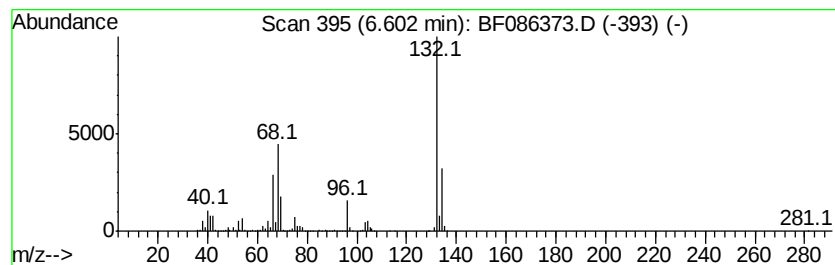

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
Data File : BF086373.D
Acq On : 23 Apr 2016 6:19
Operator : UM/SJ
Sample : H2634-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-13

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.01	6.2	ng	292068	1	6.84	940582	20.0
unknown6.60	6.60	70.7	ng	3322820	1	6.84	940582	20.0