


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042216\
 Data File : BF086386.D
 Acq On : 23 Apr 2016 12:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF042216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 25 10:49:13 2016

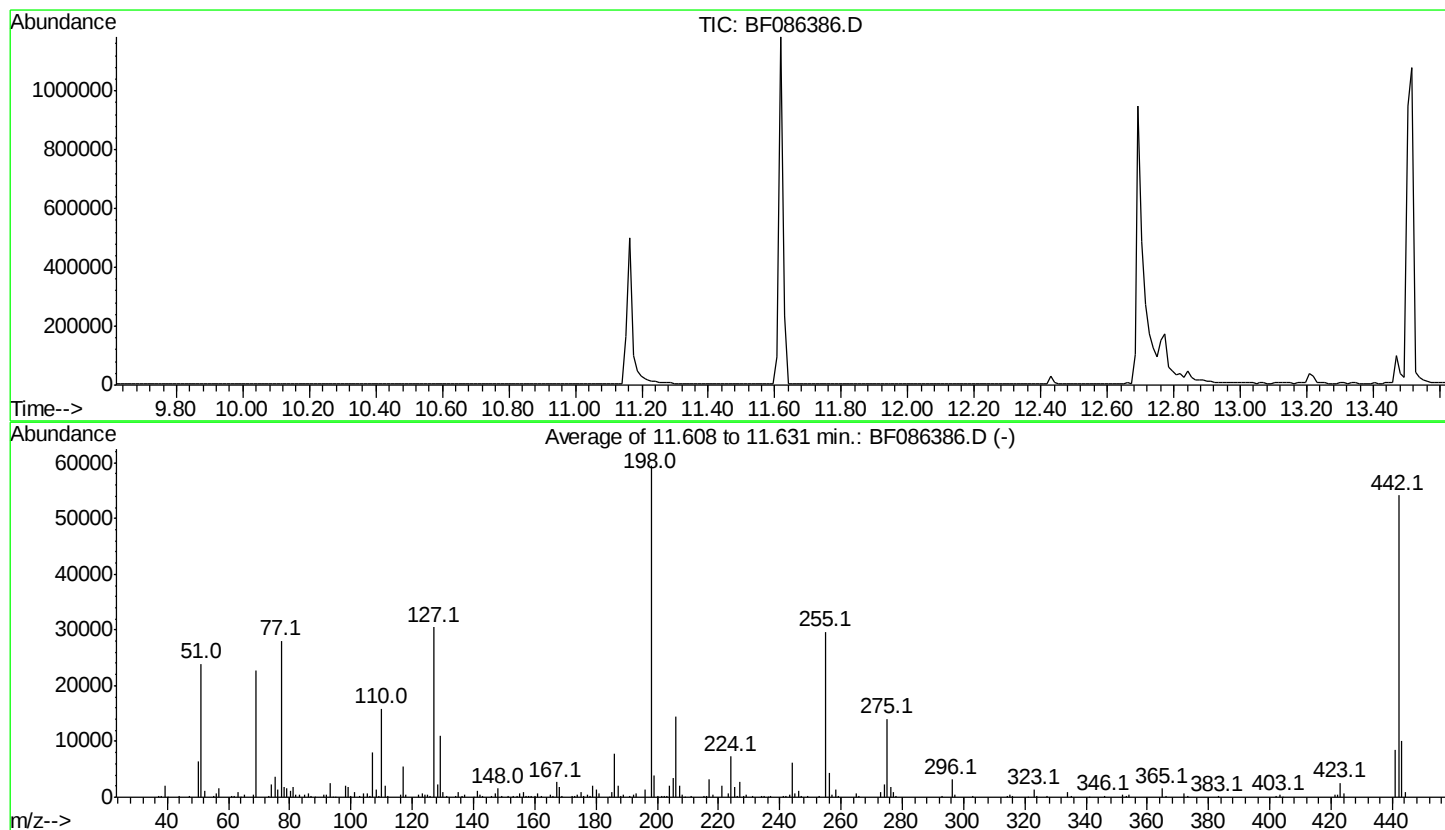

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	23899	PASS
68	69	0.00	2	1.7	394	PASS
69	198	0.00	100	38.3	22793	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	30459	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59470	PASS
199	198	5	9	6.6	3928	PASS
275	198	10	60	23.7	14089	PASS
365	198	1	100	2.6	1560	PASS
441	442	0.01	24	15.6	8449	PASS
442	198	50	100	91.0	54098	PASS
443	442	15	24	18.6	10068	PASS