
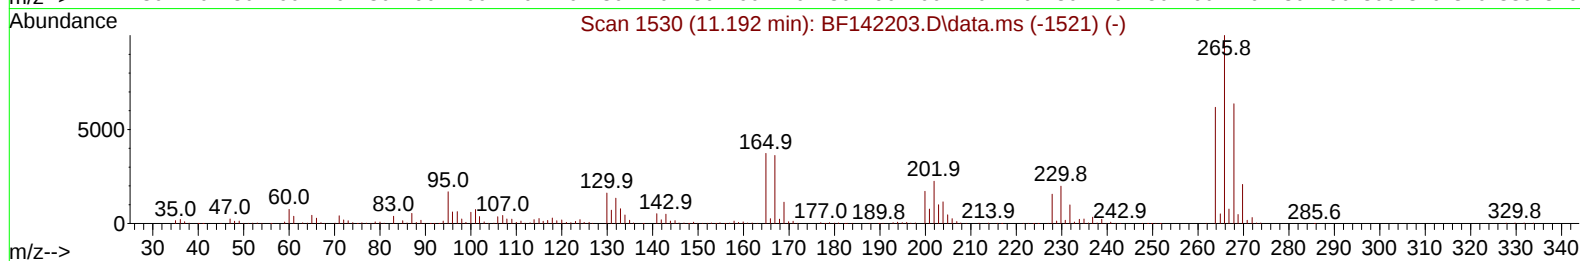
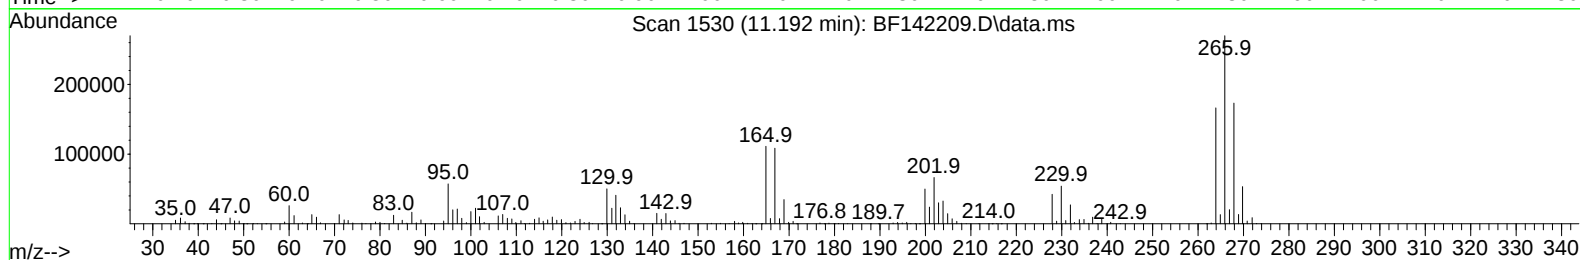


Quant Time: Apr 22 09:09:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 22 02:14:30 2025
Response via : Initial Calibration

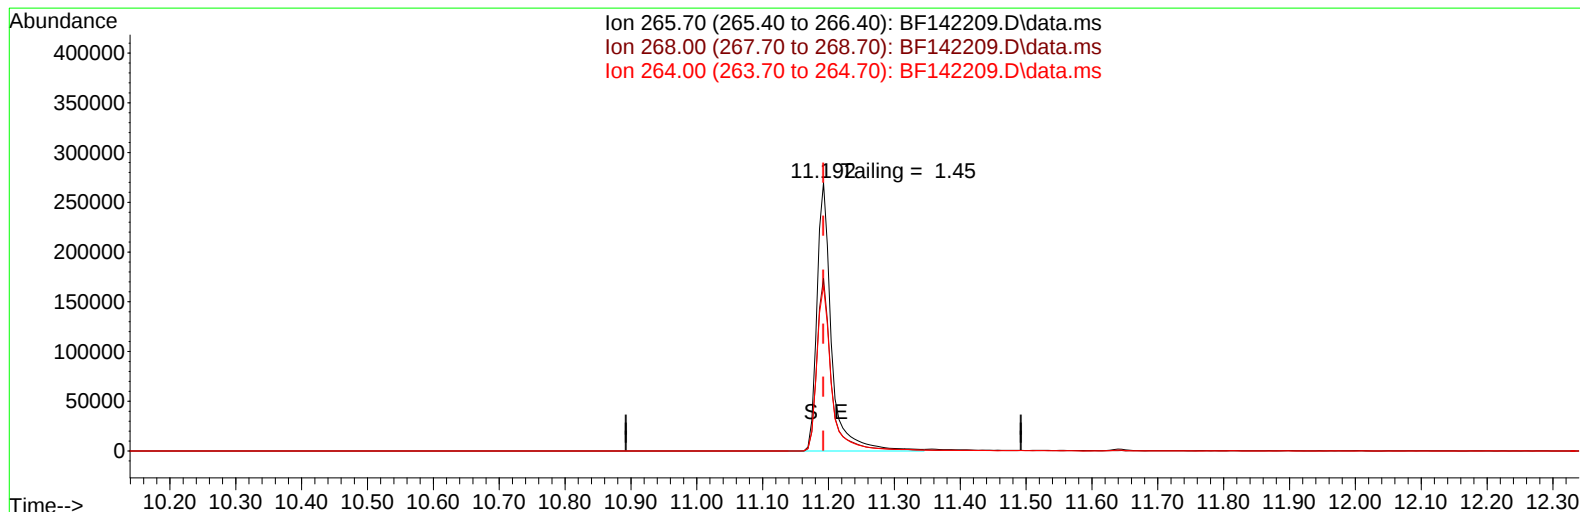

TIC: BF142209.D\data.ms

(70) Pentachlorophenol (C)




11.192min (+ 0.000) 24355.42 ng

response **415153**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.22
264.00	61.80	61.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042225\
Data File : BF142209.D
Acq On : 22 Apr 2025 08:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 22 09:09:44 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 22 02:14:30 2025
Response via : Initial Calibration

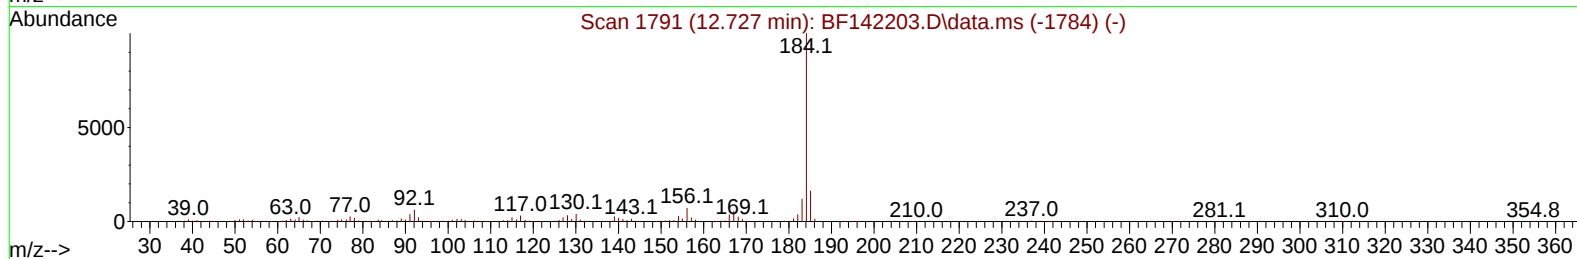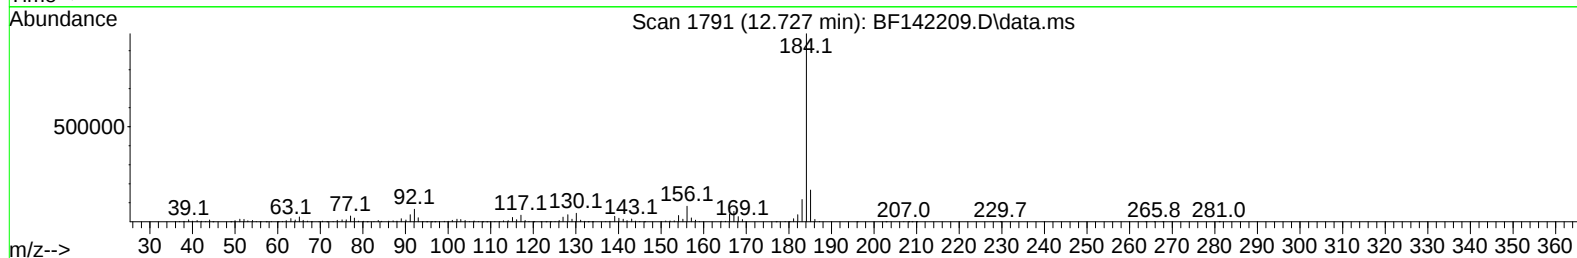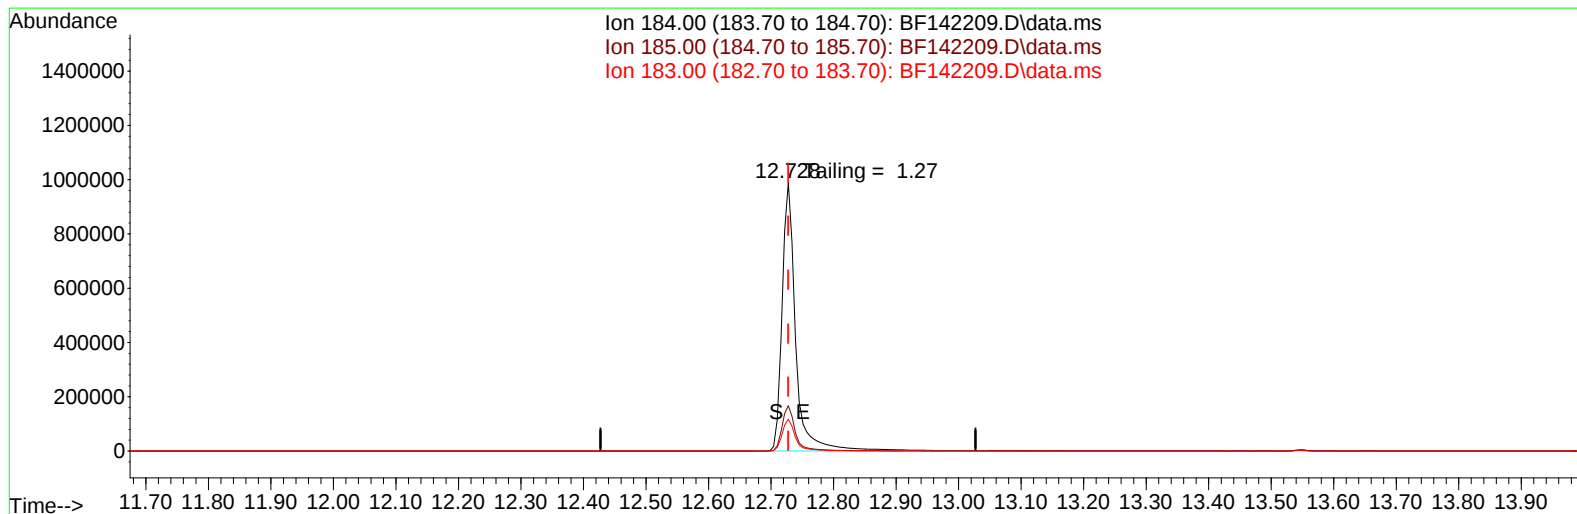

TIC: BF142209.D\data.ms

(77) Benzidine**12.727min (+ 0.000) 124267.94 ng****response 1513832**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.30	16.90
183.00	12.00	11.81
0.00	0.00	0.00