

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042225\
Data File : BF142213.D
Acq On : 22 Apr 2025 15:41
Operator : RC/JU
Sample : PB167672BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167672BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	555	561	583	rBV	4915622	6598282	41.79%	8.463%
2	6.492	725	731	746	rBV	4901851	6650611	42.12%	8.530%
3	6.863	789	794	806	rBV	1975049	2485492	15.74%	3.188%
4	7.428	883	890	905	rBV	4997522	7005253	44.37%	8.985%
5	8.145	1006	1012	1040	rVB	2518325	3423898	21.68%	4.391%
6	9.222	1188	1195	1224	rBV	11571596	15328431	97.08%	19.660%
7	9.904	1305	1311	1328	rBV	3033876	4101514	25.98%	5.261%
8	10.692	1439	1445	1481	rBV	5078531	7019697	44.46%	9.003%
9	11.392	1558	1564	1582	rBV	3073296	4270518	27.05%	5.477%
10	12.974	1827	1833	1855	rBV	11404525	15789660	100.00%	20.252%
11	14.033	2007	2013	2029	rBV	1897893	2811766	17.81%	3.606%
12	15.504	2257	2263	2284	rBV	1365990	2481372	15.72%	3.183%




Sum of corrected areas: 77966494

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042225\
Data File : BF142213.D
Acq On : 22 Apr 2025 15:41
Operator : RC/JU
Sample : PB167672BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167672BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

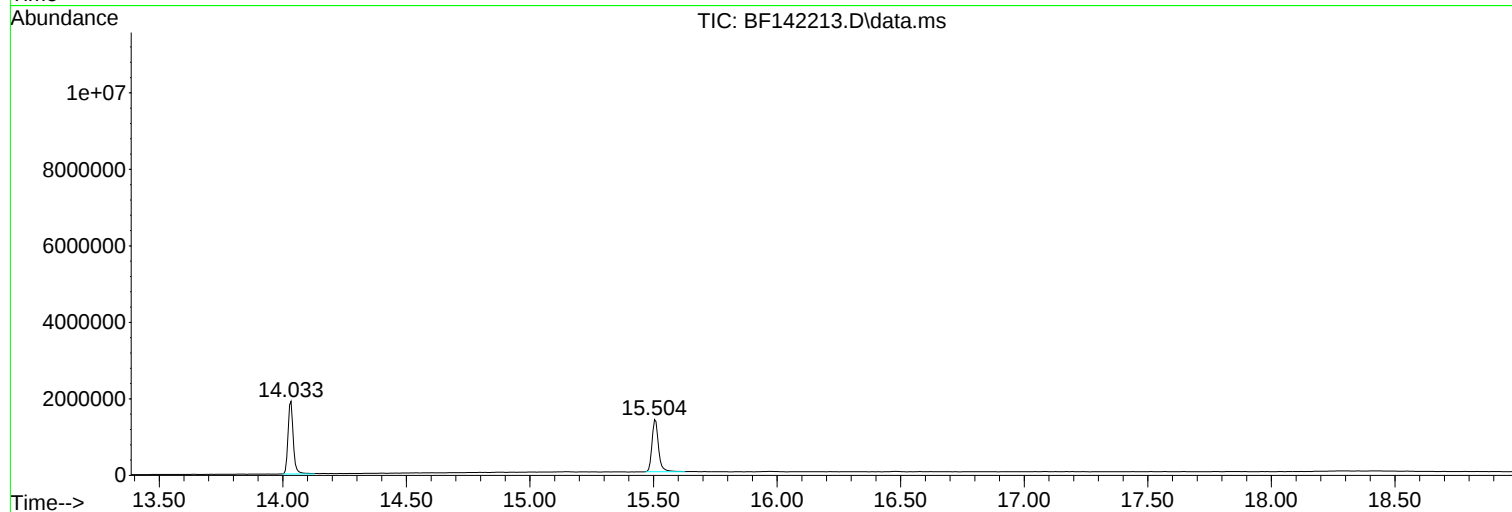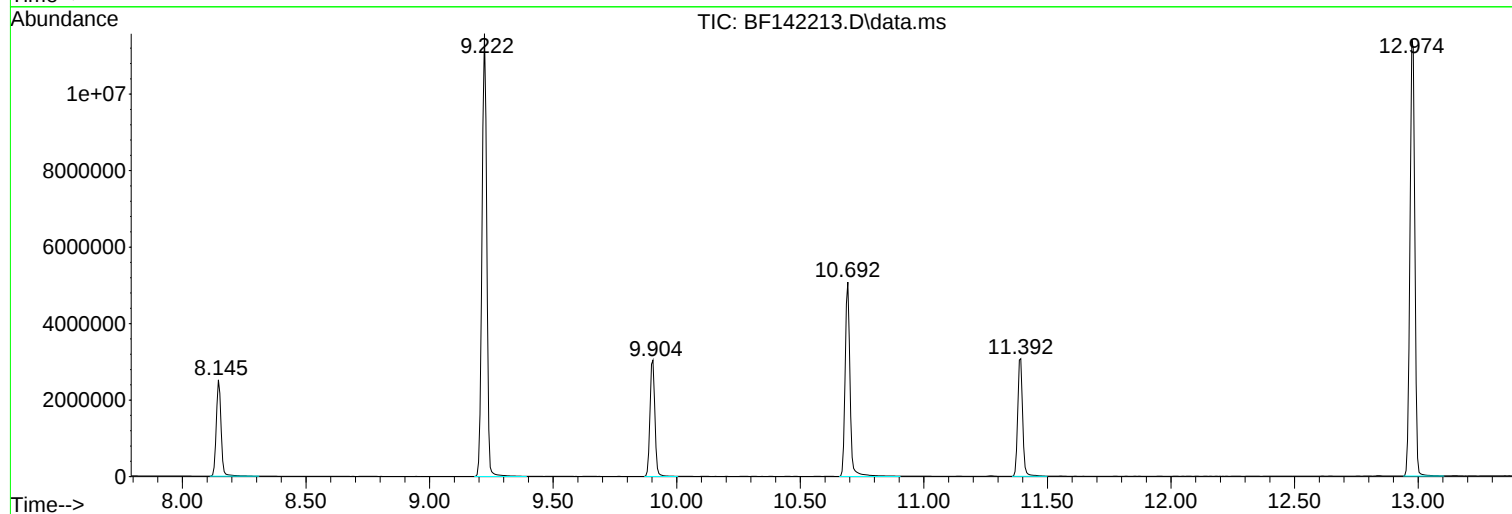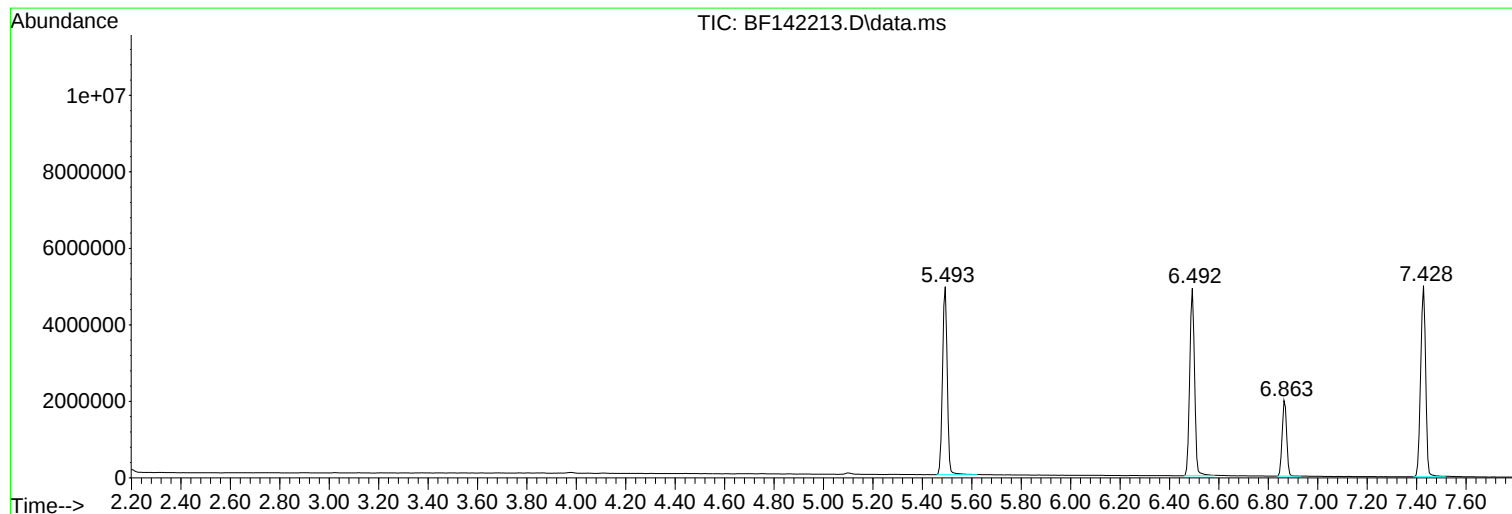

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042225\
Data File : BF142213.D
Acq On : 22 Apr 2025 15:41
Operator : RC/JU
Sample : PB167672BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167672BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042225\
Data File : BF142213.D
Acq On : 22 Apr 2025 15:41
Operator : RC/JU
Sample : PB167672BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167672BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------