

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042315\
 Data File : BF078771.D
 Acq On : 24 Apr 2015 5:19
 Operator : TP/IZ
 Sample : G1987-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-22

Quant Time: Apr 24 06:03:45 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 24 04:11:59 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.76	152	28258	20.00	ng	0.00
21) Naphthalene-d8	7.92	136	114182	20.00	ng	0.00
38) Acenaphthene-d10	11.10	164	58107	20.00	ng	0.00
63) Phenanthrene-d10	13.83	188	114028	20.00	ng	0.00
75) Chrysene-d12	17.71	240	129906	20.00	ng	0.00
86) Perylene-d12	19.43	264	127899	20.00	ng	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	3.78	112	92467	53.95	ng	0.01
7) Phenol-d6	5.27	99	70981	33.05	ng	0.00
23) Nitrobenzene-d5	6.70	82	163783	86.94	ng	0.00
41) 2,4,6-Tribromophenol	12.57	330	68028	141.16	ng	0.00
44) 2-Fluorobiphenyl	9.93	172	356903	87.80	ng	0.00
78) Terphenyl-d14	16.38	244	359939	62.61	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	5.29	94	795	0.31	ng	# 36
15) Benzyl Alcohol	5.99	79	2696	1.79	ng	# 51
20) 3+4-Methylphenols	6.51	107	2099	1.00	ng	# 40
22) Acetophenone	6.42	105	713	0.27	ng	# 58
24) Nitrobenzene	6.70	77	274	0.14	ng	# 30
31) Naphthalene	7.95	128	987	0.17	ng	# 69
37) 2-Methylnaphthalene	9.21	142	499	0.12	ng	# 1
47) 2-Nitroaniline	10.33	65	8216	8.88	ng	# 26
49) Dimethylphthalate	10.73	163	3609	0.83	ng	# 76
54) Dibenzofuran	11.49	168	269	0.05	ng	# 44
57) Fluorene	12.11	166	219	0.05	ng	# 9
59) Diethylphthalate	12.06	149	2098	0.50	ng	# 86
62) Azobenzene	12.49	77	2699	0.70	ng	# 1
70) Phenanthrene	13.87	178	348	0.05	ng	# 60
73) Di-n-butylphthalate	14.99	149	1292	0.19	ng	# 79
74) Fluoranthene	15.77	202	554	0.08	ng	# 61
76) Benzidine	16.06	184	1853	0.37	ng	# 66
77) Pyrene	16.09	202	571	0.07	ng	# 58
80) Benzo(a)anthracene	17.71	228	508	0.07	ng	# 52
81) 3,3'-Dichlorobenzidine	17.71	252	253	0.10	ng	# 25
82) Chrysene	17.71	228	508	0.07	ng	# 49
83) Bis(2-ethylhexyl)phthalate	17.85	149	1031	0.21	ng	# 52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042315\
Data File : BF078771.D
Acq On : 24 Apr 2015 5:19
Operator : TP/IZ
Sample : G1987-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-22

Quant Time: Apr 24 06:03:45 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 24 04:11:59 2015
Response via : Initial Calibration




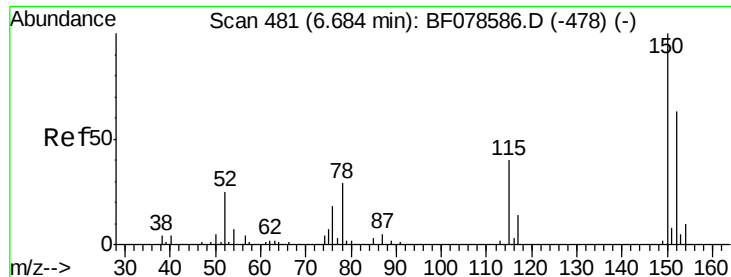




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 5.76 min Scan# 400
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Instrument :
 BNA_F
 ClientSampleId :
 MW-22

Tgt Ion:152 Resp: 28258
 Ion Ratio Lower Upper
 152 100
 150 157.3 125.9 188.9
 115 57.0 52.7 79.1




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E





#5
 2-Fluorophenol
 Concen: 53.95 ng
 RT: 3.78 min Scan# 227
 Delta R.T. 0.01 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion:112 Resp: 92467
 Ion Ratio Lower Upper
 112 100
 64 51.8 39.9 59.9
 63 27.0 20.2 30.4



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0





#7

Phenol-d6

Concen: 33.05 ng

RT: 5.27 min Scan# 357

Delta R.T. 0.00 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19

Instrument :

BNA_F

ClientSampleId :

MW-22


Tgt Ion: 99 Resp: 70981

Ion Ratio Lower Upper

99 100

42 16.8 14.8 22.2




71 32.8 26.6 39.8



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



#10

Phenol

Concen: 0.31 ng

RT: 5.29 min Scan# 359

Delta R.T. 0.01 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19


Tgt Ion: 94 Resp: 795

Ion Ratio Lower Upper

94 100

65 0.0 4.9 44.9#



66 76.1 13.8 53.8#




Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0





#15

Benzyl Alcohol

Concen: 1.79 ng

RT: 5.99 min Scan# 420

Delta R.T. -0.05 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19

Instrument :

BNA_F

ClientSampled :

MW-22





Tgt Ion: 79 Resp: 2696

Ion Ratio Lower Upper

79 100

108 32.5 57.6 86.4#

77 107.6 53.5 80.3#



#20

3+4-Methylphenols

Concen: 1.00 ng

RT: 6.51 min Scan# 466

Delta R.T. -0.02 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19

Tgt Ion: 107 Resp: 2099




Ion Ratio Lower Upper


107 100

108 0.0 64.4 104.4#

77 37.1 9.7 49.7

79 24.9 4.0 44.0









#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.92 min Scan# 589
Delta R.T. 0.00 min
Lab File: BF078771.D
Acq: 24 Apr 2015 5:19




Instrument :
BNA_F
ClientSampleId :
MW-22


Tgt Ion:	136	Resp:	114182
Ion	Ratio	Lower	Upper
136	100		
137	10.0	9.0	13.4
54	6.1	7.0	10.6#
68	4.7	5.4	8.2#



#22
Acetophenone
Concen: 0.27 ng
RT: 6.42 min Scan# 458
Delta R.T. -0.03 min
Lab File: BF078771.D
Acq: 24 Apr 2015 5:19

Tgt Ion:	105	Resp:	713
Ion	Ratio	Lower	Upper
105	100		
71	0.0	5.5	8.3#
51	0.0	16.0	24.0#
120	0.0	17.8	26.6#





#23

Nitrobenzene-d5

Concen: 86.94 ng

RT: 6.70 min Scan# 482

Delta R.T. 0.00 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19

Instrument :

BNA_F

ClientSampled :

MW-22


Tgt Ion: 82 Resp: 163783

Ion Ratio Lower Upper

82 100

128 44.0 31.8 47.8




54 49.5 41.5 62.3



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): B

Ion 54.00 (53.70 to 54.70): BF0



#24

Nitrobenzene

Concen: 0.14 ng

RT: 6.70 min Scan# 482

Delta R.T. -0.03 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19


Tgt Ion: 77 Resp: 274

Ion Ratio Lower Upper

77 100

123 0.0 46.9 70.3#



65 0.0 9.5 14.3#




Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 123.00 (122.70 to 123.70): B

Ion 65.00 (64.70 to 65.70): BF0





#31

Naphthalene

Concen: 0.17 ng

RT: 7.95 min Scan# 592

Delta R.T. 0.00 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19

Instrument :

BNA_F

ClientSampleId :

MW-22


Tgt Ion:128 Resp: 987

Ion Ratio Lower Upper

128 100

129 0.0 8.6 12.8#




127 0.0 10.7 16.1#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



#37

2-Methylnaphthalene

Concen: 0.12 ng

RT: 9.21 min Scan# 702

Delta R.T. 0.00 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19


Tgt Ion:142 Resp: 499

Ion Ratio Lower Upper

142 100

141 221.1 70.3 105.5#



115 0.0 24.6 37.0#




Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E









#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 11.10 min Scan# 867
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19




Instrument :
 BNA_F
 ClientSampleId :
 MW-22


Tgt Ion:164 Resp: 58107
 Ion Ratio Lower Upper
 164 100
 162 102.7 82.2 123.2
 160 43.9 34.7 52.1



#41
 2,4,6-Tribromophenol
 Concen: 141.16 ng
 RT: 12.57 min Scan# 996
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion:330 Resp: 68028
 Ion Ratio Lower Upper
 330 100
 332 98.1 78.6 117.8
 141 40.1 31.2 46.8









#44
 2-Fluorobiphenyl
 Concen: 87.80 ng
 RT: 9.93 min Scan# 765
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19




Instrument :
 BNA_F
 ClientSampleId :
 MW-22


Tgt Ion: 172 Resp: 356903
 Ion Ratio Lower Upper
 172 100
 171 34.6 28.6 42.8
 170 23.5 18.5 27.7



#47
 2-Nitroaniline
 Concen: 8.88 ng
 RT: 10.33 min Scan# 800
 Delta R.T. -0.01 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion: 65 Resp: 8216
 Ion Ratio Lower Upper
 65 100
 92 99.8 51.3 76.9#
 138 0.0 70.4 105.6#





#49

Dimethylphthalate

Concen: 0.83 ng

RT: 10.73 min Scan# 835

Delta R.T. -0.01 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19

Instrument :

BNA_F

ClientSampleId :

MW-22


Tgt Ion:163 Resp: 3609

Ion Ratio Lower Upper

163 100

194 0.0 2.3 3.5#




164 0.0 8.6 13.0#



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



#54

Dibenzofuran

Concen: 0.05 ng

RT: 11.49 min Scan# 901

Delta R.T. 0.00 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19


Tgt Ion:168 Resp: 269

Ion Ratio Lower Upper

168 100

139 0.0 31.0 46.4#



169 0.0 10.7 16.1#




Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E









#57
Fluorene
 Concen: 0.05 ng
 RT: 12.11 min Scan# 956
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19




Instrument :
 BNA_F
 ClientSampleId :
 MW-22


Tgt Ion:166 Resp: 219
 Ion Ratio Lower Upper
 166 100
 165 0.0 78.9 118.3#
 167 0.0 10.7 16.1#



#59
Diethylphthalate
 Concen: 0.50 ng
 RT: 12.06 min Scan# 951
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion:149 Resp: 2098
 Ion Ratio Lower Upper
 149 100
 177 24.0 17.4 26.2
 150 0.0 9.4 14.2#





#62

Azobenzene

Concen: 0.70 ng

RT: 12.49 min Scan# 989

Delta R.T. 0.02 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19

Instrument :

BNA_F

ClientSampleId :

MW-22

Tgt Ion: 77 Resp: 2699


Ion Ratio Lower Upper

77 100

182 67.7 0.0 36.8#

105 143.2 0.3 40.3#

51 41.5 9.1 49.1






Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 182.00 (181.70 to 182.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 51.00 (50.70 to 51.70): BF0



#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 13.83 min Scan# 1106

Delta R.T. 0.00 min

Lab File: BF078771.D

Acq: 24 Apr 2015 5:19


Tgt Ion: 188 Resp: 114028

Ion Ratio Lower Upper

188 100

94 9.4 9.0 13.4



80 10.8 9.5 14.3




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0









#70
 Phenanthrene
 Concen: 0.05 ng
 RT: 13.87 min Scan# 1110
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19




Instrument :
 BNA_F
 ClientSampleId :
 MW-22


Tgt Ion:178 Resp: 348
 Ion Ratio Lower Upper
 178 100
 176 0.0 15.4 23.0#
 179 0.0 12.2 18.2#



#73
 Di-n-butylphthalate
 Concen: 0.19 ng
 RT: 14.99 min Scan# 1208
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion:149 Resp: 1292
 Ion Ratio Lower Upper
 149 100
 150 0.0 7.1 10.7#
 104 0.0 3.8 5.6#









#74
 Fluoranthene
 Concen: 0.08 ng
 RT: 15.77 min Scan# 1276
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Instrument :
 BNA_F
 ClientSampleId :
 MW-22

Tgt Ion: 202 Resp: 554
 Ion Ratio Lower Upper
 202 100
 101 0.0 0.0 35.2
 203 0.0 0.0 38.5




Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 203.00 (202.70 to 203.70): E






#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 17.71 min Scan# 1446
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion: 240 Resp: 129906
 Ion Ratio Lower Upper
 240 100
 120 10.7 7.1 10.7#
 236 24.8 21.4 32.2



Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E









#76
Benzidine
Concen: 0.37 ng
RT: 16.06 min Scan# 1301
Delta R.T. 0.01 min
Lab File: BF078771.D
Acq: 24 Apr 2015 5:19

Instrument :
BNA_F
ClientSampleId :
MW-22

Tgt Ion:184 Resp: 1853
Ion Ratio Lower Upper
184 100
185 0.0 12.2 18.2#
183 0.0 9.5 14.3#




Abundance Ion 184.00 (183.70 to 184.70): E
Ion 185.00 (184.70 to 185.70): E
Ion 183.00 (182.70 to 183.70): E






#77
Pyrene
Concen: 0.07 ng
RT: 16.09 min Scan# 1304
Delta R.T. 0.00 min
Lab File: BF078771.D
Acq: 24 Apr 2015 5:19

Tgt Ion:202 Resp: 571
Ion Ratio Lower Upper
202 100
200 0.0 16.3 24.5#
203 0.0 13.8 20.6#



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E









#78
 Terphenyl-d14
 Concen: 62.61 ng
 RT: 16.38 min Scan# 1329
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19




Instrument :
 BNA_F
 ClientSampleId :
 MW-22


Tgt Ion: 244 Resp: 359939
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.0 7.4
 122 12.1 7.1 10.7#



#80
 Benzo(a)anthracene
 Concen: 0.07 ng
 RT: 17.71 min Scan# 1446
 Delta R.T. 0.01 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion: 228 Resp: 508
 Ion Ratio Lower Upper
 228 100
 226 0.0 21.3 31.9#
 229 0.0 15.4 23.2#









#81
 3,3'-Dichlorobenzidine
 Concen: 0.10 ng
 RT: 17.71 min Scan# 1446
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Instrument :
 BNA_F
 ClientSampleId :
 MW-22

Tgt Ion: 252 Resp: 253
 Ion Ratio Lower Upper
 252 100
 254 0.0 51.2 76.8#
 126 0.0 6.3 9.5#




Abundance Ion 252.00 (251.70 to 252.70): E
 Ion 254.00 (253.70 to 254.70): E
 Ion 126.00 (125.70 to 126.70): E






#82
 Chrysene
 Concen: 0.07 ng
 RT: 17.71 min Scan# 1446
 Delta R.T. -0.03 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion: 228 Resp: 508
 Ion Ratio Lower Upper
 228 100
 226 0.0 24.2 36.4#
 229 0.0 15.8 23.8#



Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 226.00 (225.70 to 226.70): E
 Ion 229.00 (228.70 to 229.70): E







#83
 Bis(2-ethylhexyl)phthalate
 Concen: 0.21 ng
 RT: 17.85 min Scan# 1458
 Delta R.T. 0.00 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Instrument :
 BNA_F
 ClientSampled :
 MW-22



Tgt Ion:149 Resp: 1031
 Ion Ratio Lower Upper
 149 100
 167 0.0 22.2 33.2#
 279 0.0 3.2 4.8#



Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E




Time-->




#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 19.43 min Scan# 1596
 Delta R.T. 0.01 min
 Lab File: BF078771.D
 Acq: 24 Apr 2015 5:19

Tgt Ion:264 Resp: 127899
 Ion Ratio Lower Upper
 264 100
 260 23.2 18.6 27.8
 265 21.4 17.0 25.6



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E



Time-->

