


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042315\
 Data File : BG016668.D
 Acq On : 24 Apr 2015 1:30
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 23 19:19:11 2015

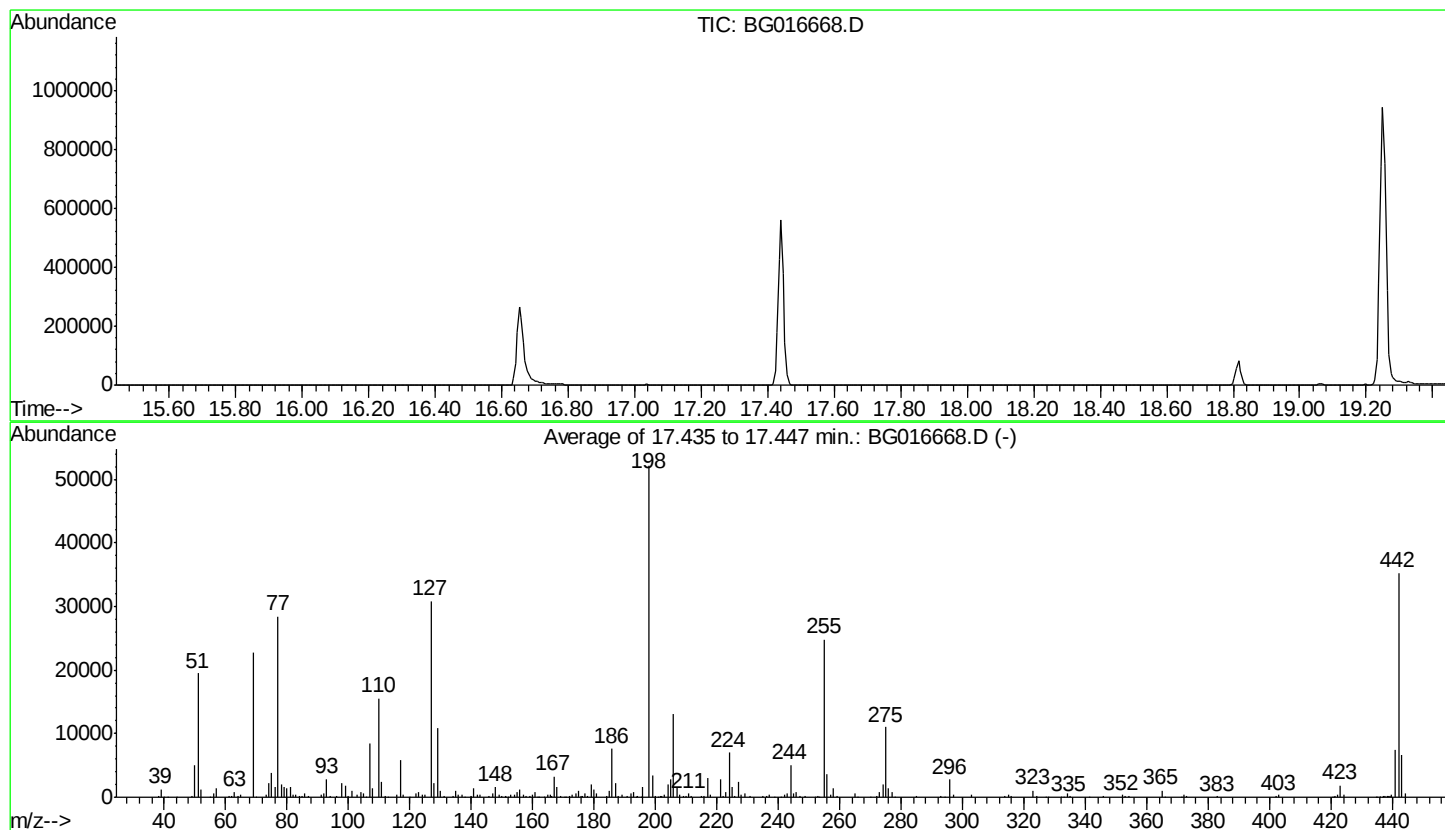

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	19437	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.6	22754	PASS
70	69	0.00	2	0.2	50	PASS
127	198	10	80	59.3	30898	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52133	PASS
199	198	5	9	6.5	3407	PASS
275	198	10	60	21.2	11059	PASS
365	198	1	100	2.1	1090	PASS
441	442	0.01	24	21.2	7473	PASS
442	198	50	100	67.6	35250	PASS
443	442	15	24	18.7	6608	PASS