
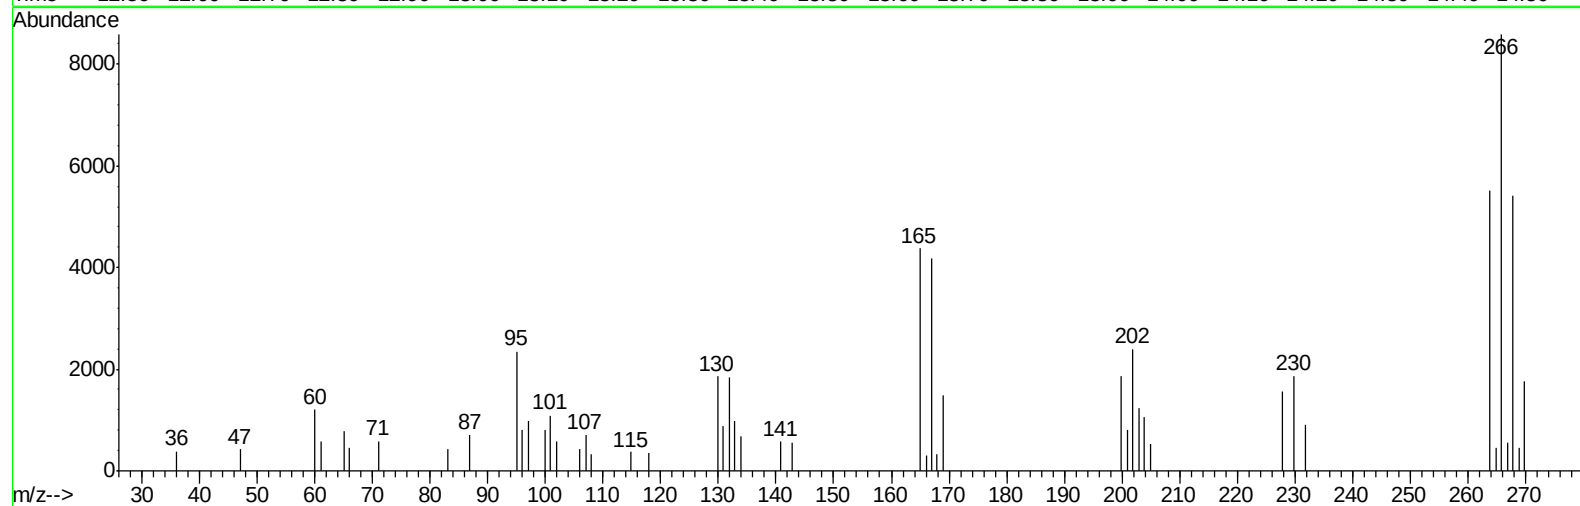


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042315\
Data File : BF078745.D
Acq On : 23 Apr 2015 11:33
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:39:24 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 24 00:49:54 2015
Response via : Initial Calibration

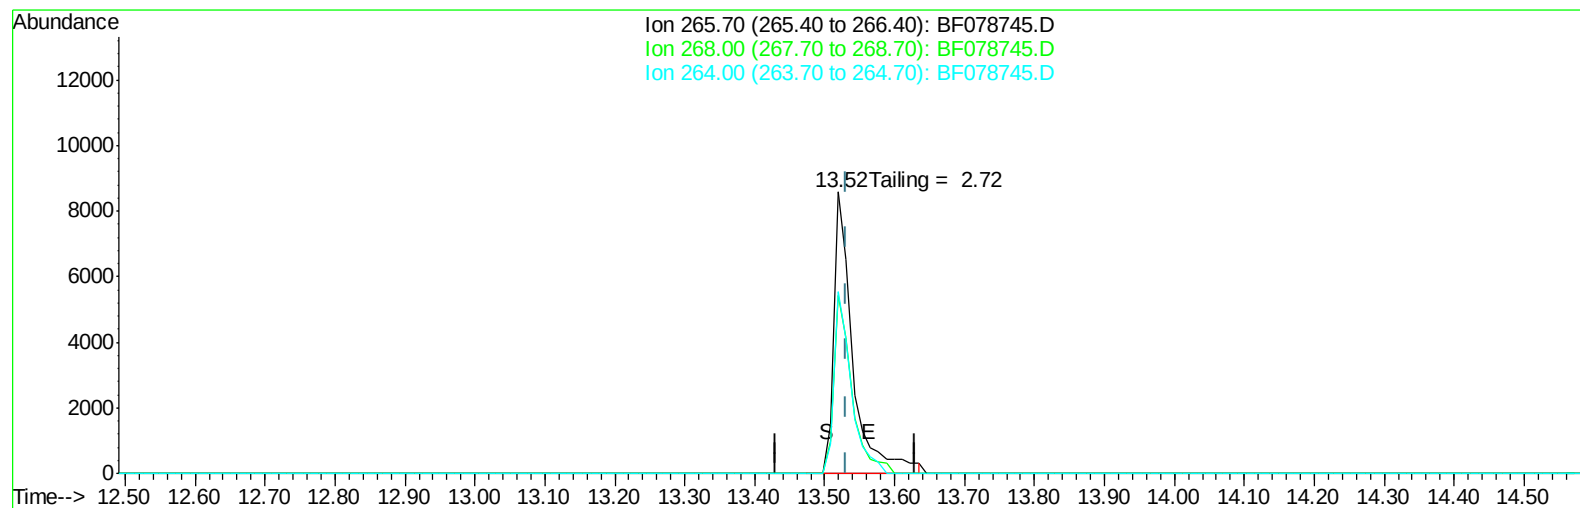

TIC: BF078745.D

(69) Pentachlorophenol (C)



13.520min (-0.011) 0.00ng

response 15200

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	63.14
264.00	62.50	64.34
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042315\
Data File : BF078745.D
Acq On : 23 Apr 2015 11:33
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:39:24 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 24 00:49:54 2015
Response via : Initial Calibration

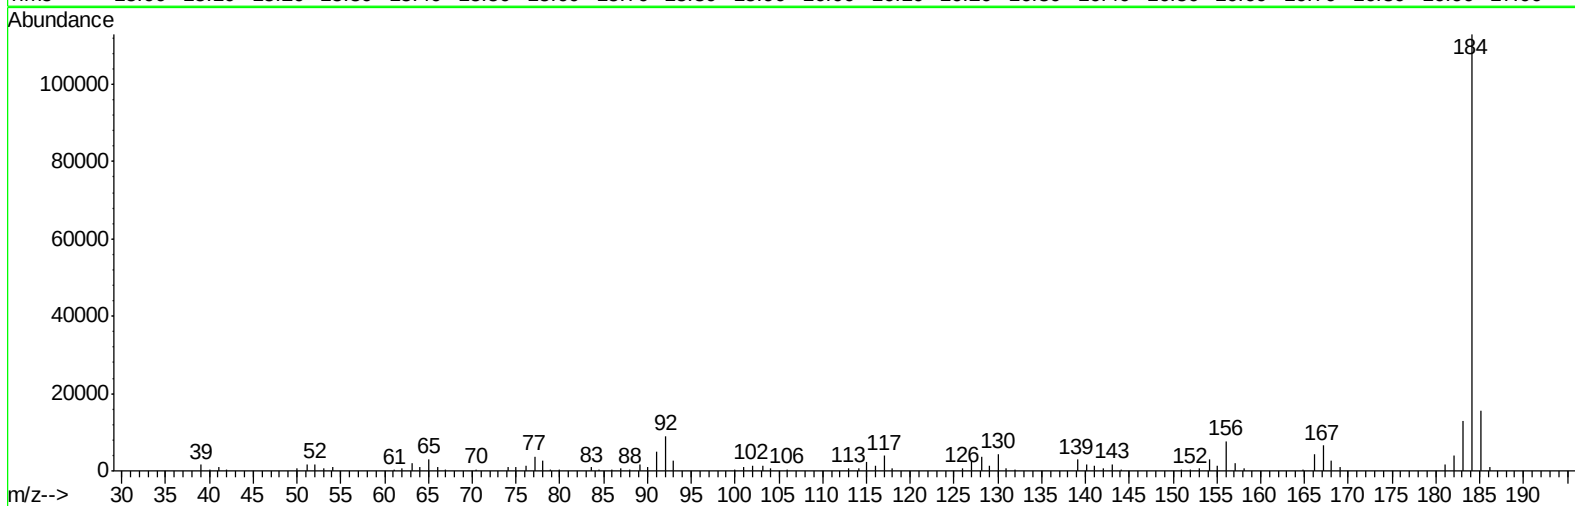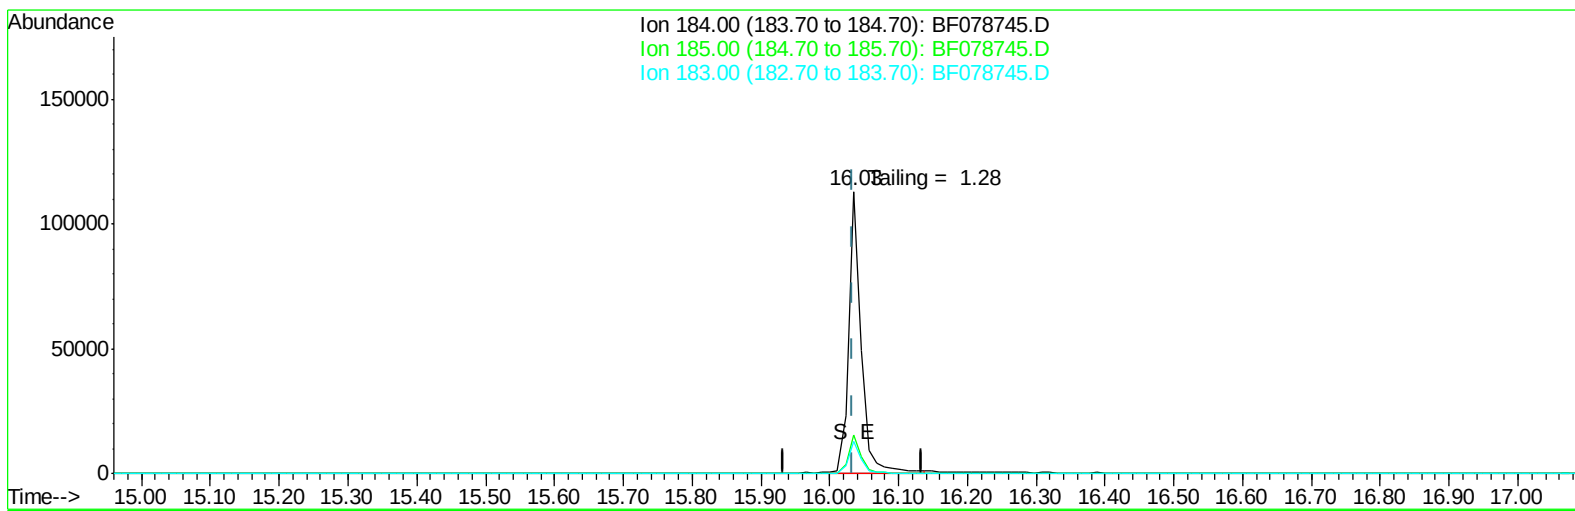

TIC: BF078745.D

(76) Benzidine

16.034min (+0.000) 0.00ng

response 140407

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.88
183.00	11.90	11.30
0.00	0.00	0.00