

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042315\
 Data File : BF078750.D
 Acq On : 23 Apr 2015 15:57
 Operator : TP/IZ
 Sample : G1938-17 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-79S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.404	18	19	24	rVV	25946	43144	1.40%	0.819%
2	1.484	24	26	66	rVB	1526144	3085033	100.00%	58.569%
3	3.770	224	226	236	rVB	56506	82098	2.66%	1.559%
4	5.256	354	356	366	rBV	60392	95795	3.11%	1.819%
5	5.393	366	368	371	rBV	83866	99543	3.23%	1.890%
6	5.759	397	400	404	rVB	67542	102981	3.34%	1.955%
7	5.987	417	420	423	rBV	63261	76721	2.49%	1.457%
8	6.696	479	482	487	rBB	40783	57904	1.88%	1.099%
9	7.907	586	588	591	rBV	107804	143638	4.66%	2.727%
10	9.919	762	764	767	rBV	92875	120554	3.91%	2.289%
11	11.096	864	867	870	rBV	125385	169563	5.50%	3.219%
12	12.559	992	995	999	rBB	28807	44268	1.43%	0.840%
13	13.828	1103	1106	1108	rBV	128013	182122	5.90%	3.458%
14	15.771	1274	1276	1279	rBB	44506	48612	1.58%	0.923%
15	16.080	1301	1303	1306	rBV	51391	55845	1.81%	1.060%
16	16.365	1326	1328	1331	rVB	120523	154718	5.02%	2.937%
17	17.703	1442	1445	1447	rBV	218422	272887	8.85%	5.181%
18	18.994	1555	1558	1562	rBV	29339	73394	2.38%	1.393%
19	19.349	1587	1589	1592	rVV	24449	34795	1.13%	0.661%
20	19.417	1592	1595	1600	rBV	179598	269628	8.74%	5.119%
21	20.023	1643	1648	1652	rBV5	14554	54103	1.75%	1.027%


Sum of corrected areas: 5267346

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042315\
Data File : BF078750.D
Acq On : 23 Apr 2015 15:57
Operator : TP/IZ
Sample : G1938-17 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-79S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

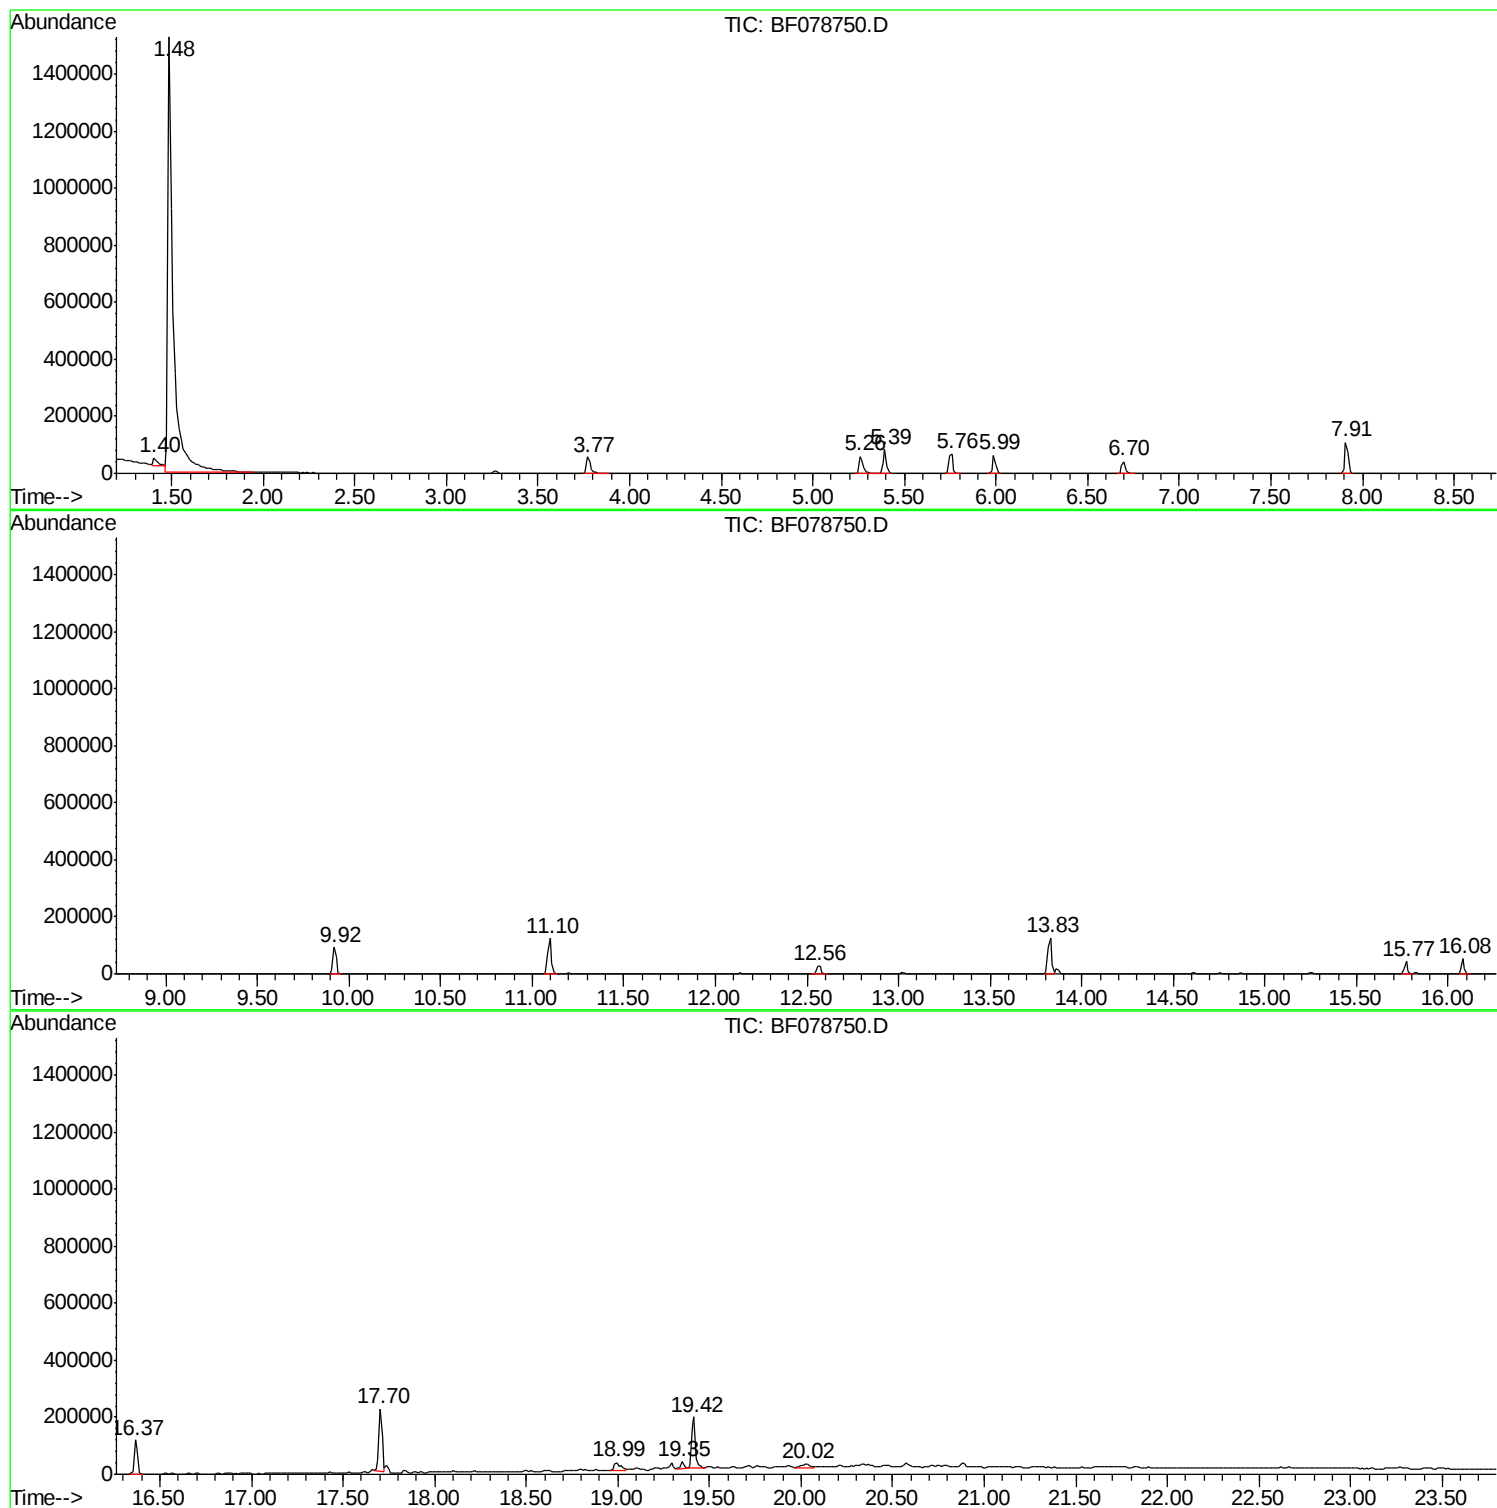

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042315\
Data File : BF078750.D
Acq On : 23 Apr 2015 15:57
Operator : TP/IZ
Sample : G1938-17 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-79S










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown5.39 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.39	19.33 ng	99543	1,4-Dichlorobenzene-d4	5.76

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Xenon	132	Xe	007440-63-3	9
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

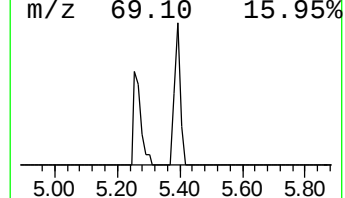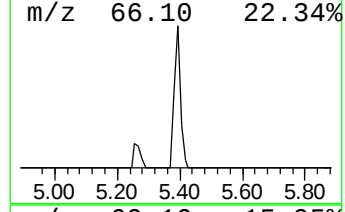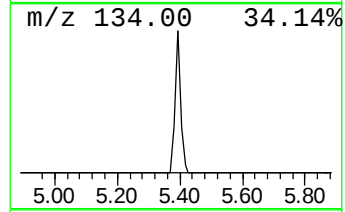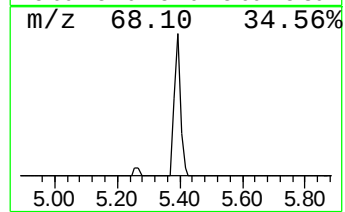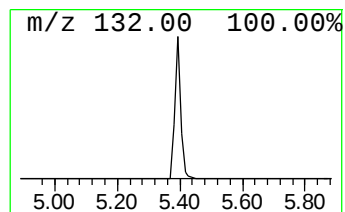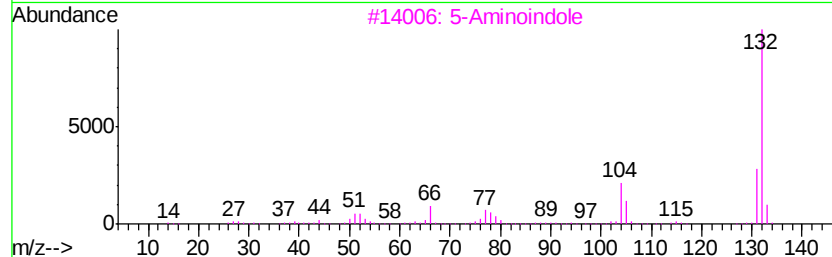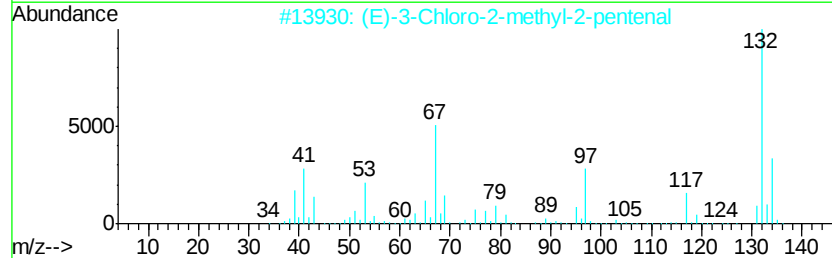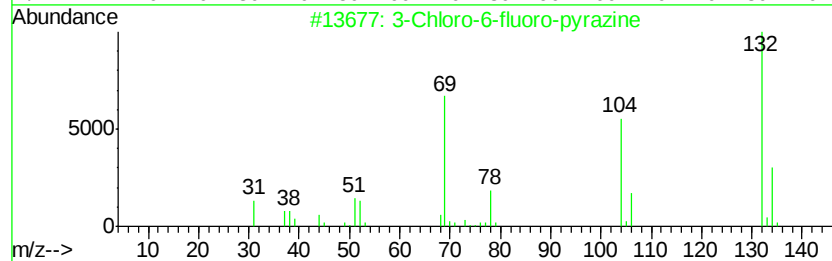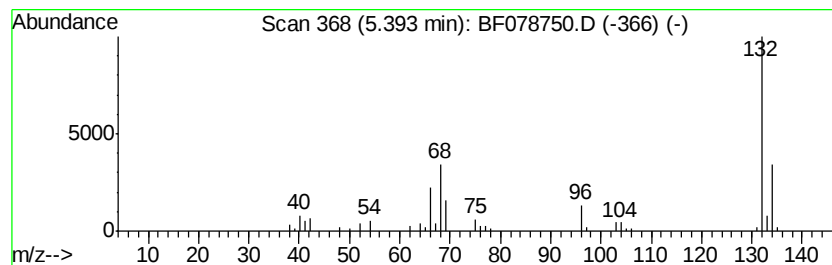

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042315\
Data File : BF078750.D
Acq On : 23 Apr 2015 15:57
Operator : TP/IZ
Sample : G1938-17 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-79S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.39	5.39	19.3	ng	99543	1	5.76	102981	20.0