
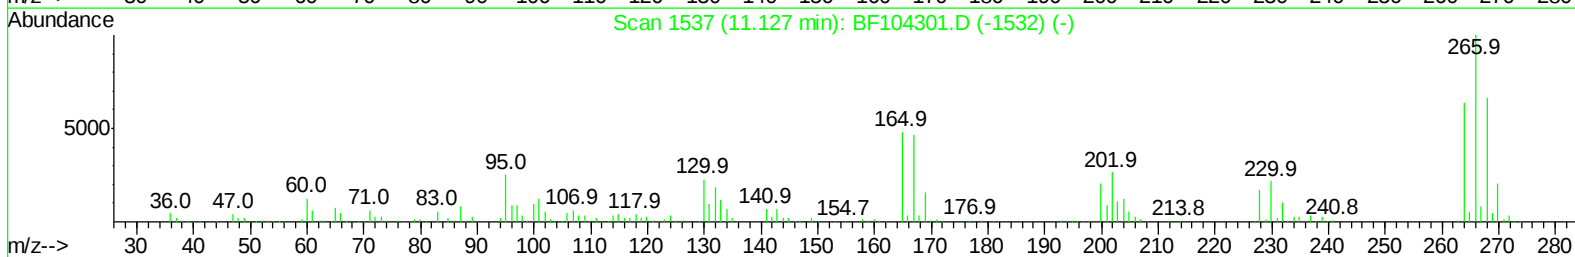
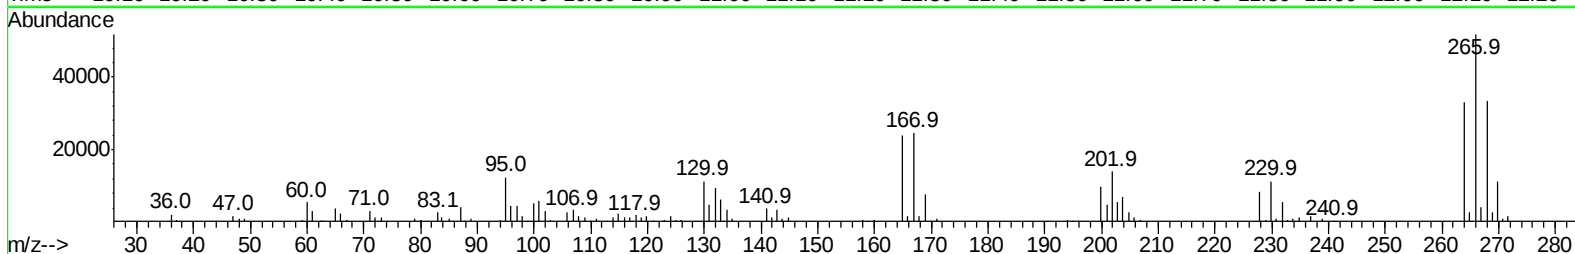


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042318\  
Data File : BF104698.D  
Acq On : 23 Apr 2018 9:38  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:23:50 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Apr 23 15:38:25 2018  
Response via : Initial Calibration

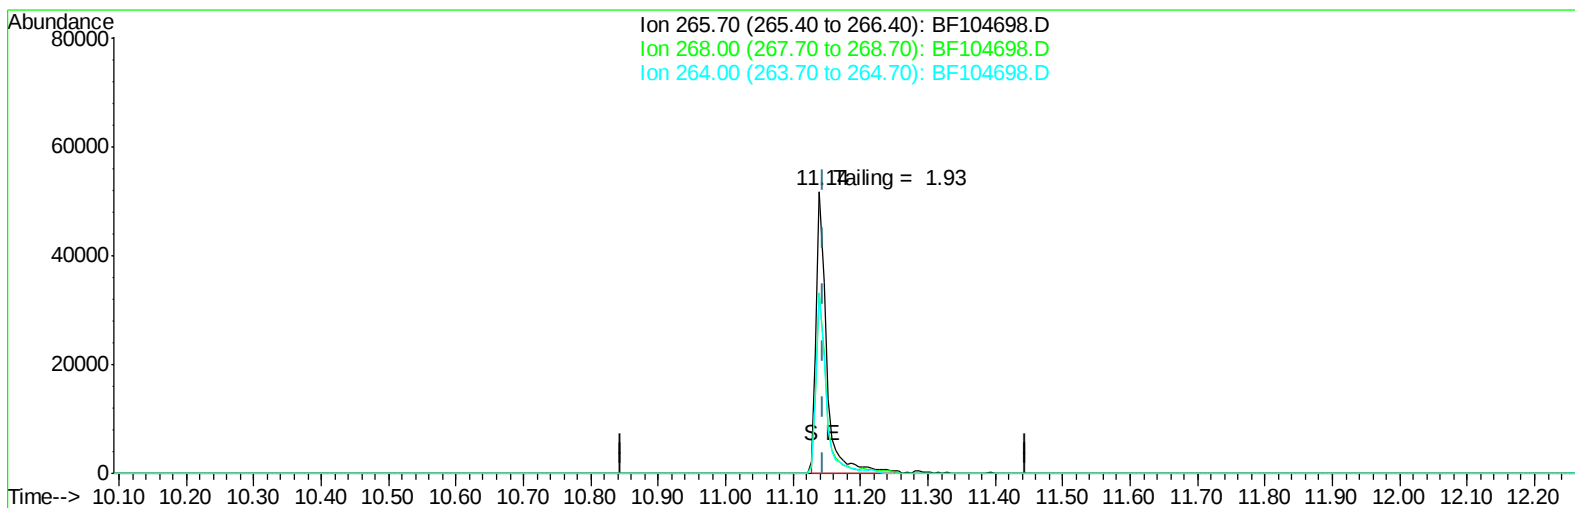

TIC: BF104698.D

(69) Pentachlorophenol (C)




11.139min (-0.006) 37574.83ng

response 54531

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 64.33 |
| 264.00 | 61.90 | 63.89 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042318\  
 Data File : BF104698.D  
 Acq On : 23 Apr 2018 9:38  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:23:50 2018  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Apr 23 15:38:25 2018  
 Response via : Initial Calibration

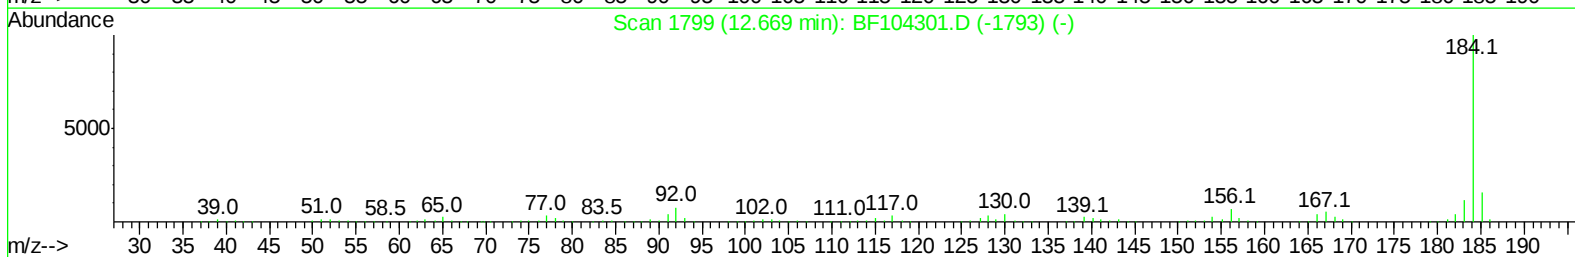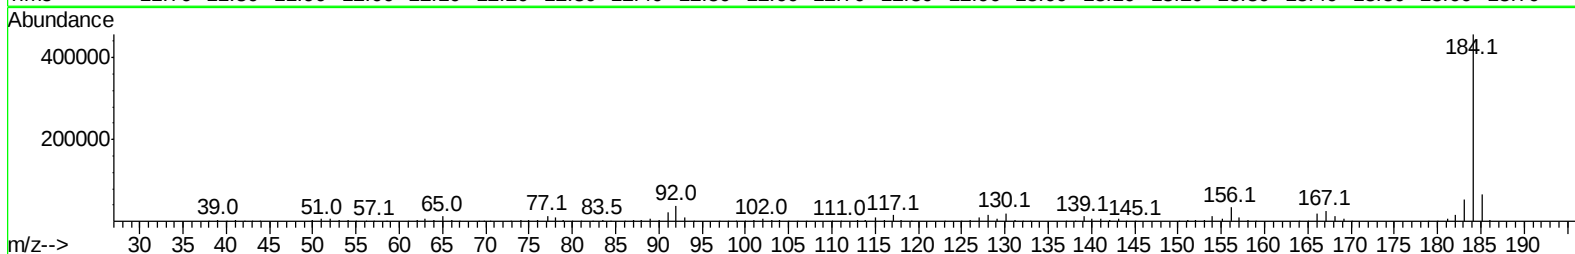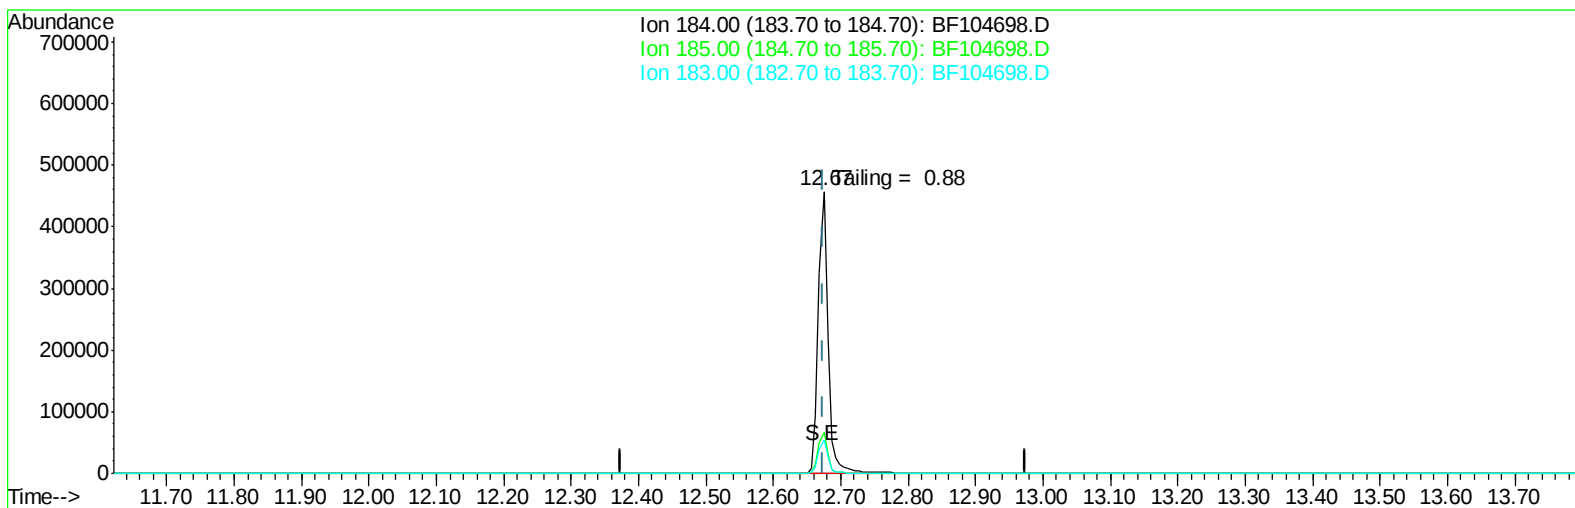

TIC: BF104698.D

(76) Benzidine

12.674min (-0.000) 0.00ng

response 440455

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.43 |
| 183.00 | 11.60 | 12.03 |
| 0.00   | 0.00  | 0.00  |