


Data Path : Z:\HPCHEM1\BNA F\Data\BF042318\
 Data File : BF104698.D
 Acq On : 23 Apr 2018 9:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 23 15:38:25 2018

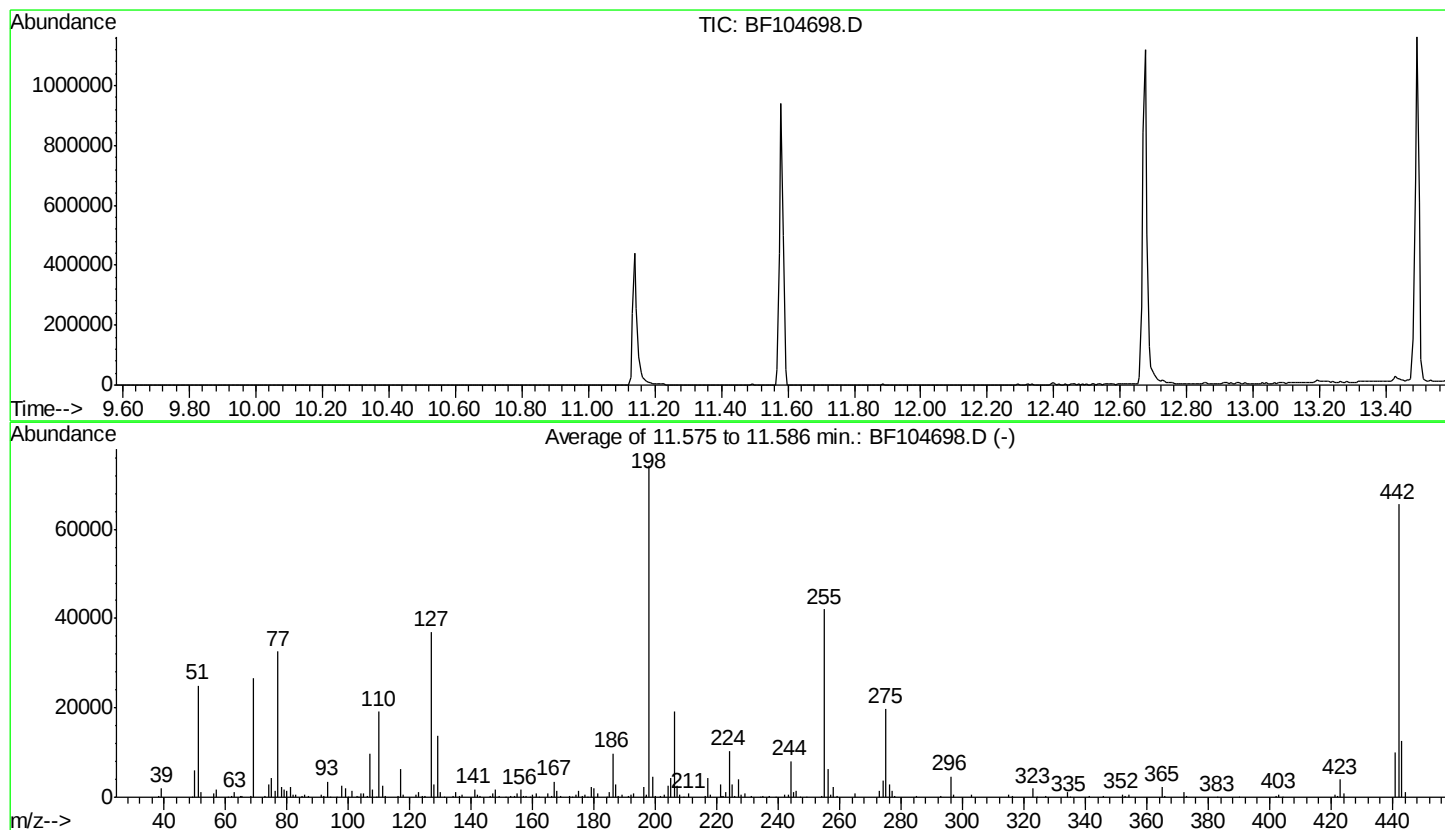

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	25017	PASS
68	69	0.00	2	1.6	419	PASS
69	198	0.00	100	35.8	26555	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	36989	PASS
197	198	0.00	2	0.7	551	PASS
198	198	100	100	100.0	74229	PASS
199	198	5	9	6.4	4718	PASS
275	198	10	60	26.8	19857	PASS
365	198	1	100	3.2	2386	PASS
441	443	0.01	100	80.6	10155	PASS
442	198	50	100	88.3	65576	PASS
443	442	15	24	19.2	12603	PASS