


Data Path : Z:\HPCHEM1\BNA F\Data\BF042318\
 Data File : BF104724.D
 Acq On : 23 Apr 2018 23:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 23 15:38:25 2018

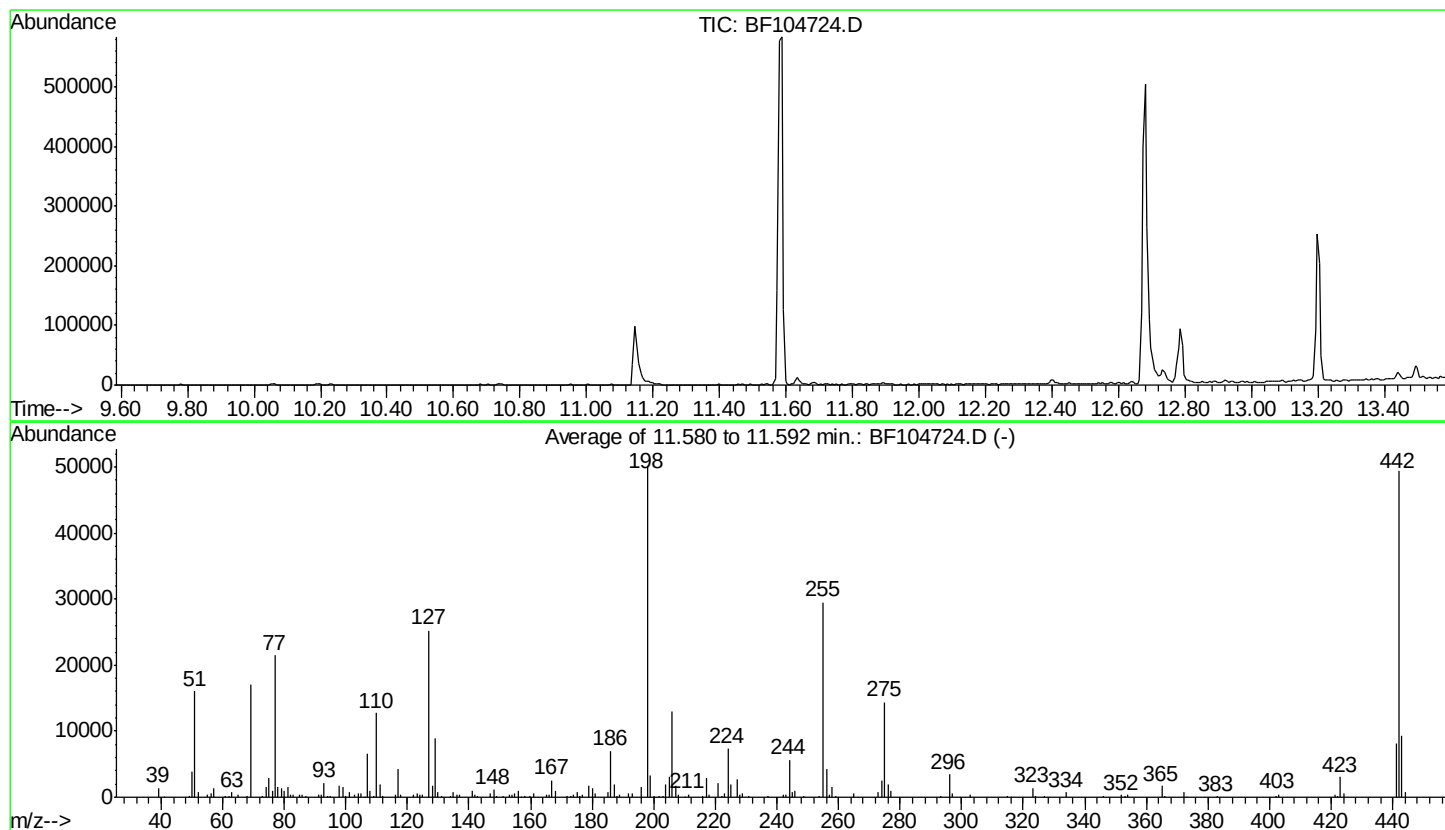

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	16020	PASS
68	69	0.00	2	1.5	256	PASS
69	198	0.00	100	33.8	16992	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	25210	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50201	PASS
199	198	5	9	6.6	3293	PASS
275	198	10	60	28.7	14422	PASS
365	198	1	100	3.5	1735	PASS
441	443	0.01	100	86.6	8124	PASS
442	198	50	100	98.3	49362	PASS
443	442	15	24	19.0	9379	PASS