

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042319\
 Data File : BF113944.D
 Acq On : 24 Apr 2019 2:46
 Operator : JU/SJ
 Sample : K2526-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 24 05:19:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 03:32:35 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	125001	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	407507	20.00	ng	0.00
39) Acenaphthene-d10	9.93	164	175442	20.00	ng	0.00
64) Phenanthrene-d10	11.42	188	336085	20.00	ng	0.00
76) Chrysene-d12	14.05	240	372440	20.00	ng	-0.02
87) Perylene-d12	15.53	264	307271	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	760192	104.02	ng	0.02
7) Phenol-d6	6.53	99	817704	89.18	ng	0.00
23) Nitrobenzene-d5	7.46	82	626991	95.00	ng	0.00
42) 2,4,6-Tribromophenol	10.72	330	280392	131.19	ng	0.00
45) 2-Fluorobiphenyl	9.25	172	1132634	100.97	ng	0.00
79) Terphenyl-d14	13.00	244	1456737	80.19	ng	0.00
Target Compounds						
9) Benzaldehyde	6.67	77	19498	Below Cal		82
19) n-Nitroso-di-n-propylamine	7.46	70	83813	14.115 ng	#	78
25) Isophorone	7.46	82	626979	46.427 ng	#	65
51) 2,6-Dinitrotoluene	9.93	165	21995	8.080 ng	#	32
57) 2,4-Dinitrotoluene	9.93	165	21995	6.402 ng	#	29
65) 4,6-Dinitro-2-methylphenol	10.72	198	413	7.535 ng	#	1
67) 4-Bromophenyl-phenylether	10.72	248	17321	4.266 ng	#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042319\
Data File : BF113944.D
Acq On : 24 Apr 2019 2:46
Operator : JU/SJ
Sample : K2526-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 24 05:19:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 03:32:35 2019
Response via : Initial Calibration

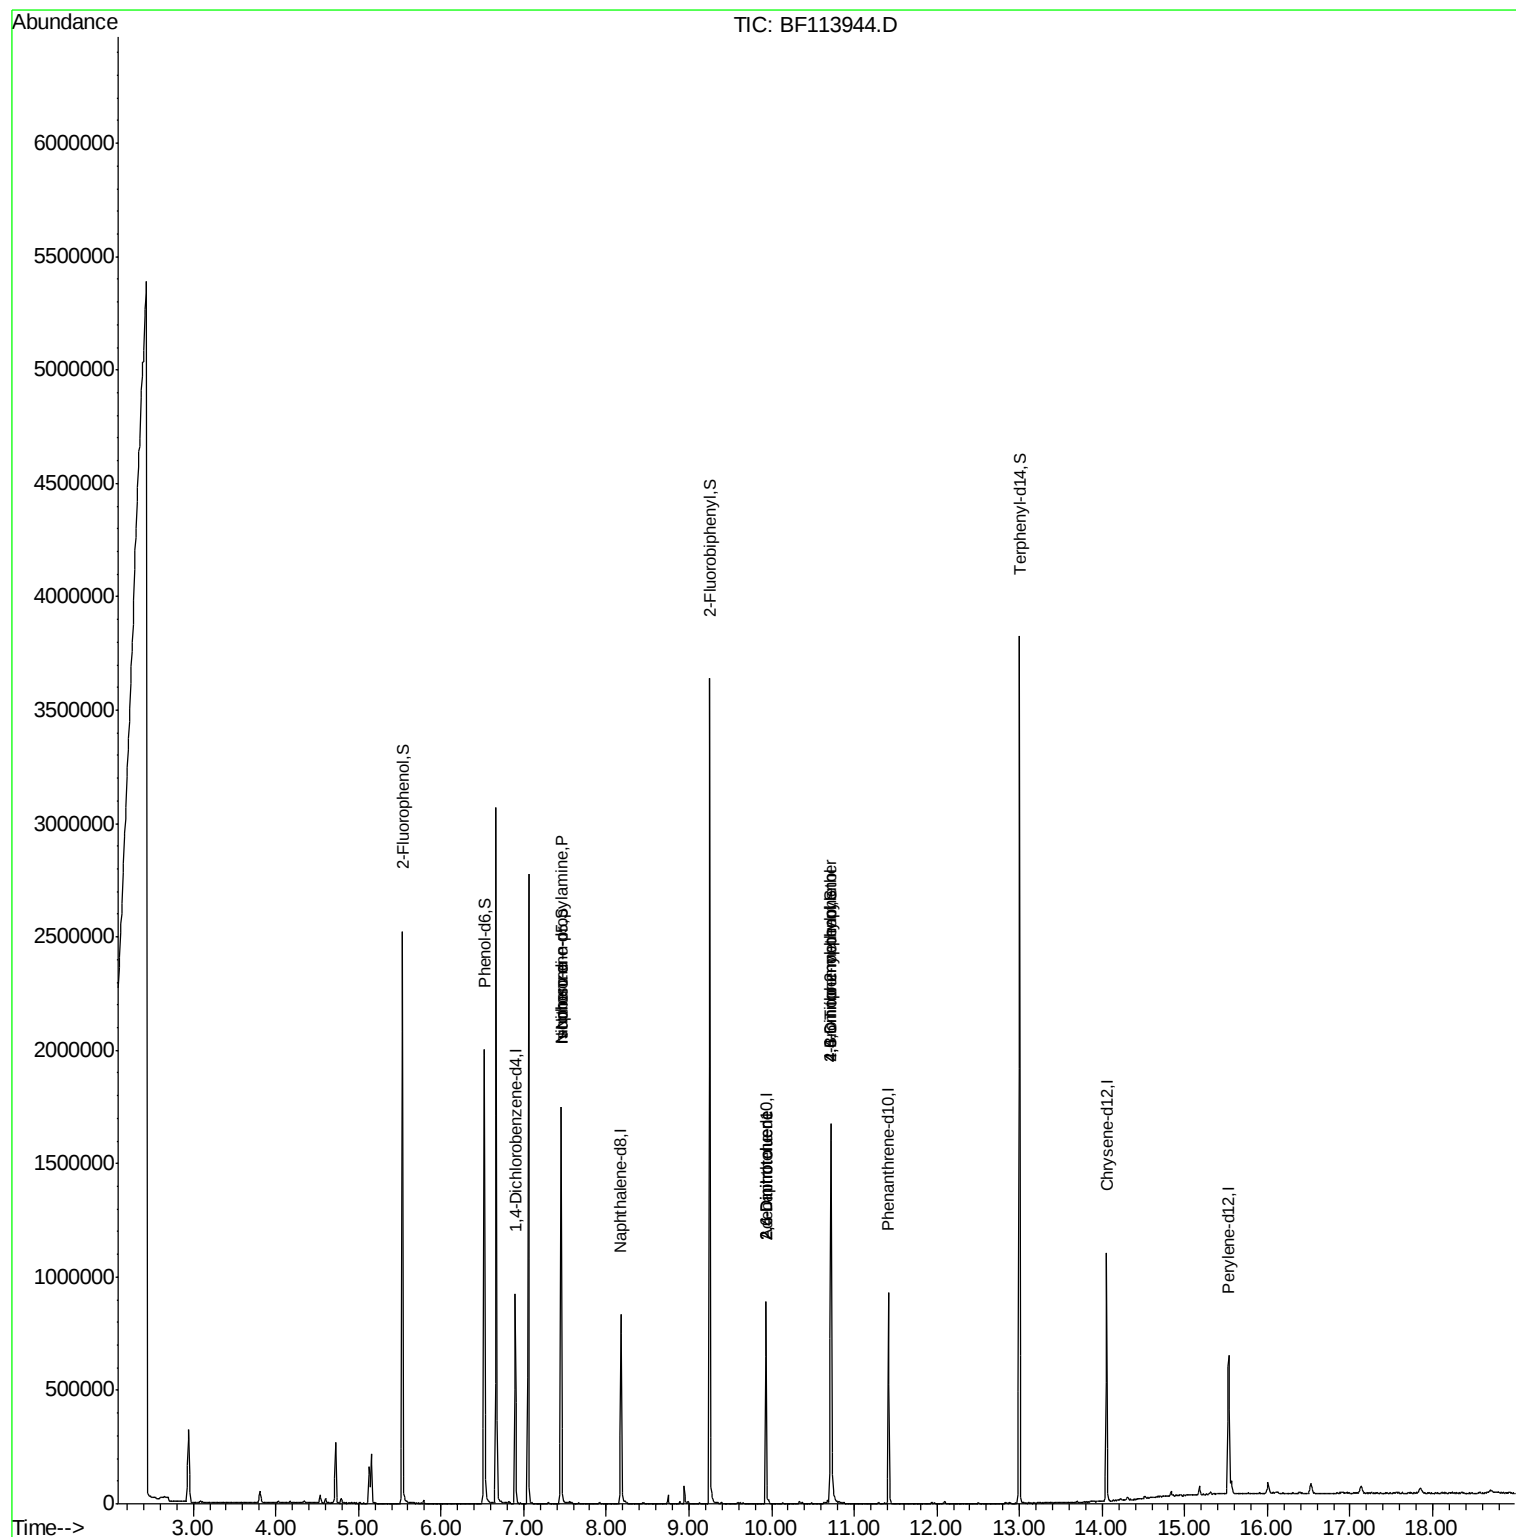

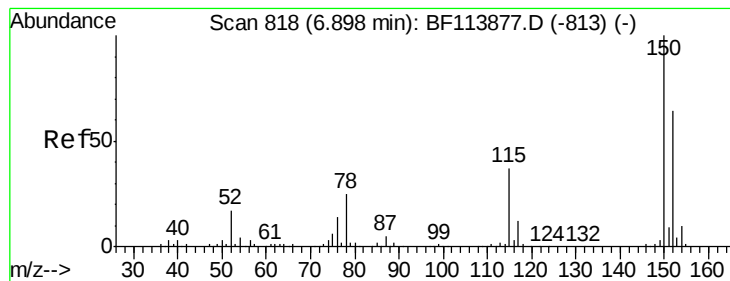


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.90 min Scan# 818
Delta R.T. -0.00 min
Lab File: BF113944.D
Acq: 24 Apr 2019 2:46

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.6	125.9	188.9
115	60.3	45.9	68.9

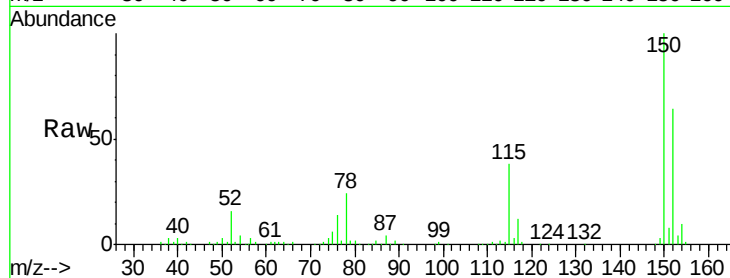


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

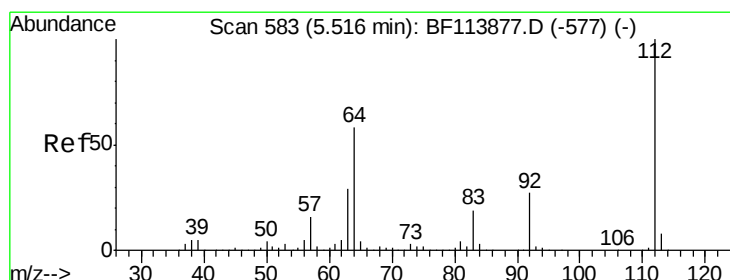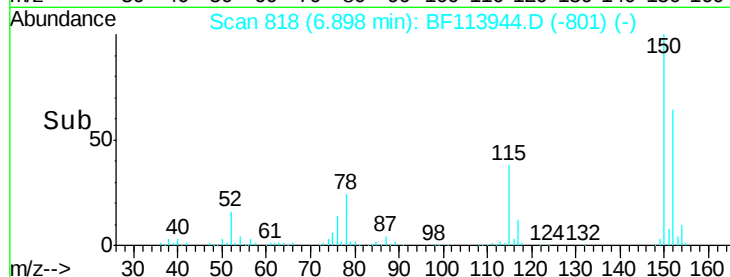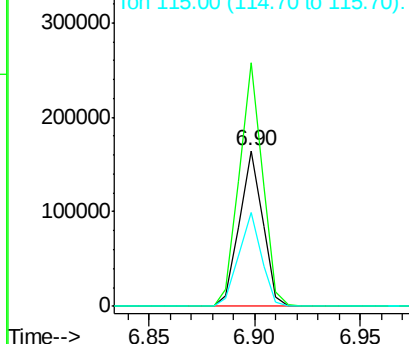



#5


2-Fluorophenol
Concen: 104.015 ng
RT: 5.53 min Scan# 586
Delta R.T. 0.02 min
Lab File: BF113944.D
Acq: 24 Apr 2019 2:46

Tgt Ion	Ratio	Lower	Upper
112	100		
64	56.0	46.6	69.8
63	27.7	23.1	34.7

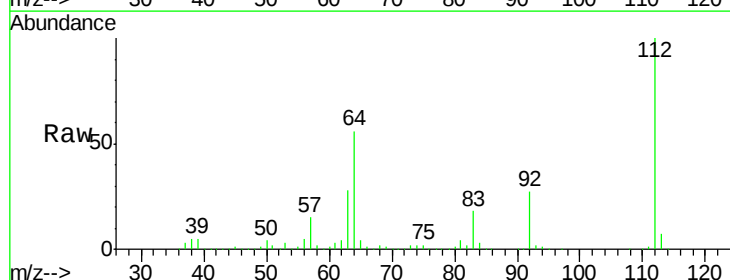

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

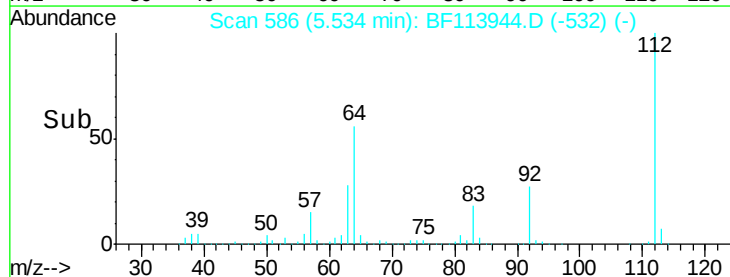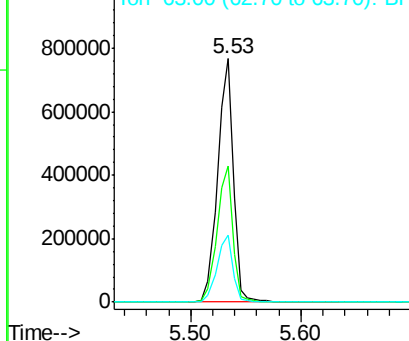

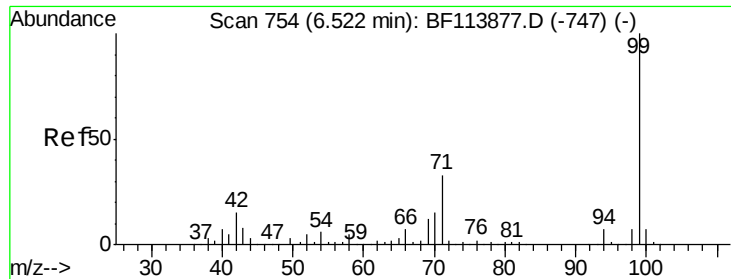

#7

Phenol-d6

Concen: 89.178 ng

RT: 6.53 min Scan# 755

Delta R.T. 0.01 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 817704

Ion Ratio Lower Upper

99 100

42 14.1 12.5 18.7




71 32.6 26.9 40.3



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

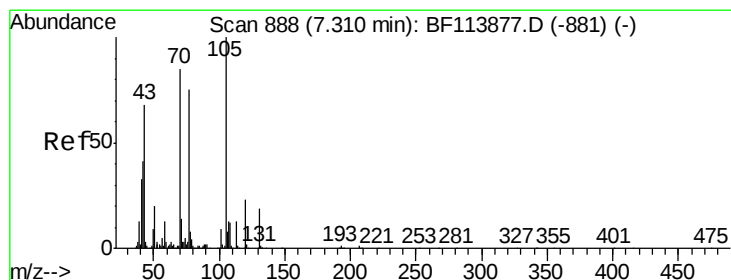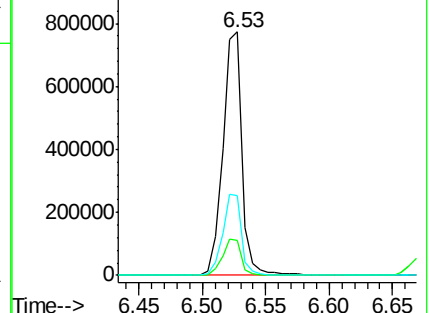

#19

n-Nitroso-di-n-propylamine

Concen: 14.115 ng

RT: 7.46 min Scan# 913

Delta R.T. 0.15 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46

Tgt Ion: 70 Resp: 83813


Ion Ratio Lower Upper

70 100

42 38.8 37.3 55.9

101 0.0 7.8 11.8#

130 2.2 18.2 27.2#






Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

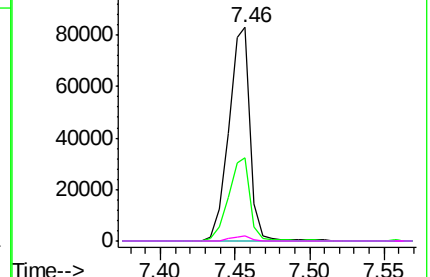

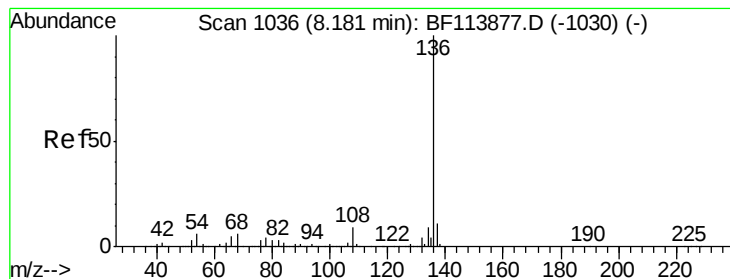

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.17 min Scan# 1035

Delta R.T. -0.01 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 407507



Ion Ratio Lower Upper

136 100

137 10.9 8.6 12.8

54 6.7 5.0 7.6

68 6.4 4.9 7.3

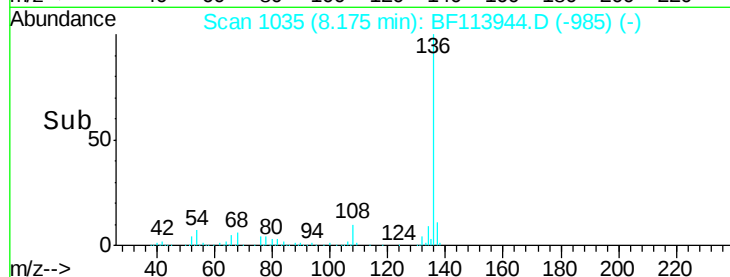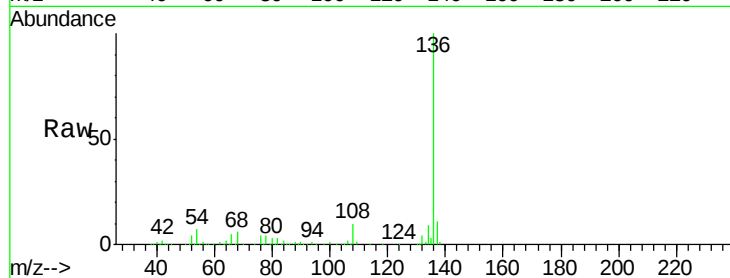


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

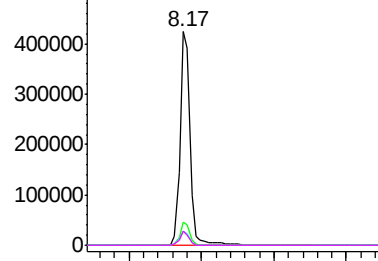

Time-->

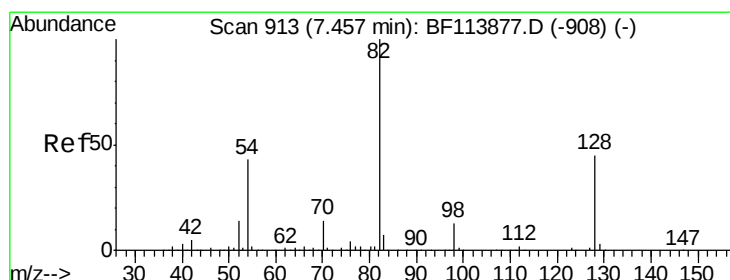

#23

Nitrobenzene-d5

Concen: 94.999 ng

RT: 7.46 min Scan# 913

Delta R.T. -0.00 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46



Tgt Ion: 82 Resp: 626991

Ion Ratio Lower Upper

82 100

128 48.1 36.8 55.2


54 41.6 33.8 50.6

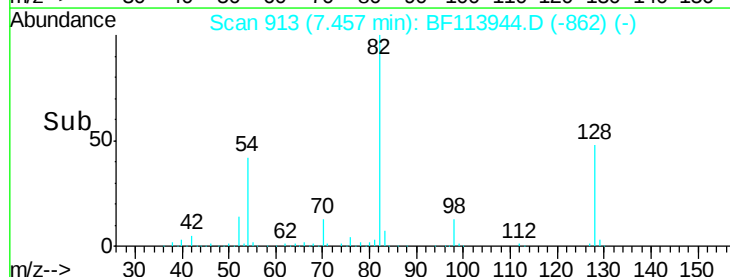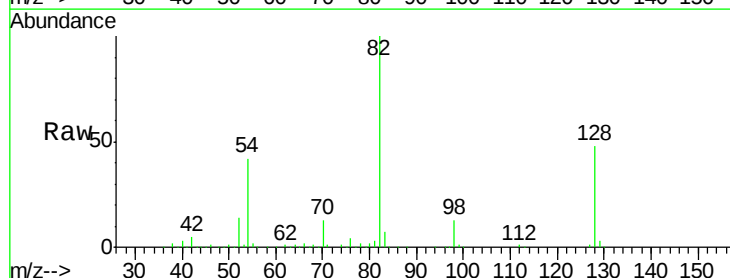


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

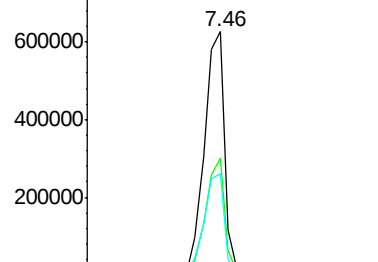

Time-->



#25

Isophorone

Concen: 46.427 ng

RT: 7.46 min Scan# 913

Delta R.T. -0.26 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 626979

Ion Ratio Lower Upper

82 100

95 0.0 5.4 8.2#




138 0.0 14.6 22.0#



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

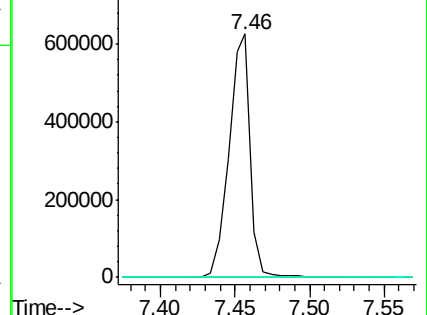

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.93 min Scan# 1334

Delta R.T. -0.00 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46


Tgt Ion:164 Resp: 175442

Ion Ratio Lower Upper

164 100

162 103.0 81.1 121.7



160 44.3 35.8 53.6




Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1



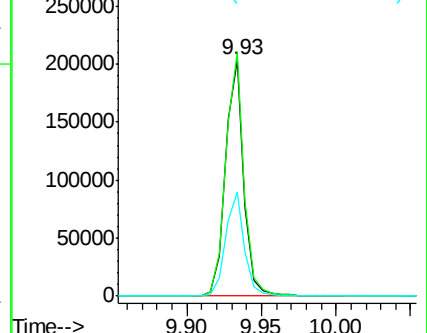





#42
 2,4,6-Tribromophenol
 Concen: 131.193 ng
 RT: 10.72 min Scan# 1468
 Delta R.T. -0.00 min
 Lab File: BF113944.D
 Acq: 24 Apr 2019 2:46




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	77.5	116.3
141	27.2	22.2	33.2

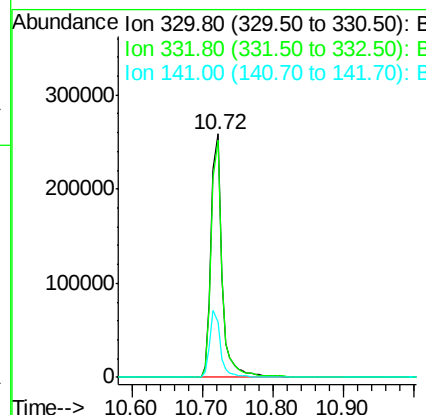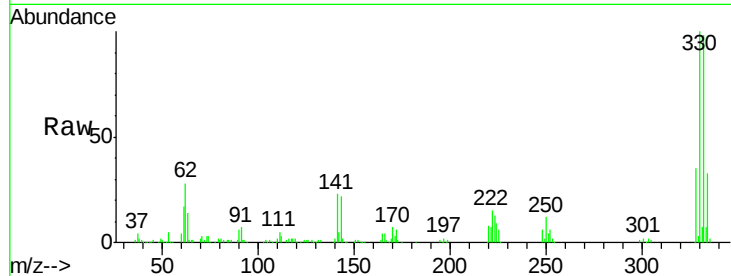

#45
 2-Fluorobiphenyl
 Concen: 100.972 ng
 RT: 9.25 min Scan# 1218
 Delta R.T. -0.01 min
 Lab File: BF113944.D
 Acq: 24 Apr 2019 2:46

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.4	44.0
170	24.0	19.9	29.9


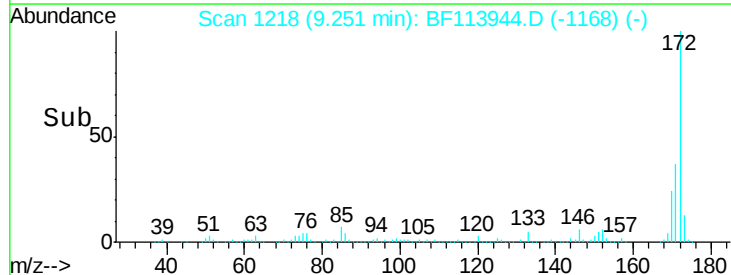
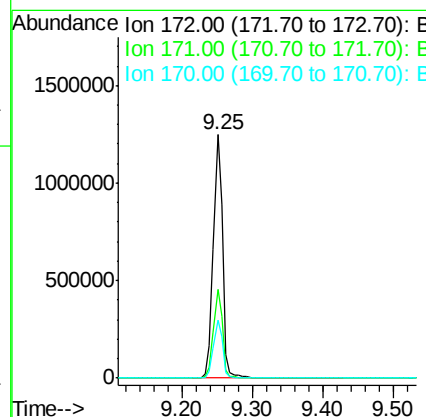



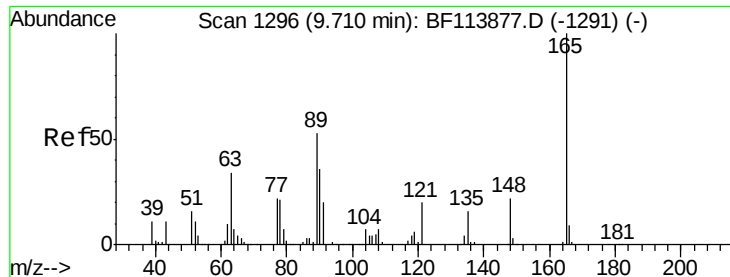

#51
 2,6-Dinitrotoluene
 Concen: 8.080 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. 0.22 min
 Lab File: BF113944.D
 Acq: 24 Apr 2019 2:46




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	33.8	50.8#
89	1.6	38.2	57.2#

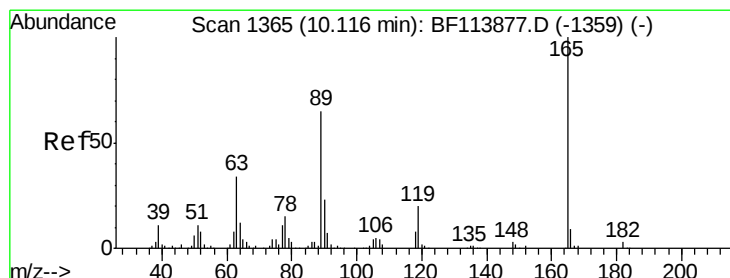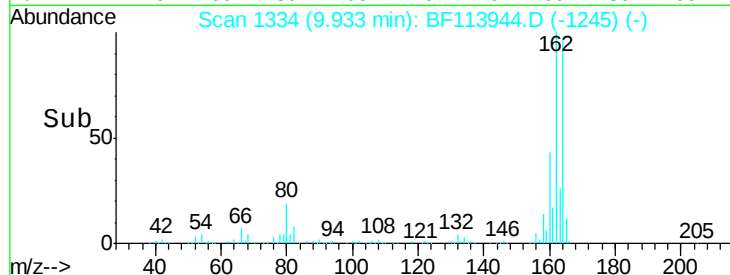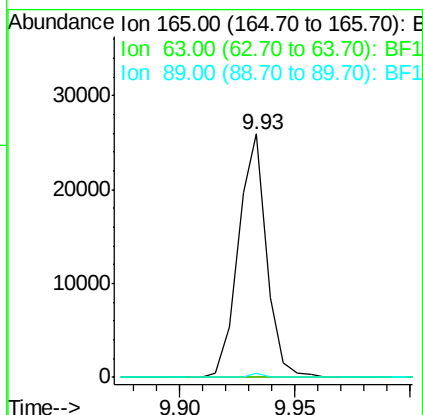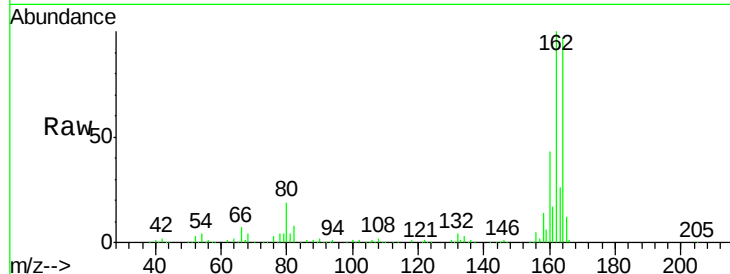

#57
 2,4-Dinitrotoluene
 Concen: 6.402 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. -0.18 min
 Lab File: BF113944.D
 Acq: 24 Apr 2019 2:46

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	27.4	41.0#
89	1.6	51.8	77.6#
182	0.0	2.2	3.2#

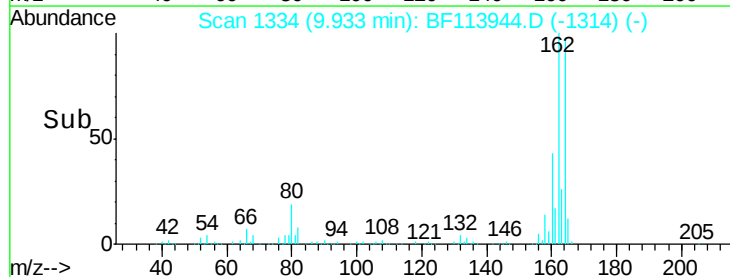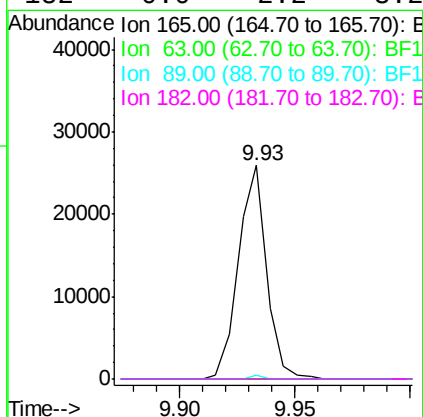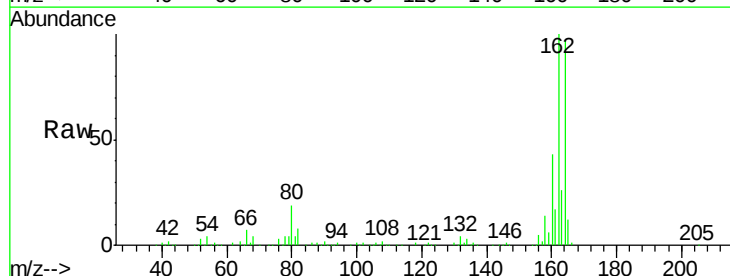



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.42 min Scan# 1586

Delta R.T. -0.00 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion:188 Resp: 336085

Ion Ratio Lower Upper

188 100

94 8.7 8.2 12.4




80 9.6 9.0 13.6



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

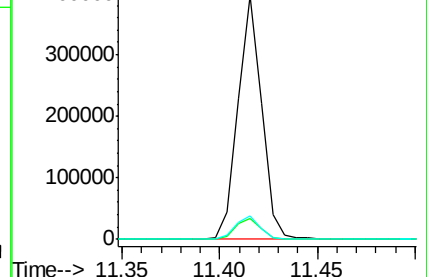

#65

4,6-Dinitro-2-methylphenol

Concen: 7.535 ng

RT: 10.72 min Scan# 1467

Delta R.T. 0.19 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46


Tgt Ion:198 Resp: 413

Ion Ratio Lower Upper

198 100

51 149.2 11.1 51.1#



105 185.3 20.7 60.7#




Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

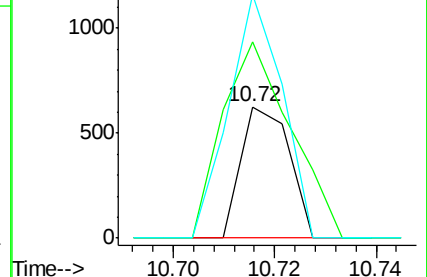


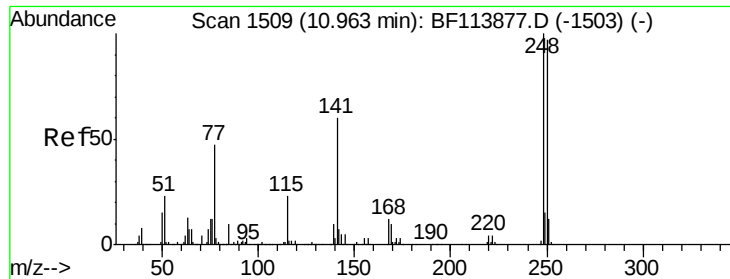




#67
 4-Bromophenyl-phenylether
 Concen: 4.266 ng
 RT: 10.72 min Scan# 1467
 Delta R.T. -0.25 min
 Lab File: BF113944.D
 Acq: 24 Apr 2019 2:46

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:248 Resp: 17321
 Ion Ratio Lower Upper
 248 100
 250 199.2 75.8 113.6#
 141 454.8 50.2 75.4#

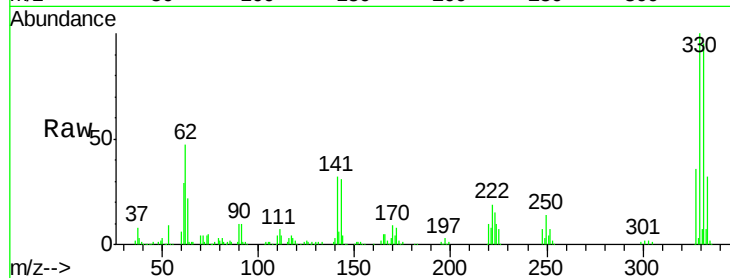


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

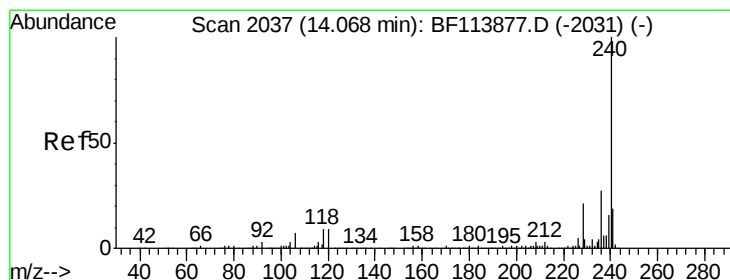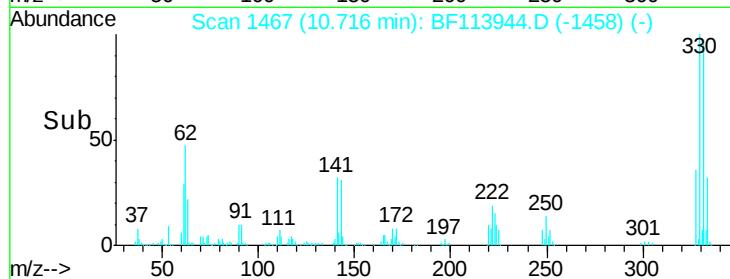
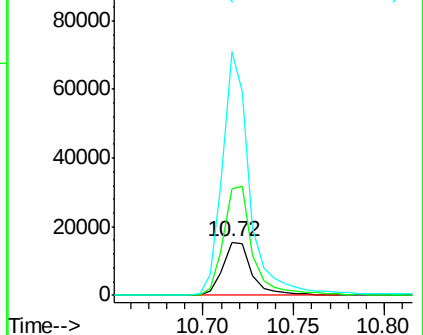



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.05 min Scan# 2034
 Delta R.T. -0.02 min
 Lab File: BF113944.D
 Acq: 24 Apr 2019 2:46

Tgt Ion:240 Resp: 372440
 Ion Ratio Lower Upper
 240 100
 120 10.5 9.3 13.9
 236 26.3 21.2 31.8

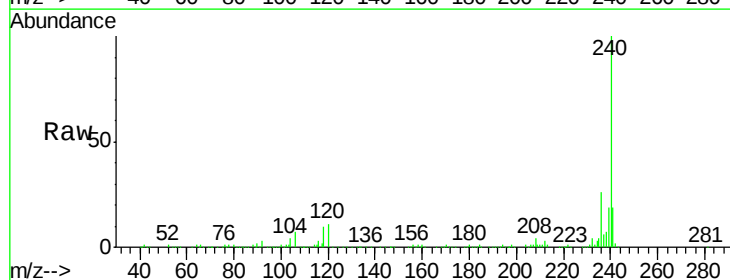

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

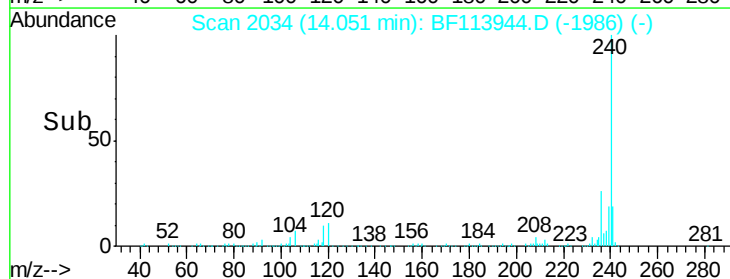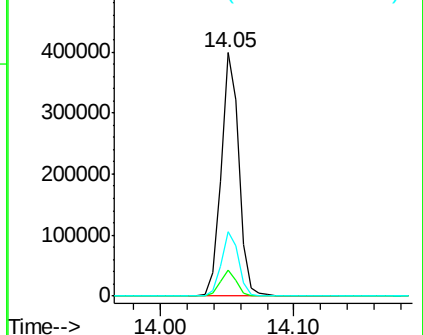

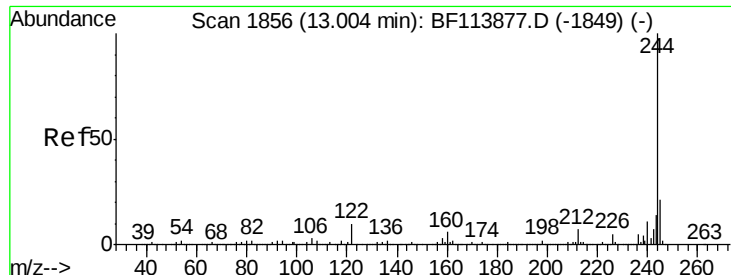

#79

Terphenyl-d14

Concen: 80.188 ng

RT: 13.00 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46


Instrument :

BNA_F

ClientSampleId :

Tot Ion:244 Resp: 1456737

Ion	Ratio	Lower	Upper
244	100		
212	6.8	5.4	8.2
122	10.7	7.6	11.4






Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

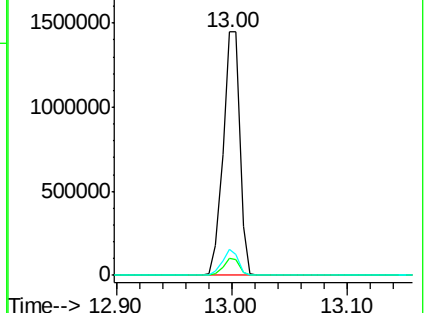

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.53 min Scan# 2286


Delta R.T. -0.04 min

Lab File: BF113944.D

Acq: 24 Apr 2019 2:46

Tgt Ion:264 Resp: 307271

Ion	Ratio	Lower	Upper
264	100		
260	23.9	18.9	28.3
265	20.9	17.3	25.9



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

