


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042319\
 Data File : BF113915.D
 Acq On : 23 Apr 2019 12:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

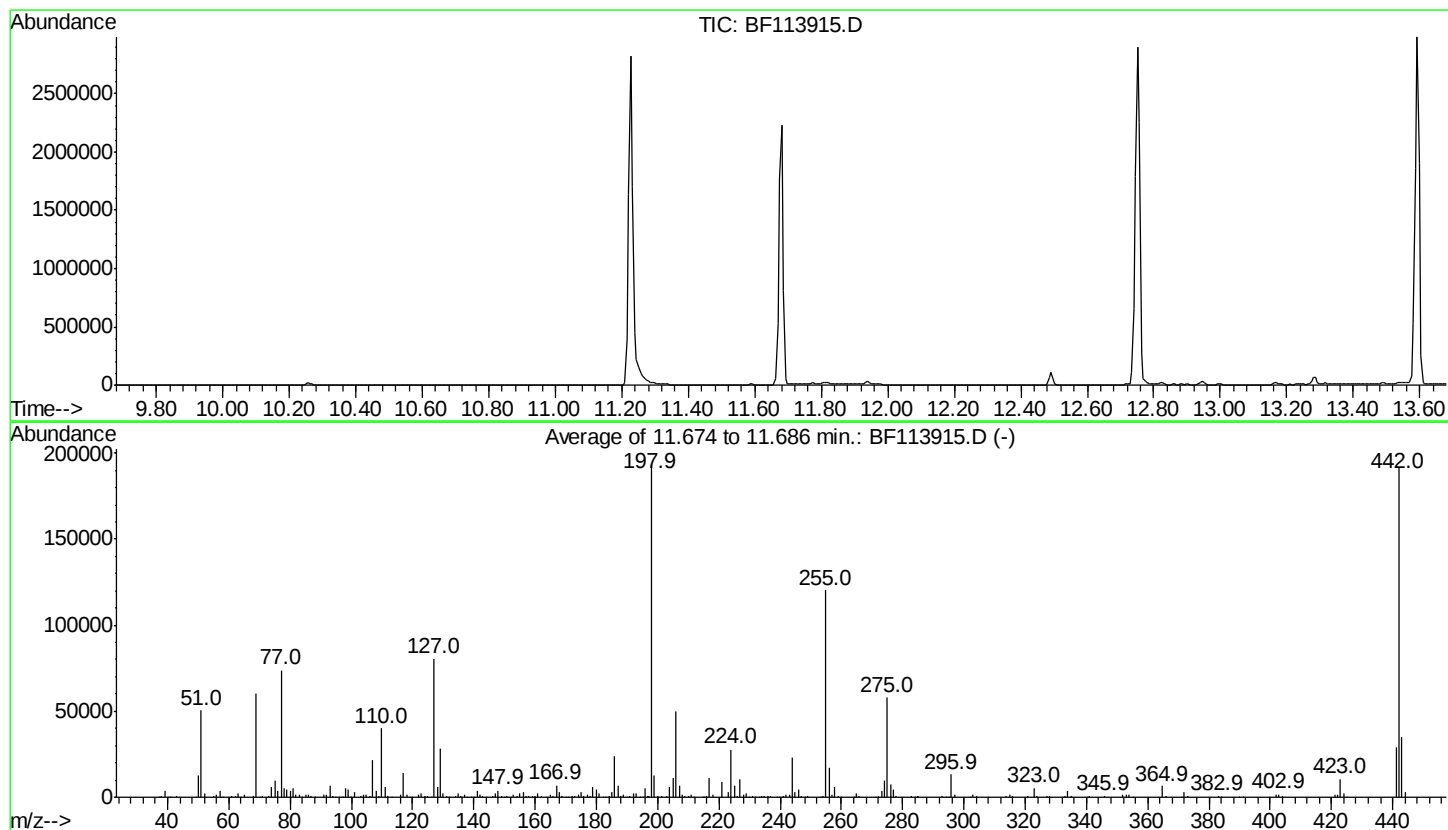

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.2	50438	PASS
68	69	0.00	2	1.6	947	PASS
69	198	0.00	100	31.2	60034	PASS
70	69	0.00	2	0.6	390	PASS
127	198	10	80	41.8	80562	PASS
197	198	0.00	2	0.4	801	PASS
198	198	100	100	100.0	192712	PASS
199	198	5	9	6.6	12739	PASS
275	198	10	60	29.9	57709	PASS
365	198	1	100	3.4	6605	PASS
441	198	0.01	100	15.1	29176	PASS
442	198	50	100	99.6	191936	PASS
443	442	15	24	18.4	35229	PASS