


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042319\
 Data File : BF113940.D
 Acq On : 24 Apr 2019 00:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

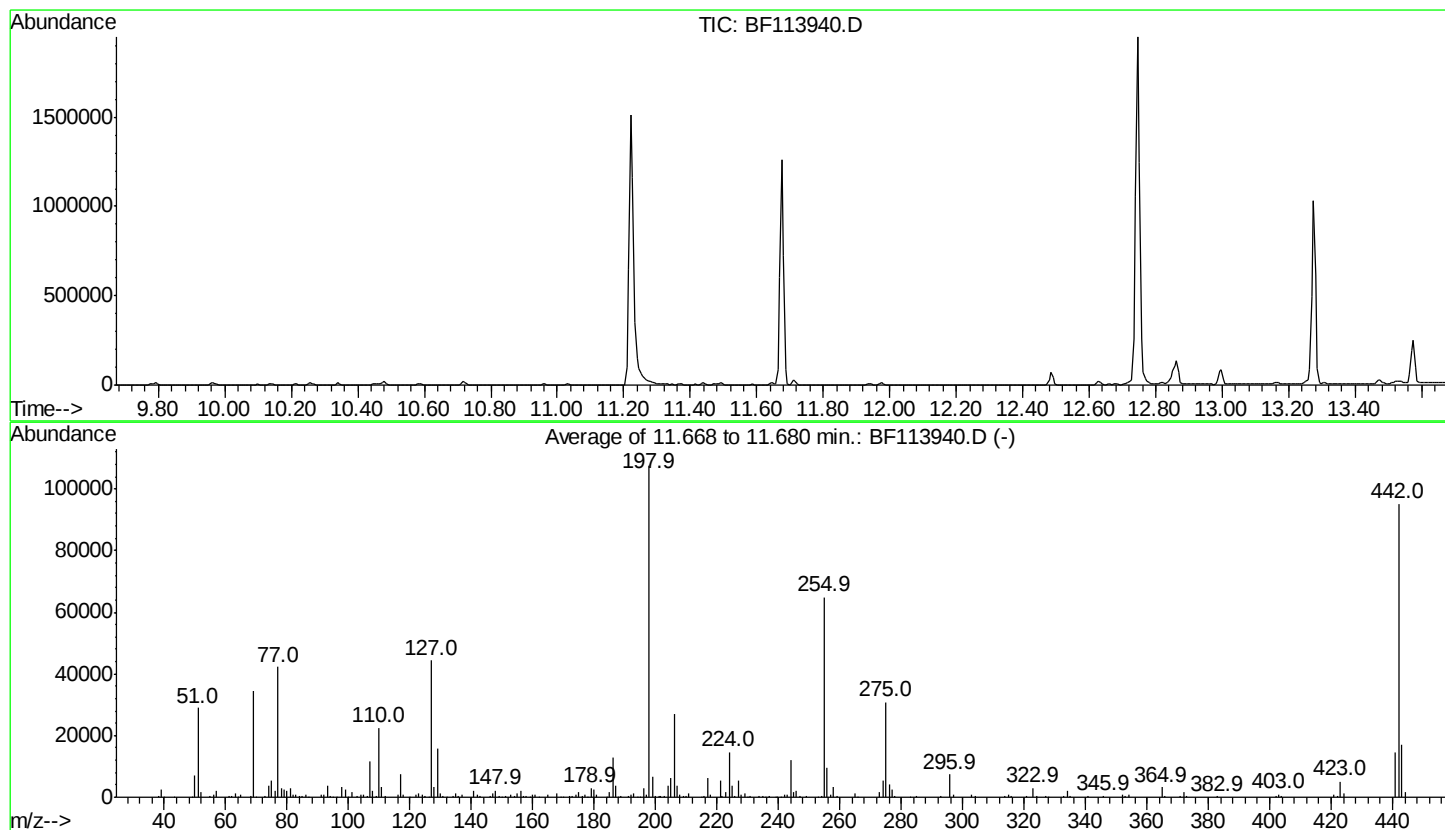

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	28948	PASS
68	69	0.00	2	1.7	577	PASS
69	198	0.00	100	31.9	34314	PASS
70	69	0.00	2	0.4	131	PASS
127	198	10	80	41.3	44370	PASS
197	198	0.00	2	0.7	714	PASS
198	198	100	100	100.0	107546	PASS
199	198	5	9	6.4	6858	PASS
275	198	10	60	28.7	30896	PASS
365	198	1	100	3.0	3278	PASS
441	198	0.01	100	13.6	14586	PASS
442	198	50	100	88.4	95109	PASS
443	442	15	24	18.1	17176	PASS