


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042321\
 Data File : BF123692.D
 Acq On : 23 Apr 2021 13:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 26 05:40:49 2021

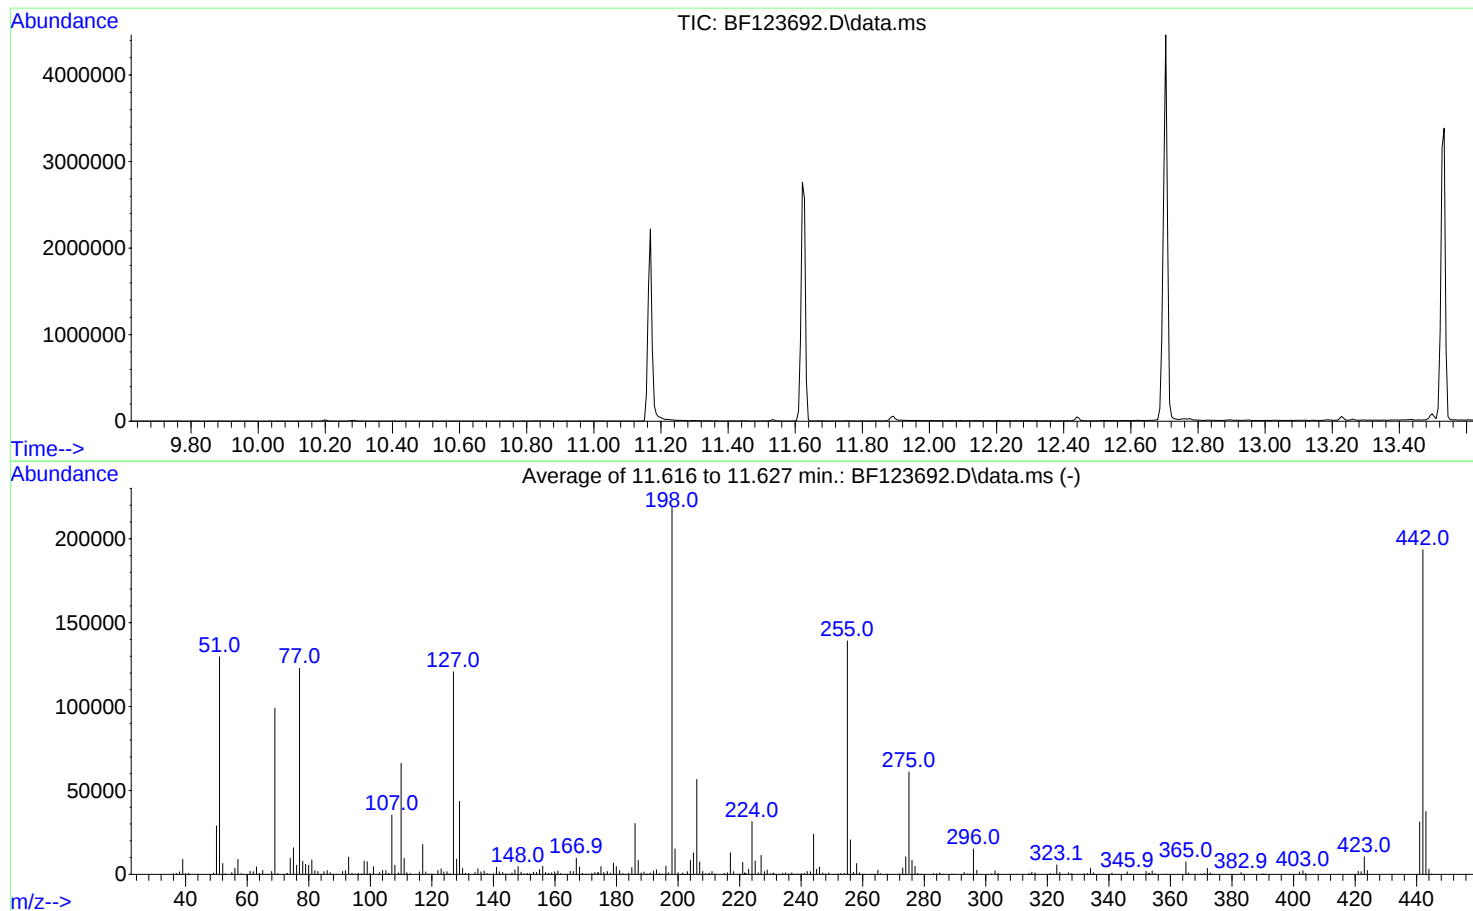




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.2	129723	PASS
68	69	0.00	2	1.7	1689	PASS
69	198	0.00	100	45.2	98997	PASS
70	69	0.00	2	0.5	459	PASS
127	198	10	80	55.1	120757	PASS
197	198	0.00	2	0.5	995	PASS
198	198	100	100	100.0	219235	PASS
199	198	5	9	6.9	15167	PASS
275	198	10	60	27.8	61037	PASS
365	198	1	100	3.4	7439	PASS
441	198	0.01	100	14.3	31258	PASS
442	442	50	100	100.0	193432	PASS
443	442	15	24	19.3	37354	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042321\
 Data File : BF123692.D
 Acq On : 23 Apr 2021 13:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 23 14:04:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 23 10:48:36 2021
 Response via : Initial Calibration

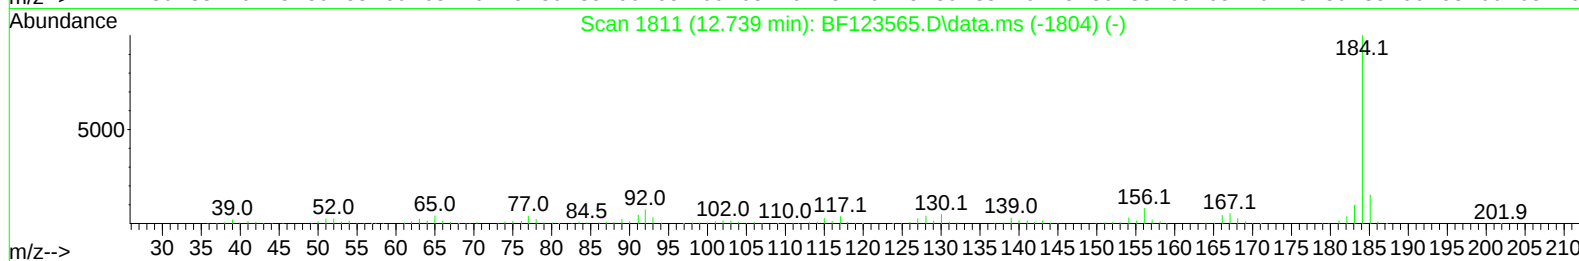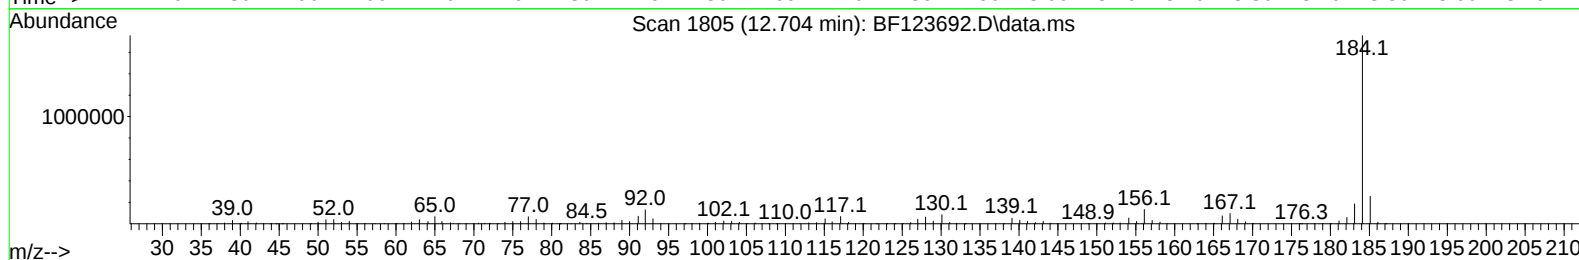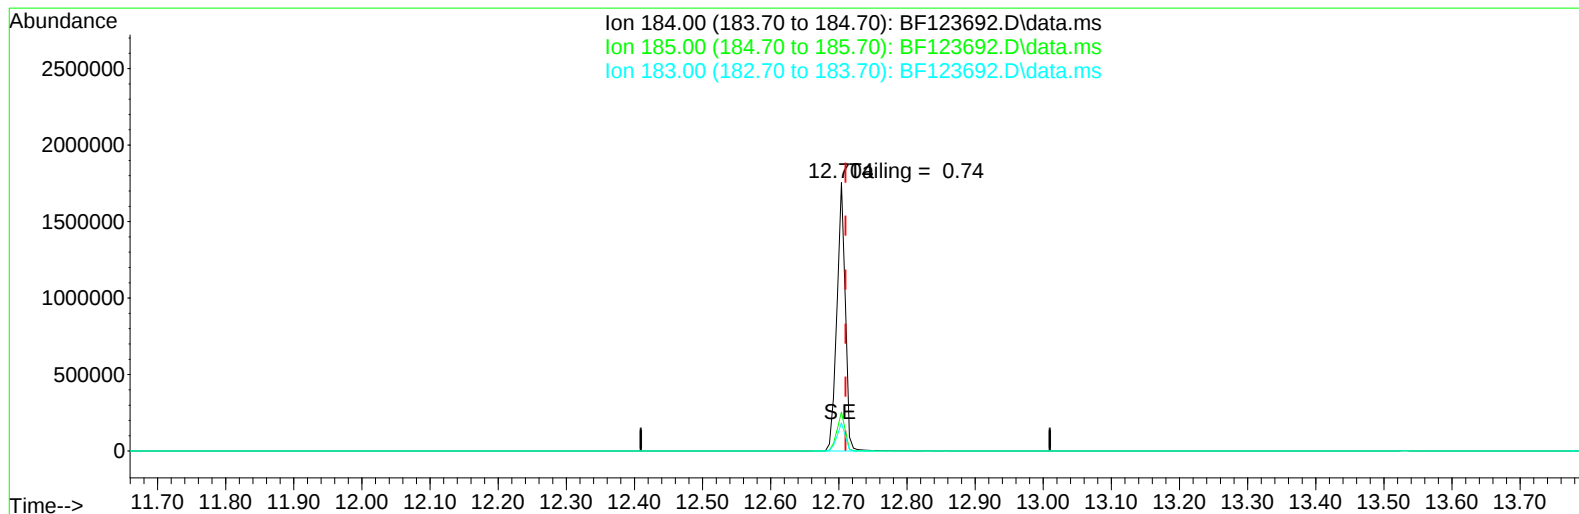

TIC: BF123692.D\data.ms

(77) Benzidine

12.704min (-0.006) 0.00 ng




response 1507660

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.55
183.00	9.80	10.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042321\
Data File : BF123692.D
Acq On : 23 Apr 2021 13:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 23 14:04:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 23 10:48:36 2021
Response via : Initial Calibration

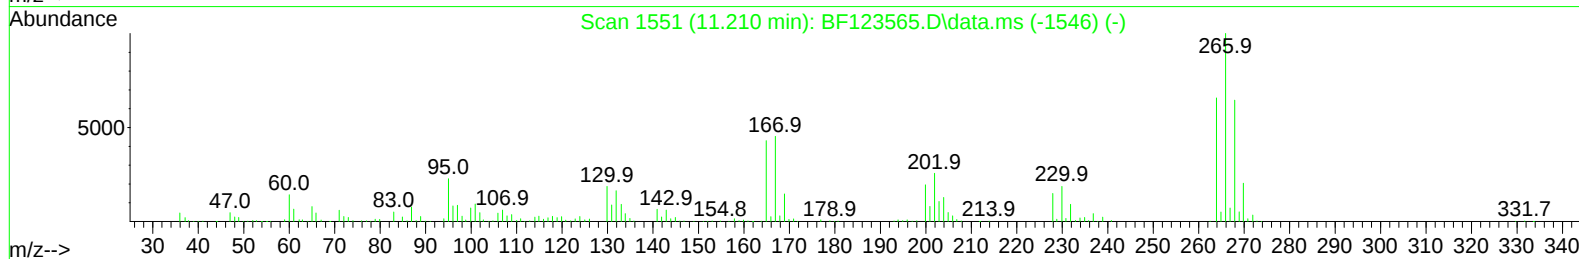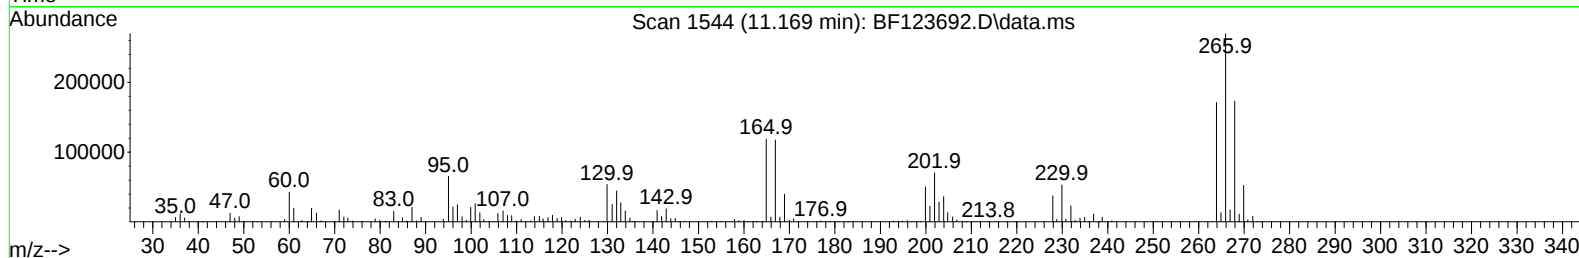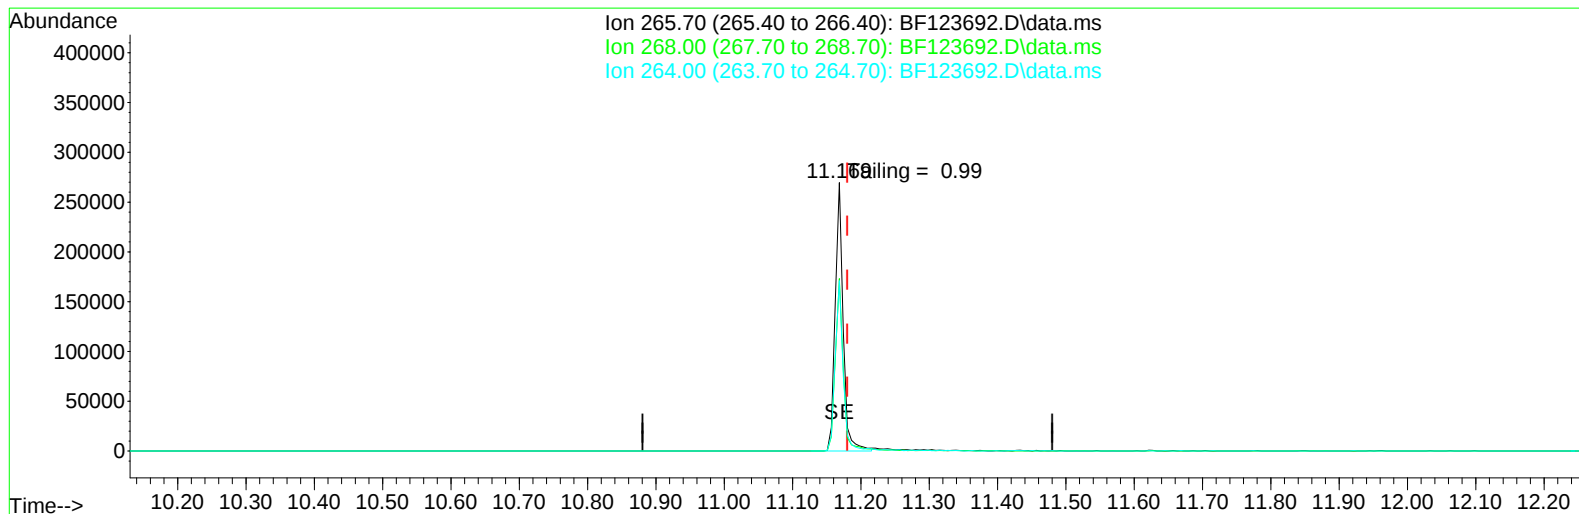

TIC: BF123692.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.012) 33957.13 ng

response 223670

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.25
264.00	65.70	63.46
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/23/2021	BNA_F	<u>BF123692.D</u>
Compound Name	Response	Retention Time
DDT	565159	13.53
DDD	7370	13.22
DDE	993	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8363	573522	1.46