
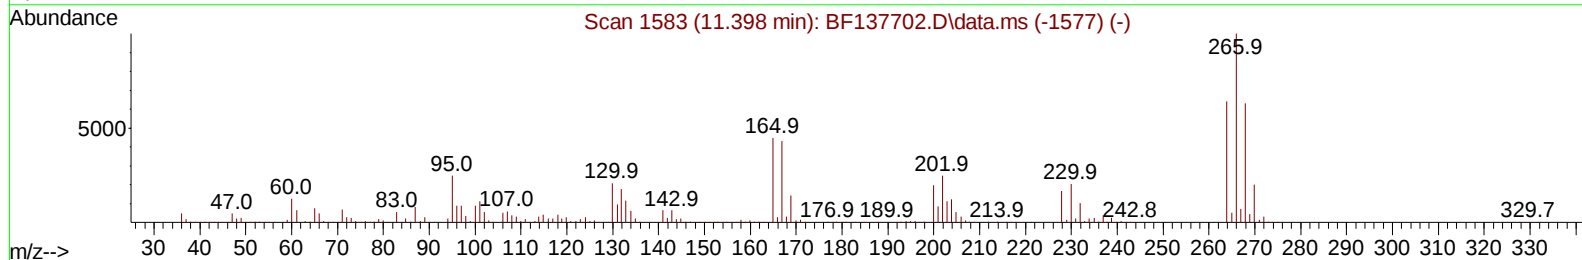
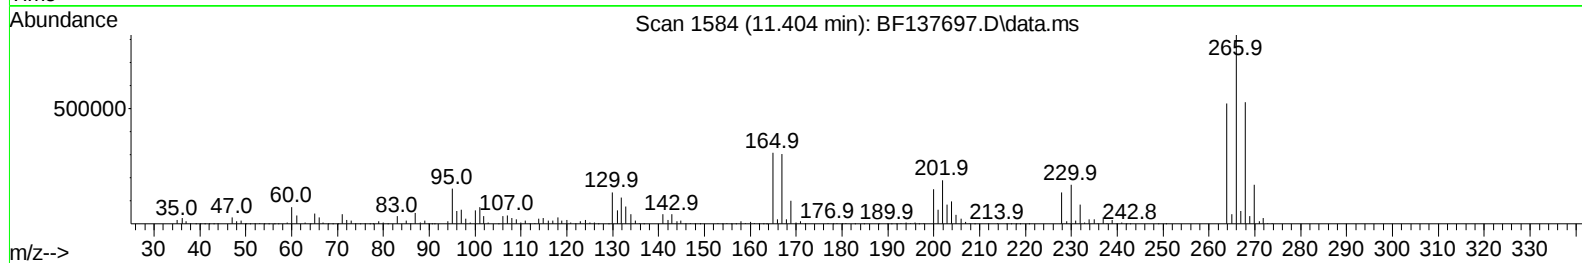


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042324\
Data File : BF137697.D
Acq On : 23 Apr 2024 16:40
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 04:07:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

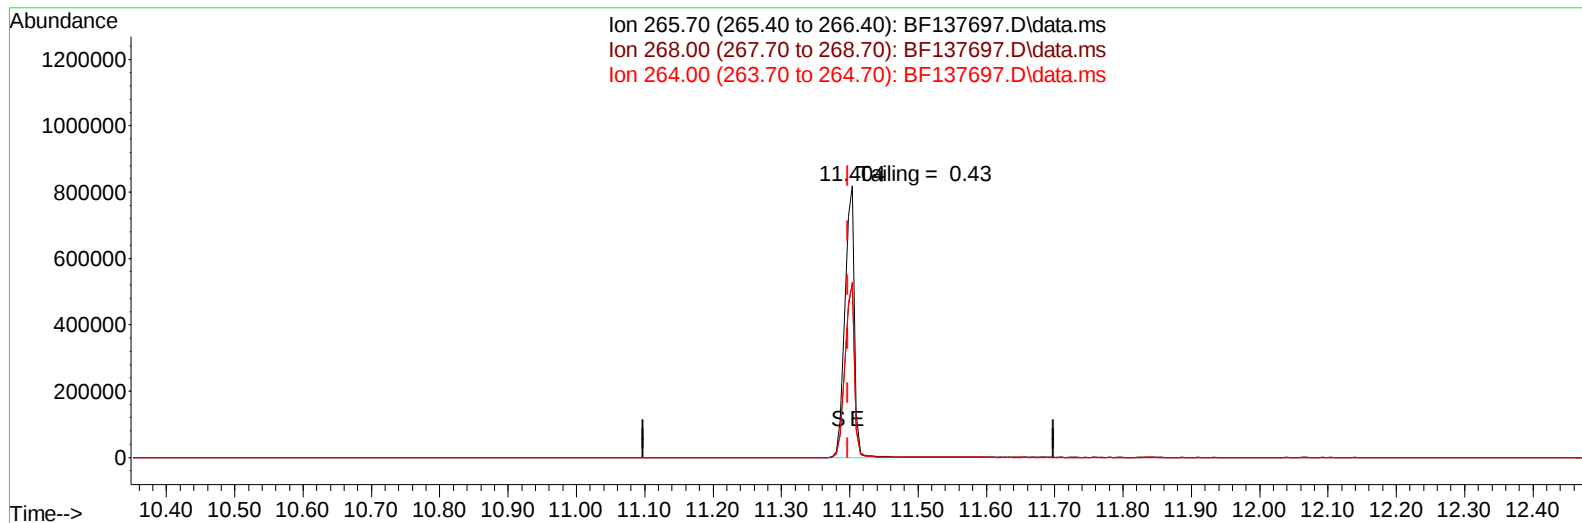

TIC: BF137697.D\data.ms

(70) Pentachlorophenol (C)




11.404min (+ 0.006) 257741.65 ng

response 790110

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.39
264.00	64.20	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042324\
Data File : BF137697.D
Acq On : 23 Apr 2024 16:40
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 04:07:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 03:57:12 2024
Response via : Initial Calibration

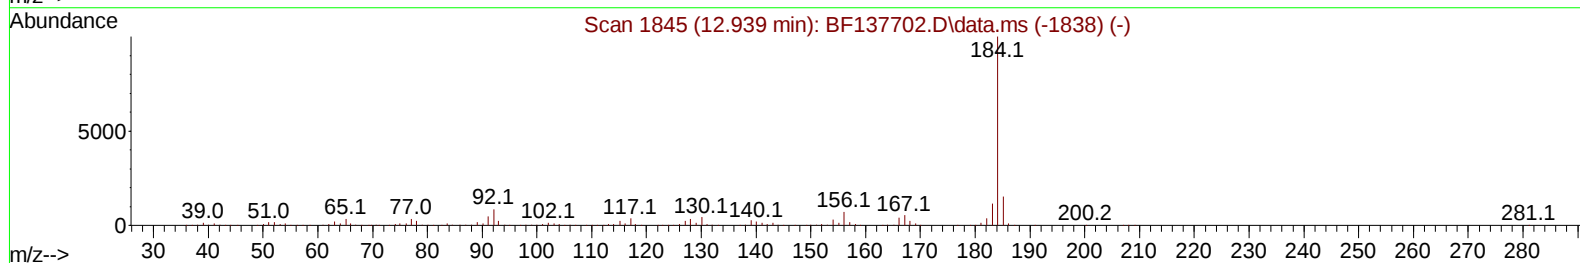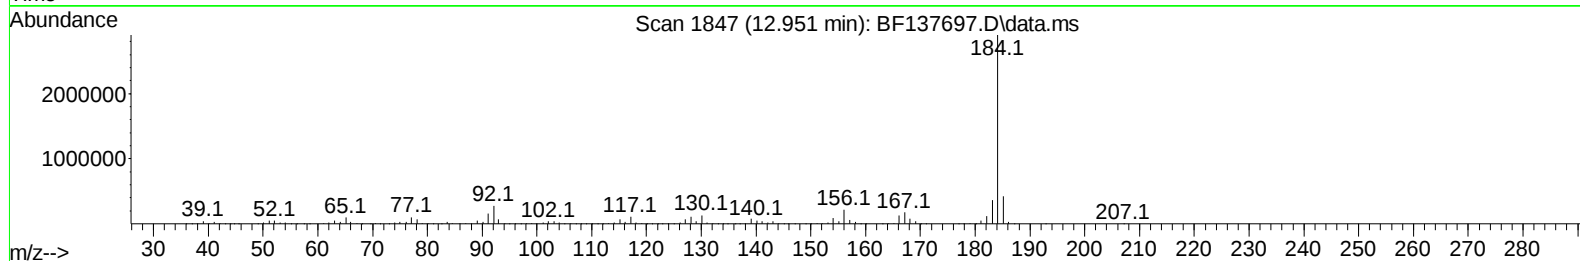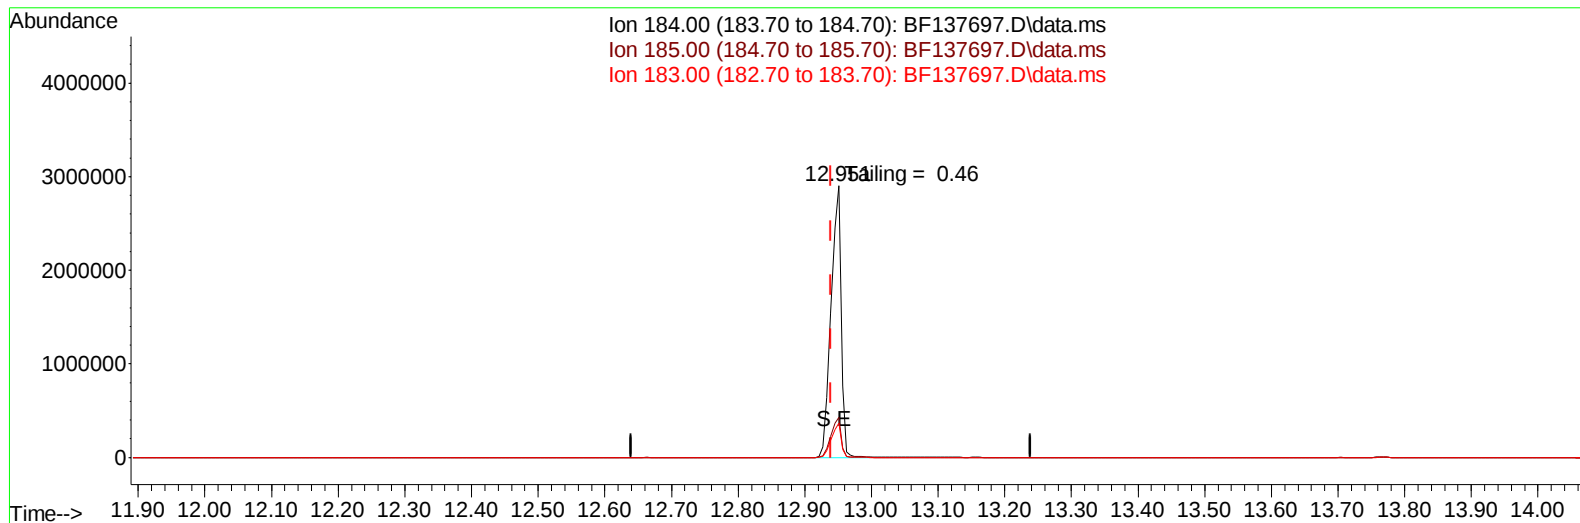

TIC: BF137697.D\data.ms

(77) Benzidine

12.951min (+ 0.012) 7756.72 ng m

response 3031902

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.67
183.00	11.70	12.53
0.00	0.00	0.00