
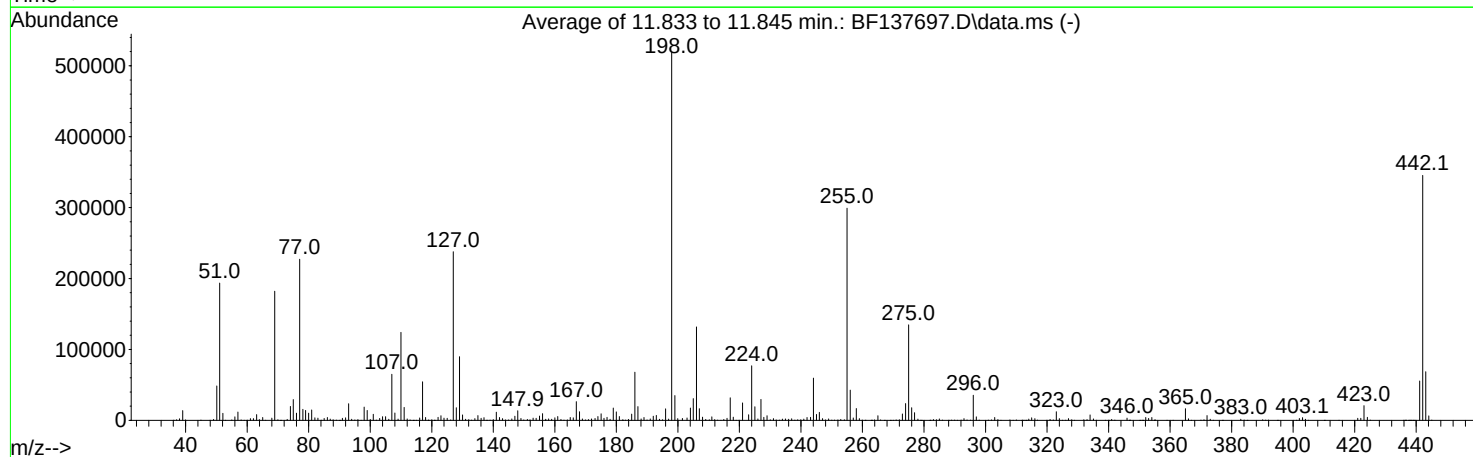


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042324\  
Data File : BF137697.D  
Acq On : 23 Apr 2024 16:40  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042324.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Apr 24 03:57:12 2024

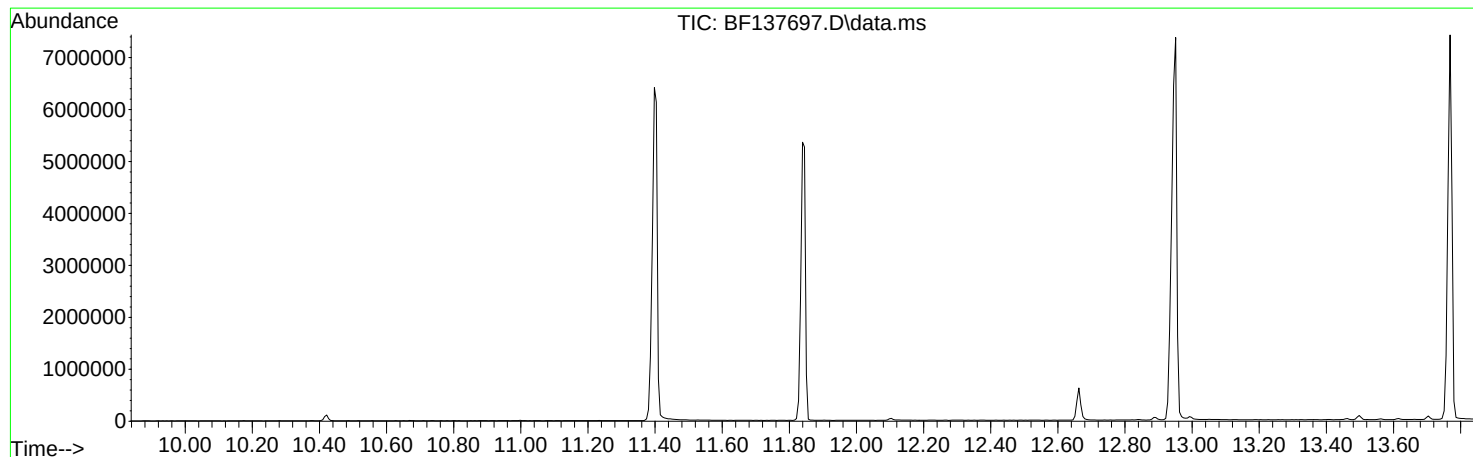




AutoFind: Scans 1657, 1658, 1659; Background Corrected with Scan 1651

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 37.3         | 193627     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 3097       | PASS                |
| 69             | 198             | 0.00            | 100             | 35.1         | 182039     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 1002       | PASS                |
| 127            | 198             | 10              | 80              | 45.8         | 237760     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 1798       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 518741     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 34885      | PASS                |
| 275            | 198             | 10              | 60              | 26.0         | 134661     | PASS                |
| 365            | 198             | 1               | 100             | 3.2          | 16467      | PASS                |
| 441            | 198             | 0.01            | 100             | 10.7         | 55599      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 345475     | PASS                |
| 443            | 442             | 15              | 24              | 19.9         | 68605      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042324\  
Data File : BF137697.D  
Acq On : 23 Apr 2024 16:40  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Apr 24 04:07:40 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 24 03:57:12 2024  
Response via : Initial Calibration

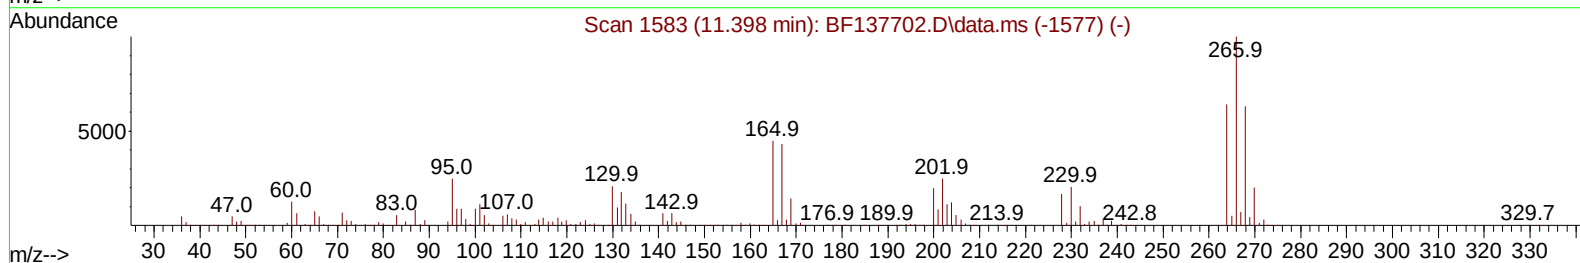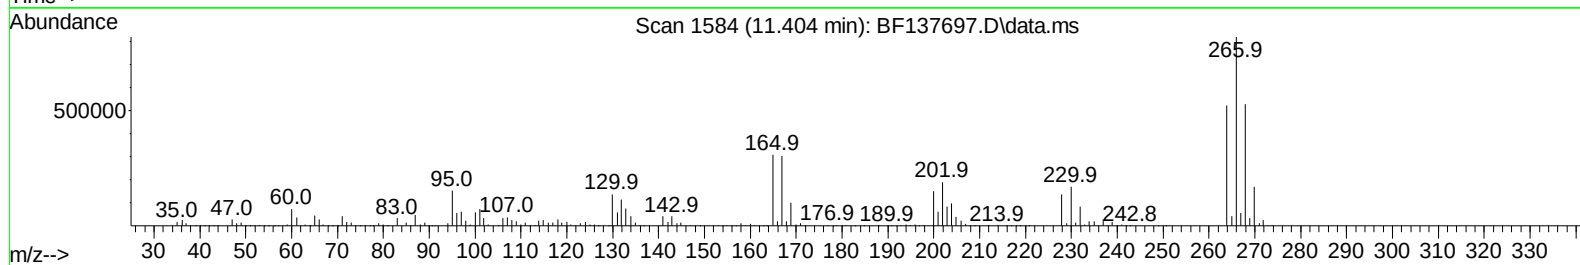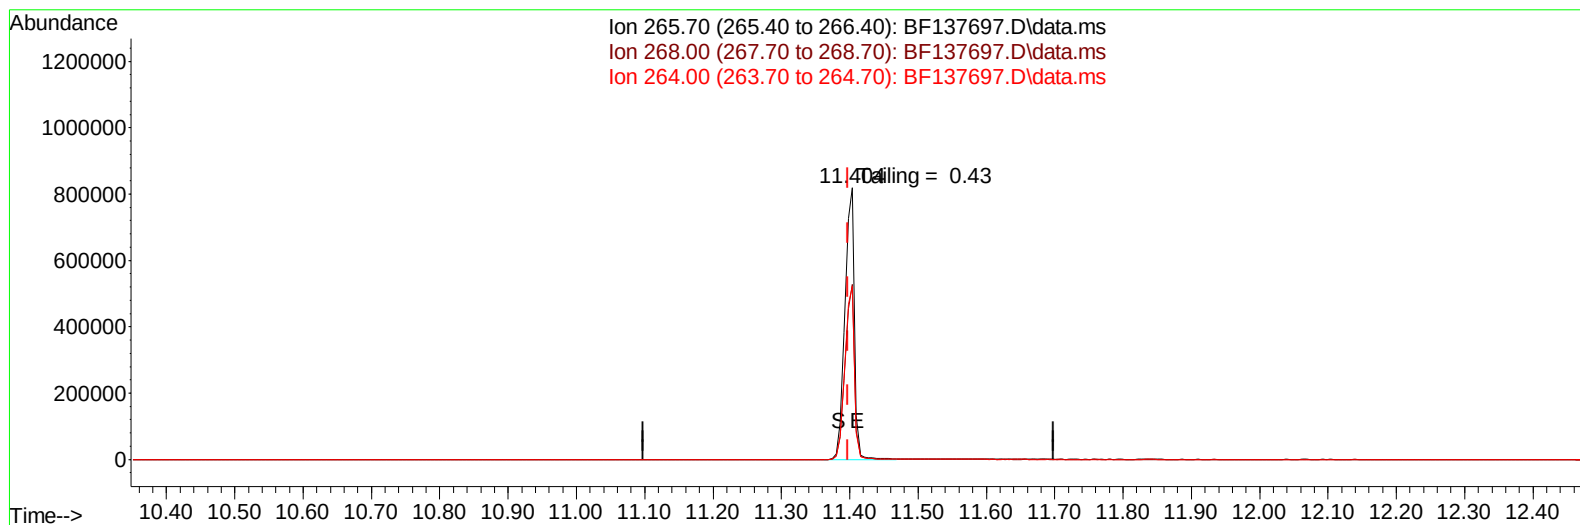

TIC: BF137697.D\data.ms

**(70) Pentachlorophenol (C)**

**11.404min (+ 0.006) 257741.65 ng**




**response 790110**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 64.39  |
| 264.00 | 64.20  | 63.70  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042324\  
Data File : BF137697.D  
Acq On : 23 Apr 2024 16:40  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Apr 24 04:07:40 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042324.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 24 03:57:12 2024  
Response via : Initial Calibration

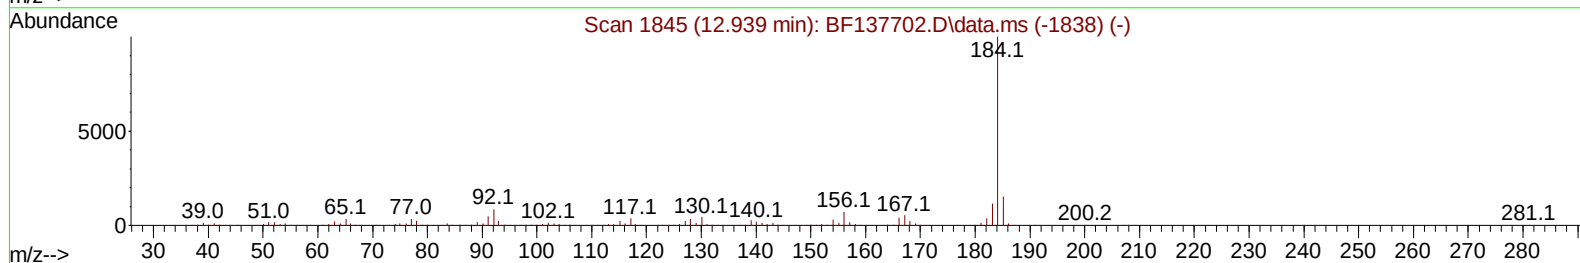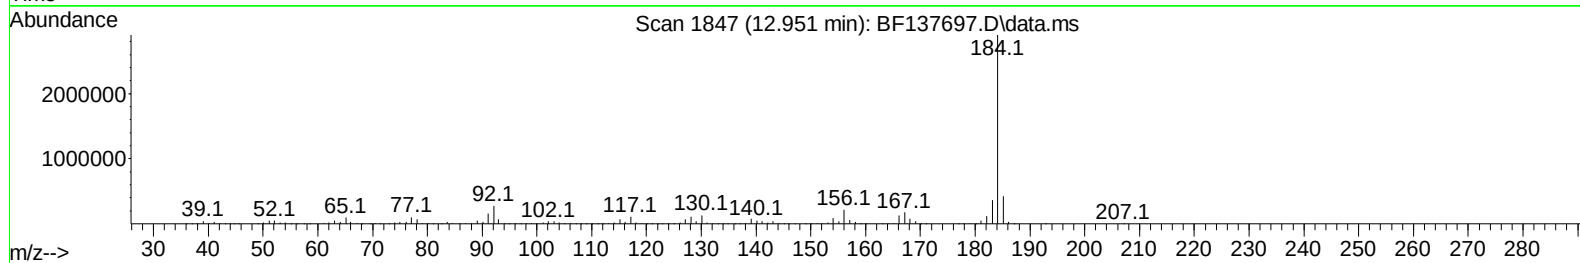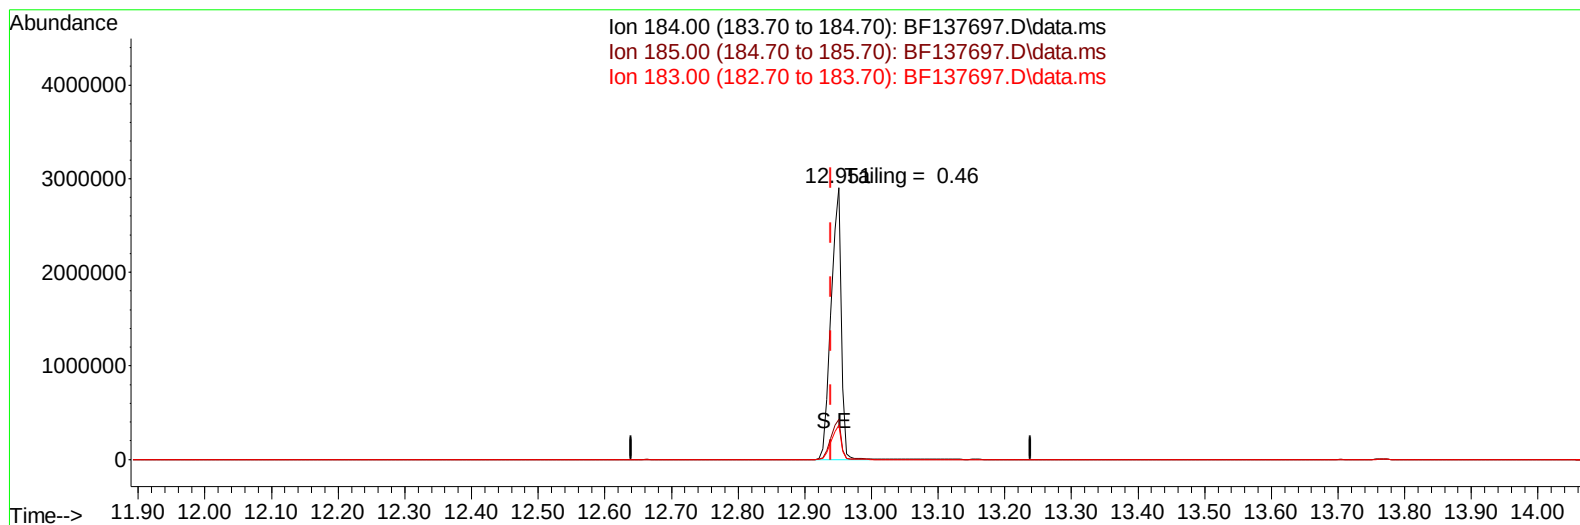

TIC: BF137697.D\data.ms

**(77) Benzidine**

**12.951min (+ 0.012) 7756.72 ng m**

**response 3031902**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.30  | 14.67  |
| 183.00 | 11.70  | 12.53  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 4/23/2024     | BNA_F            | <u>BF137697.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1193664          | 13.768             |
| DDD           | 13127            | 13.498             |
| DDE           | 175              | 13.127             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 13302         | 1206966          | 1.10               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP