
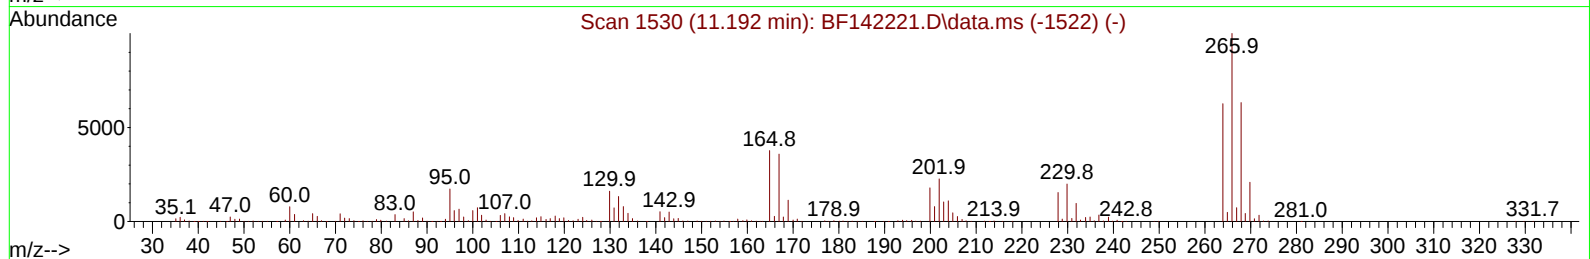
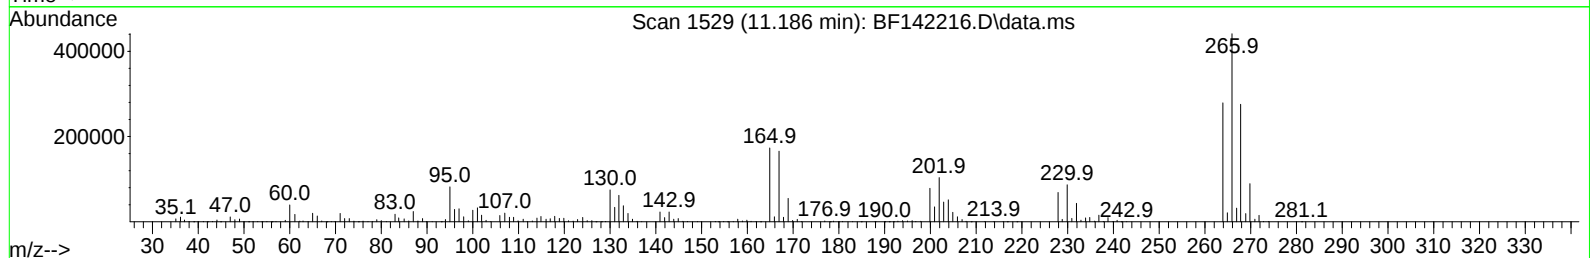


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042325\  
Data File : BF142216.D  
Acq On : 23 Apr 2025 10:18  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 14:53:51 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 23 14:53:02 2025  
Response via : Initial Calibration

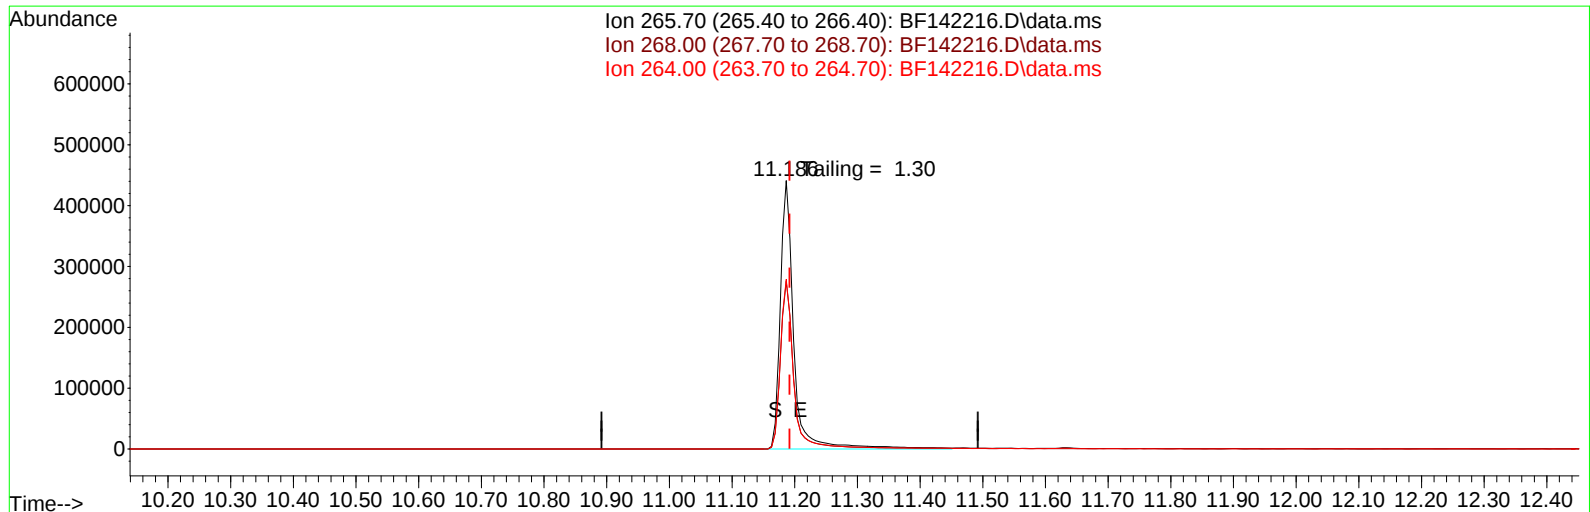

TIC: BF142216.D\data.ms

**(70) Pentachlorophenol (C)**




**11.186min (-0.006) 184361.04 ng**

**response 666551**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.20  | 62.51  |
| 264.00 | 62.70  | 63.23  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF042325\  
Data File : BF142216.D  
Acq On : 23 Apr 2025 10:18  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 14:53:51 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF042325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 23 14:53:02 2025  
Response via : Initial Calibration

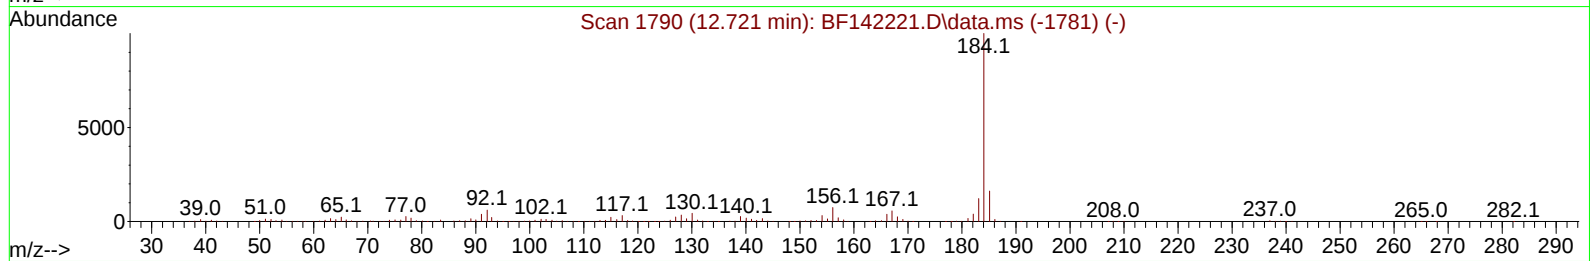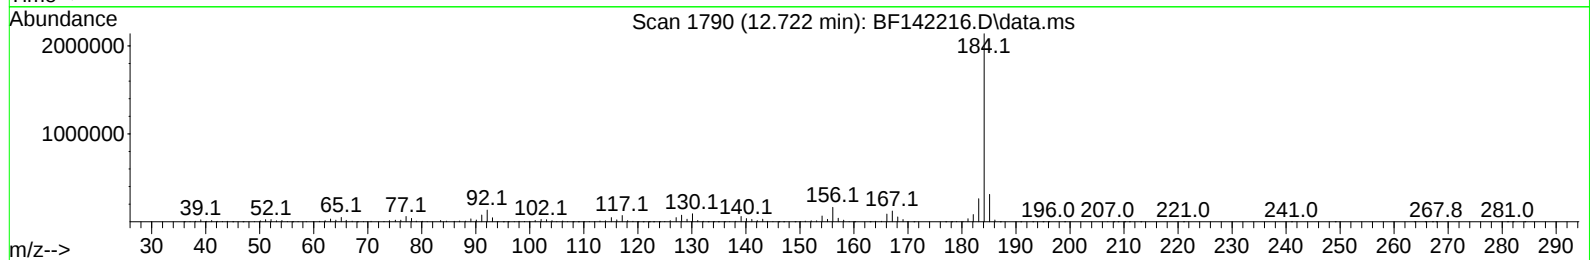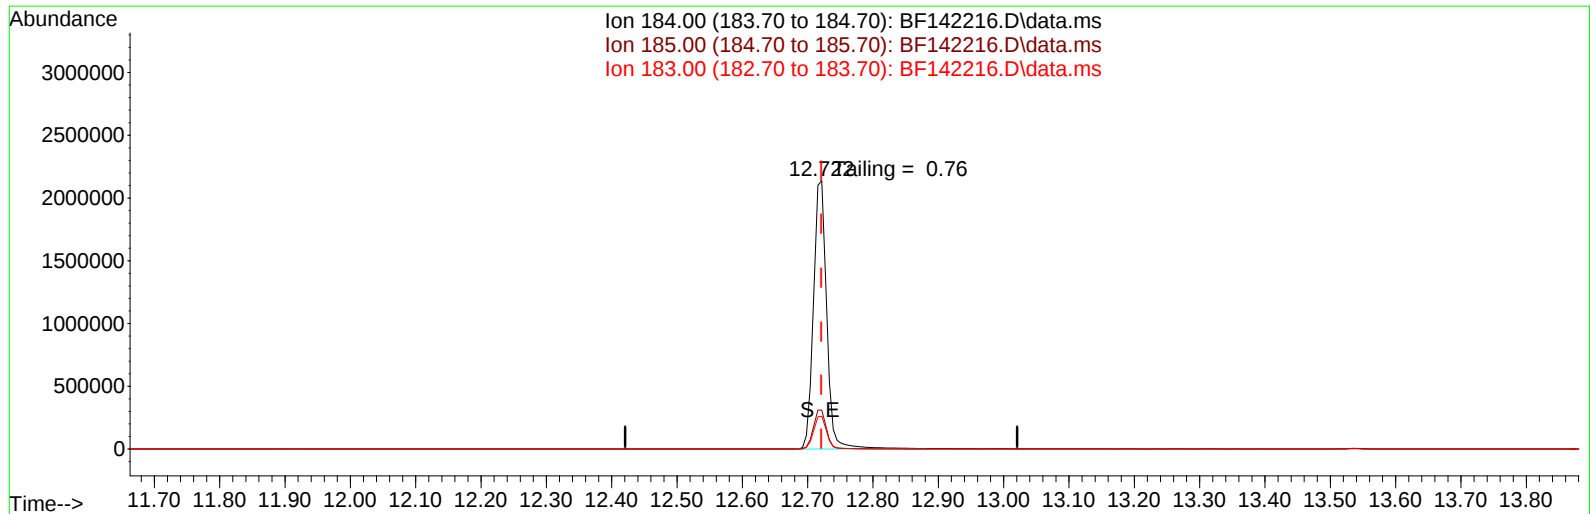

TIC: BF142216.D\data.ms

**(77) Benzidine**

12.722min (+ 0.001) 490043.66 ng

response 3028485

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 16.20  | 14.53  |
| 183.00 | 12.20  | 12.27  |
| 0.00   | 0.00   | 0.00   |