
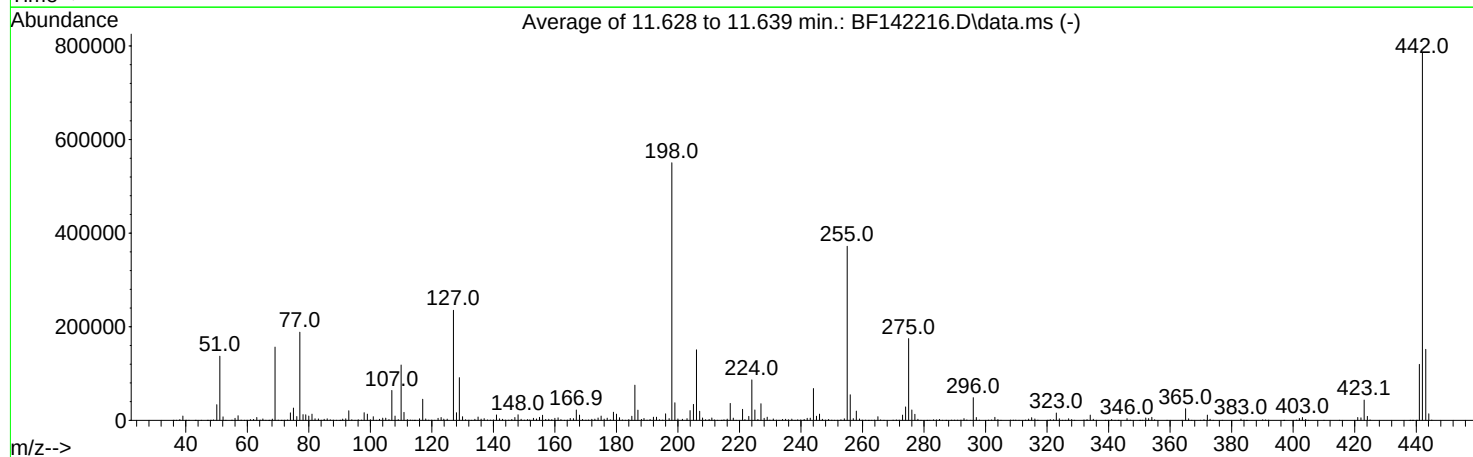


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042325\
Data File : BF142216.D
Acq On : 23 Apr 2025 10:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 23 14:53:02 2025

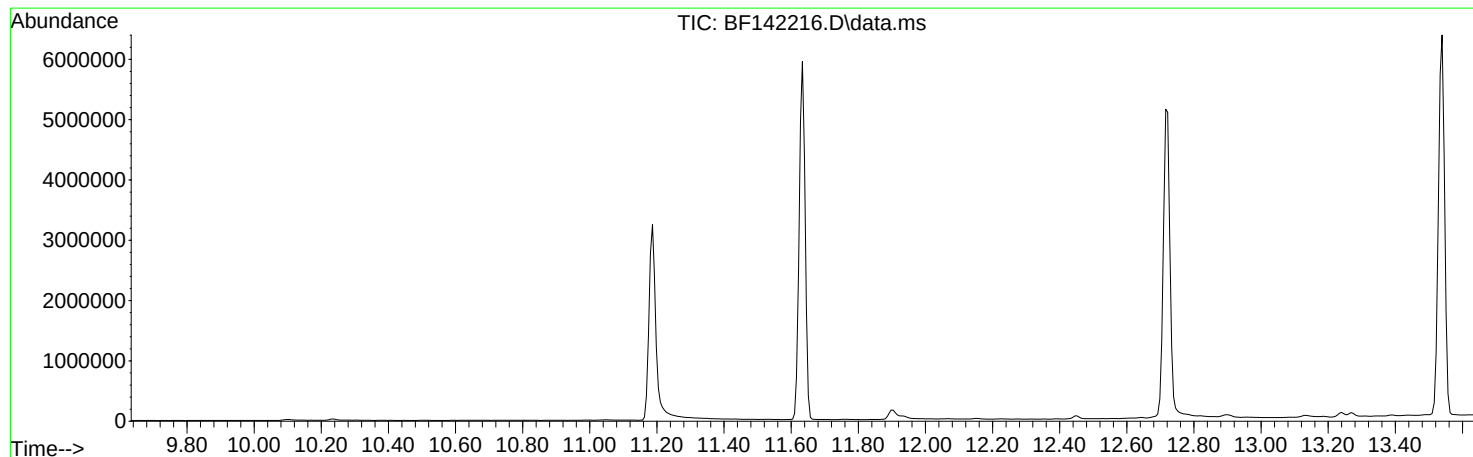

AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	137178	PASS
68	69	0.00	2	1.8	2769	PASS
69	198	0.00	100	28.4	156593	PASS
70	69	0.00	2	0.5	845	PASS
127	198	10	80	42.8	235413	PASS
197	198	0.00	2	0.7	3838	PASS
198	198	100	100	100.0	550485	PASS
199	198	5	9	6.8	37504	PASS
275	198	10	60	31.7	174741	PASS
365	198	1	100	4.5	24947	PASS
441	198	0.01	100	21.7	119616	PASS
442	442	50	100	100.0	786027	PASS
443	442	15	24	19.3	151835	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/23/2025	BNA_F	<u>BF142216.D</u>
Compound Name	Response	Retention Time
DDT	1677705	13.539
DDD	42497	13.239
DDE	6216	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
48713	1726418	2.82

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042325\
Data File : BF142216.D
Acq On : 23 Apr 2025 10:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 23 14:53:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 23 14:53:02 2025
Response via : Initial Calibration

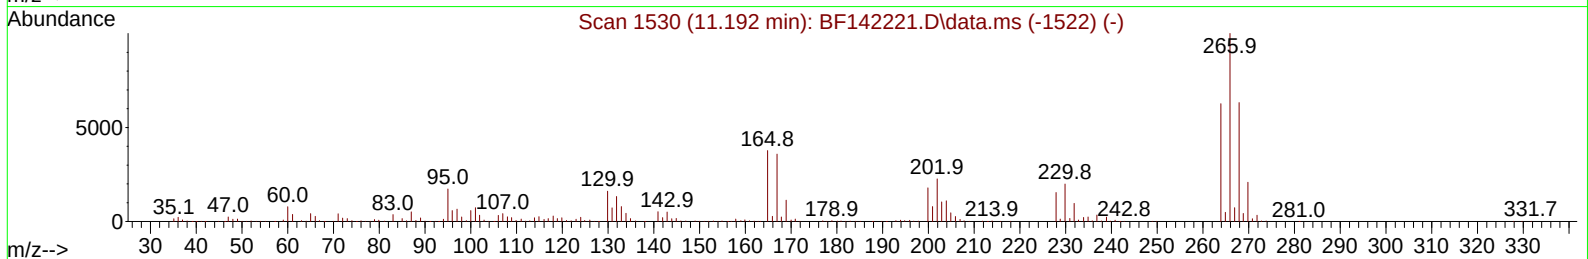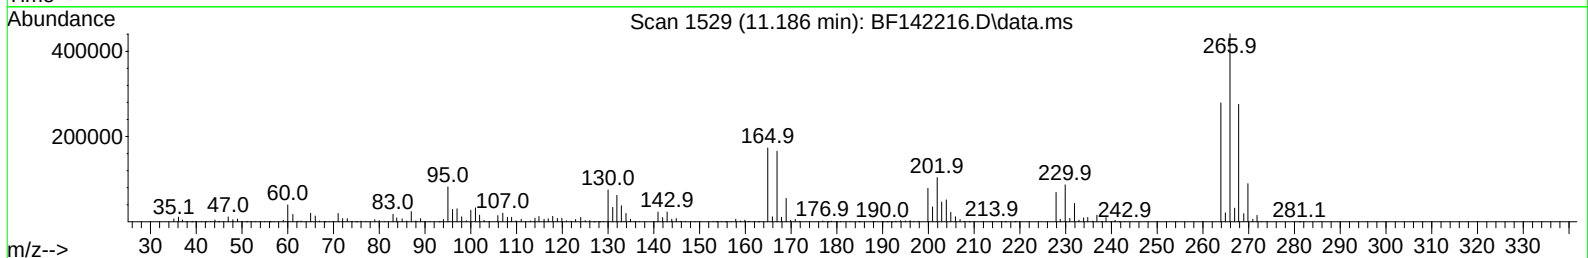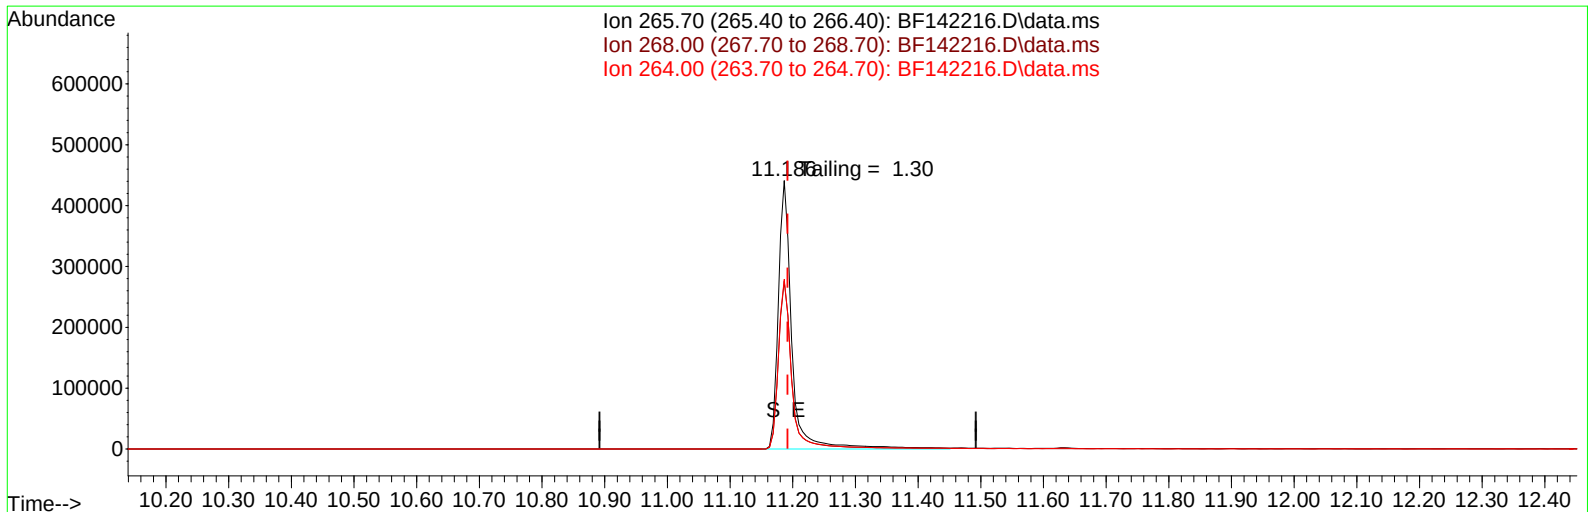

TIC: BF142216.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 184361.04 ng




response 666551

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	62.51
264.00	62.70	63.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042325\
Data File : BF142216.D
Acq On : 23 Apr 2025 10:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 23 14:53:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 23 14:53:02 2025
Response via : Initial Calibration

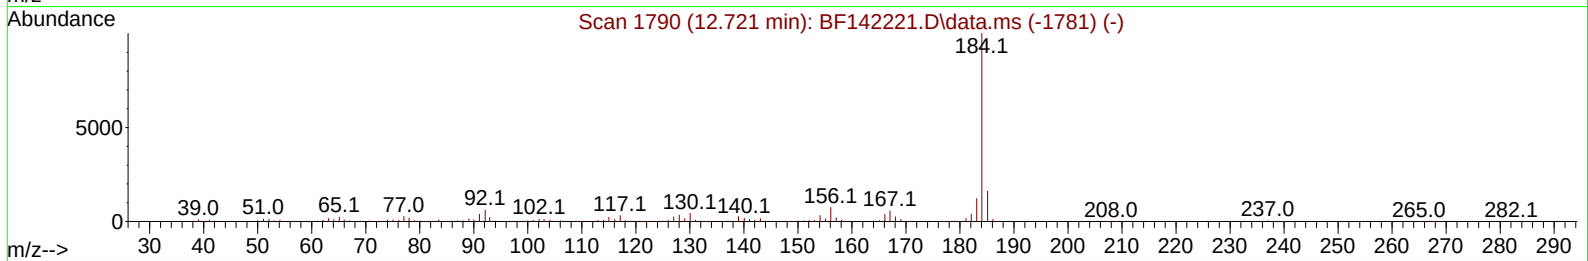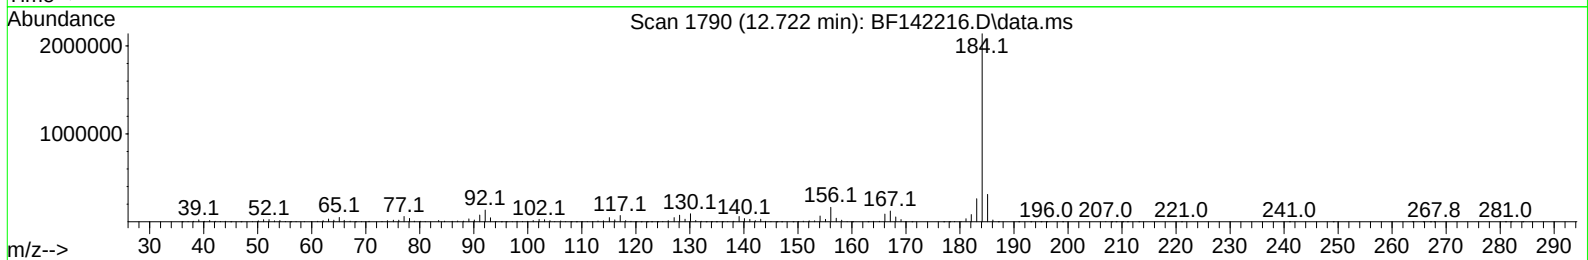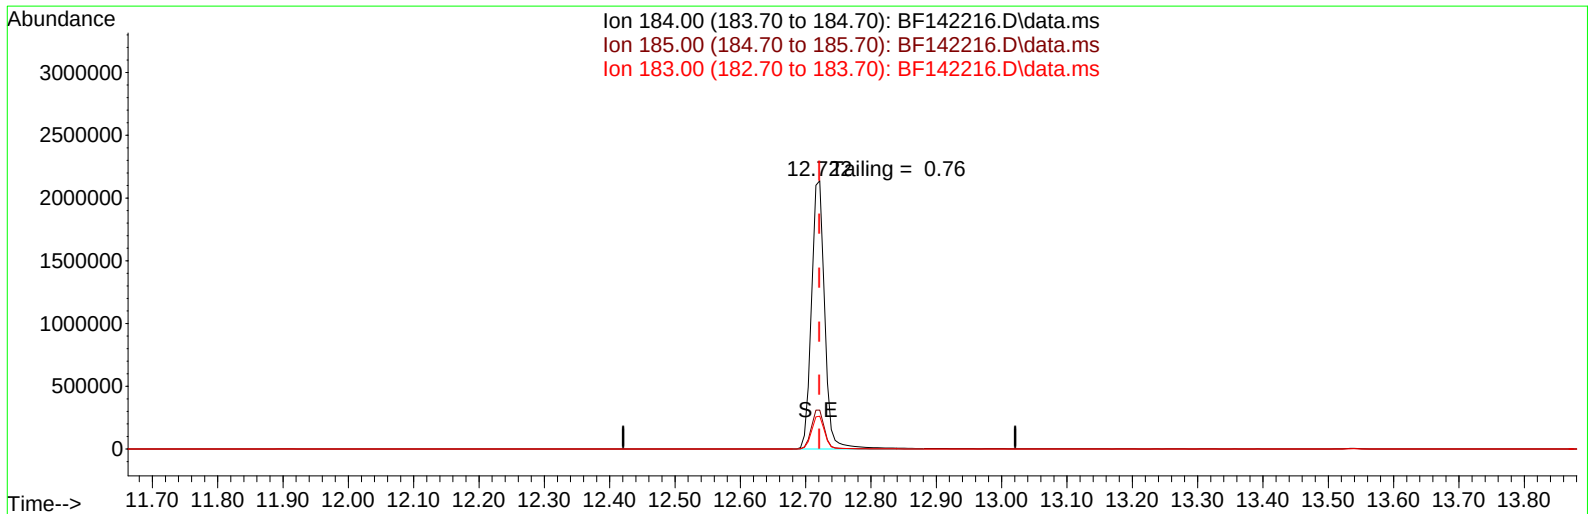

TIC: BF142216.D\data.ms

(77) Benzidine

12.722min (+ 0.001) 490043.66 ng

response 3028485

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.53
183.00	12.20	12.27
0.00	0.00	0.00