
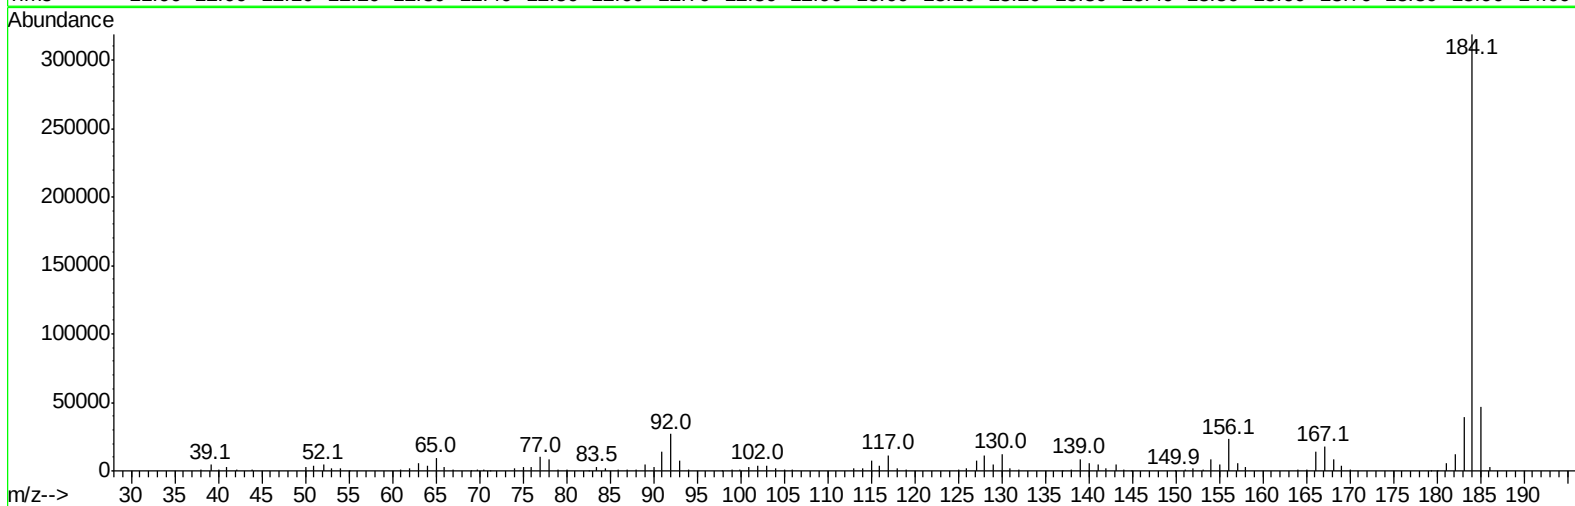


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042417\
Data File : BF094576.D
Acq On : 24 Apr 2017 10:49
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 07:18:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

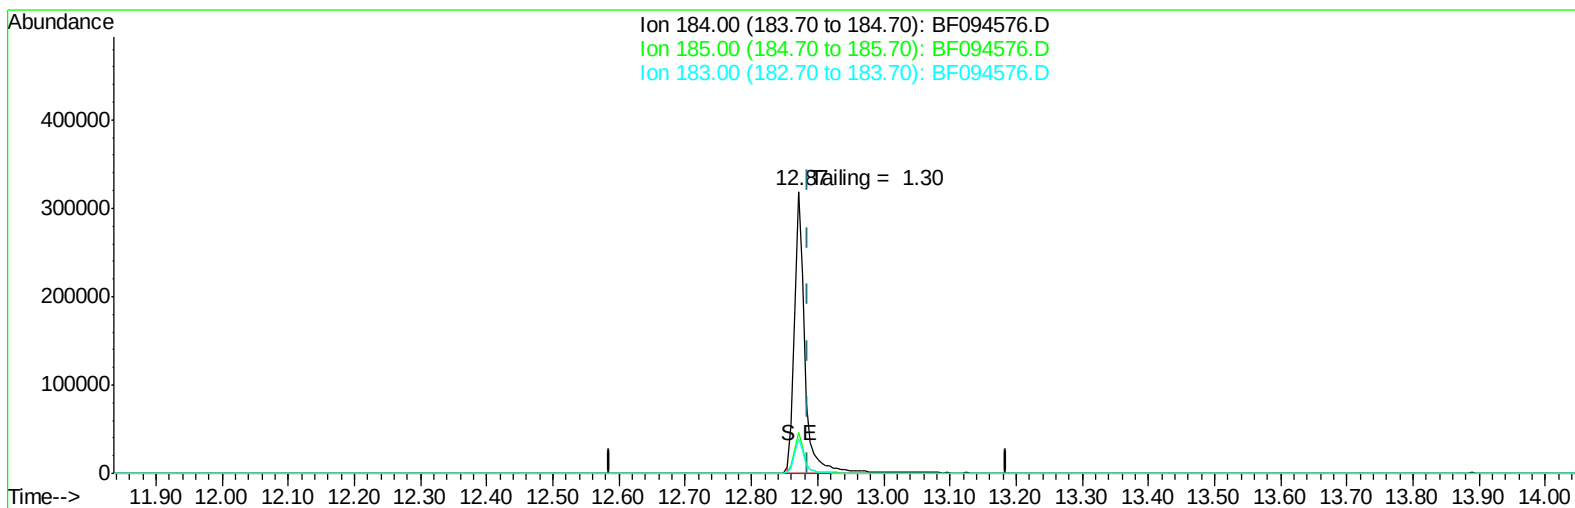

TIC: BF094576.D

(76) Benzidine



12.871min (-0.015) 0.00ng

response 362494

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.63#
183.00	12.20	12.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042417\
Data File : BF094576.D
Acq On : 24 Apr 2017 10:49
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 07:18:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

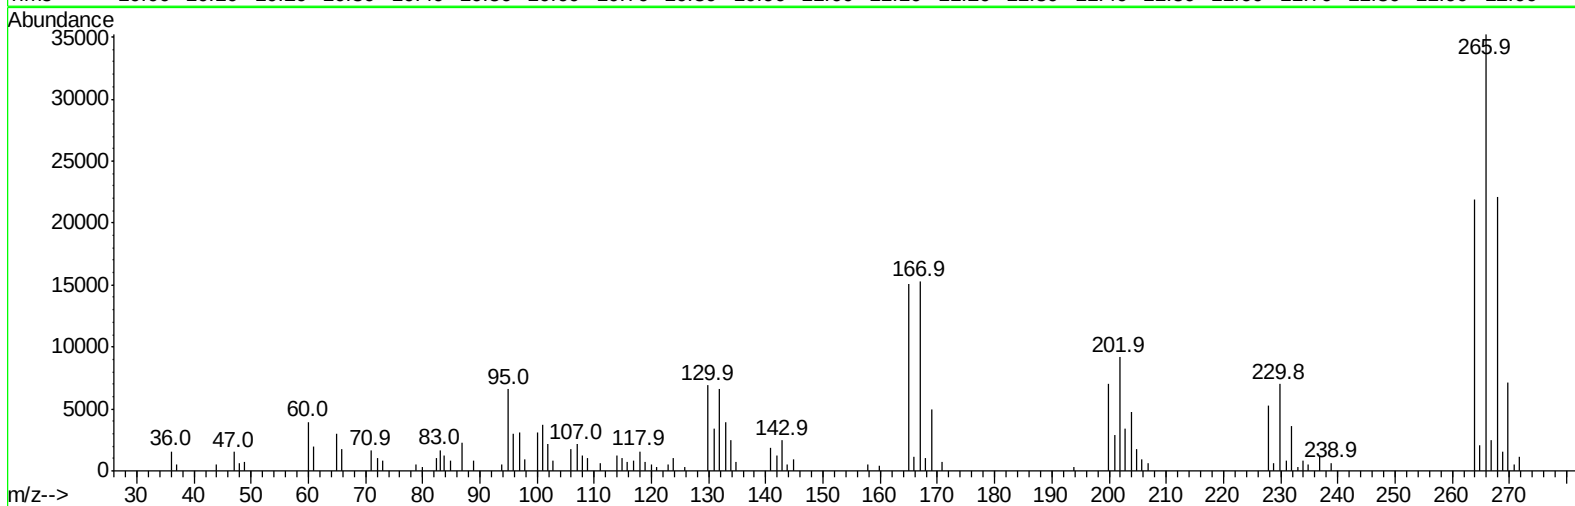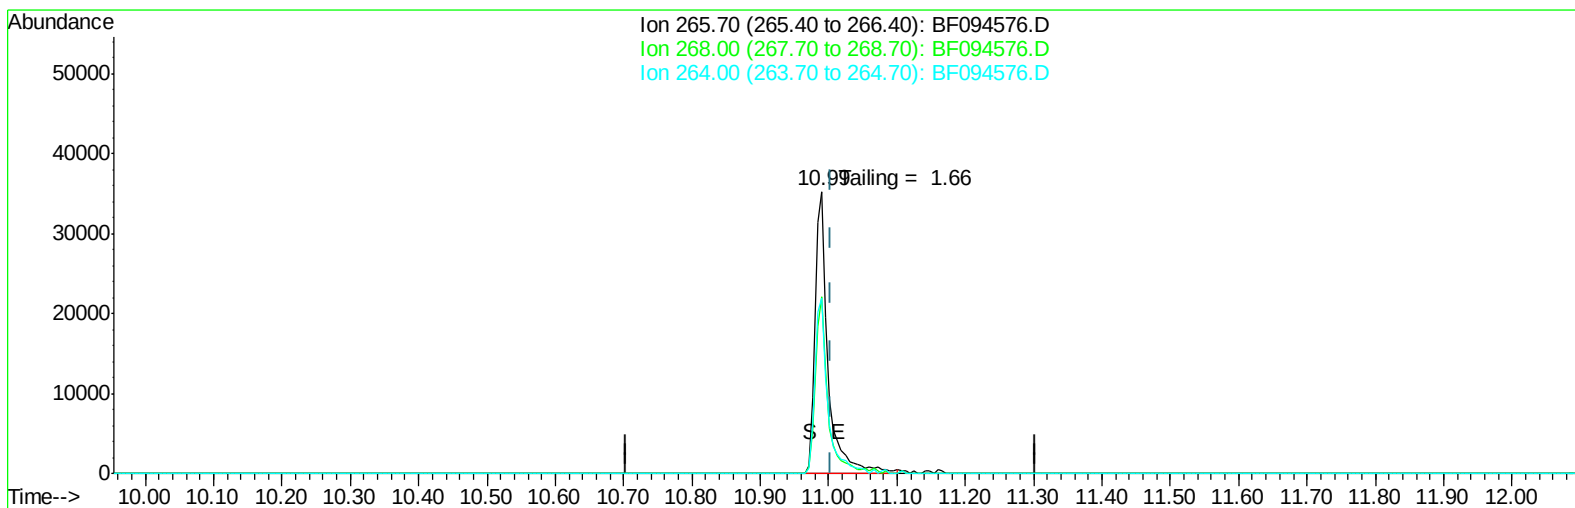

TIC: BF094576.D

(69) Pentachlorophenol (C)

10.989min (-0.015) 0.00ng

response 45930

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.79
264.00	64.60	62.27
0.00	0.00	0.00