

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042417\
 Data File : BF094584.D
 Acq On : 24 Apr 2017 14:44
 Operator : SJ/MA
 Sample : I2780-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PE-5

Quant Time: Apr 25 04:38:13 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 17 14:59:23 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	5.75	152	149381	20.00	ng	0.00
21) Naphthalene-d8	7.25	136	571696	20.00	ng	-0.01
38) Acenaphthene-d10	9.38	164	242374	20.00	ng	-0.02
63) Phenanthrene-d10	11.20	188	394893	20.00	ng	-0.02
75) Chrysene-d12	14.45	240	258033	20.00	ng	-0.02
86) Perylene-d12	16.08	264	237551	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	4.32	112	1216359	135.09	ng	0.01
7) Phenol-d6	5.40	99	1480430	139.47	ng	0.00
23) Nitrobenzene-d5	6.41	82	916412	98.98	ng	0.00
41) 2,4,6-Tribromophenol	10.36	330	260358	137.33	ng	-0.01
44) 2-Fluorobiphenyl	8.57	172	1406485	85.38	ng	-0.01
78) Terphenyl-d14	13.18	244	894559	92.67	ng	-0.01
Target Compounds						Qvalue
10) Phenol	5.40	94	93718	7.19	ng	95
49) Dimethylphthalate	9.07	163	332568	18.41	ng	98
74) Fluoranthene	12.69	202	64241	2.79	ng	97
77) Pyrene	12.97	202	58946	3.27	ng	95
80) Benzo(a)anthracene	14.44	228	31583	2.11	ng	99
82) Chrysene	14.48	228	32007	2.34	ng	98
87) Benzo(b)fluoranthene	15.67	252	52706m	3.63	ng	
89) Benzo(a)pyrene	16.02	252	33099	2.45	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042417\
Data File : BF094584.D
Acq On : 24 Apr 2017 14:44
Operator : SJ/MA
Sample : I2780-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PE-5

Quant Time: Apr 25 04:38:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

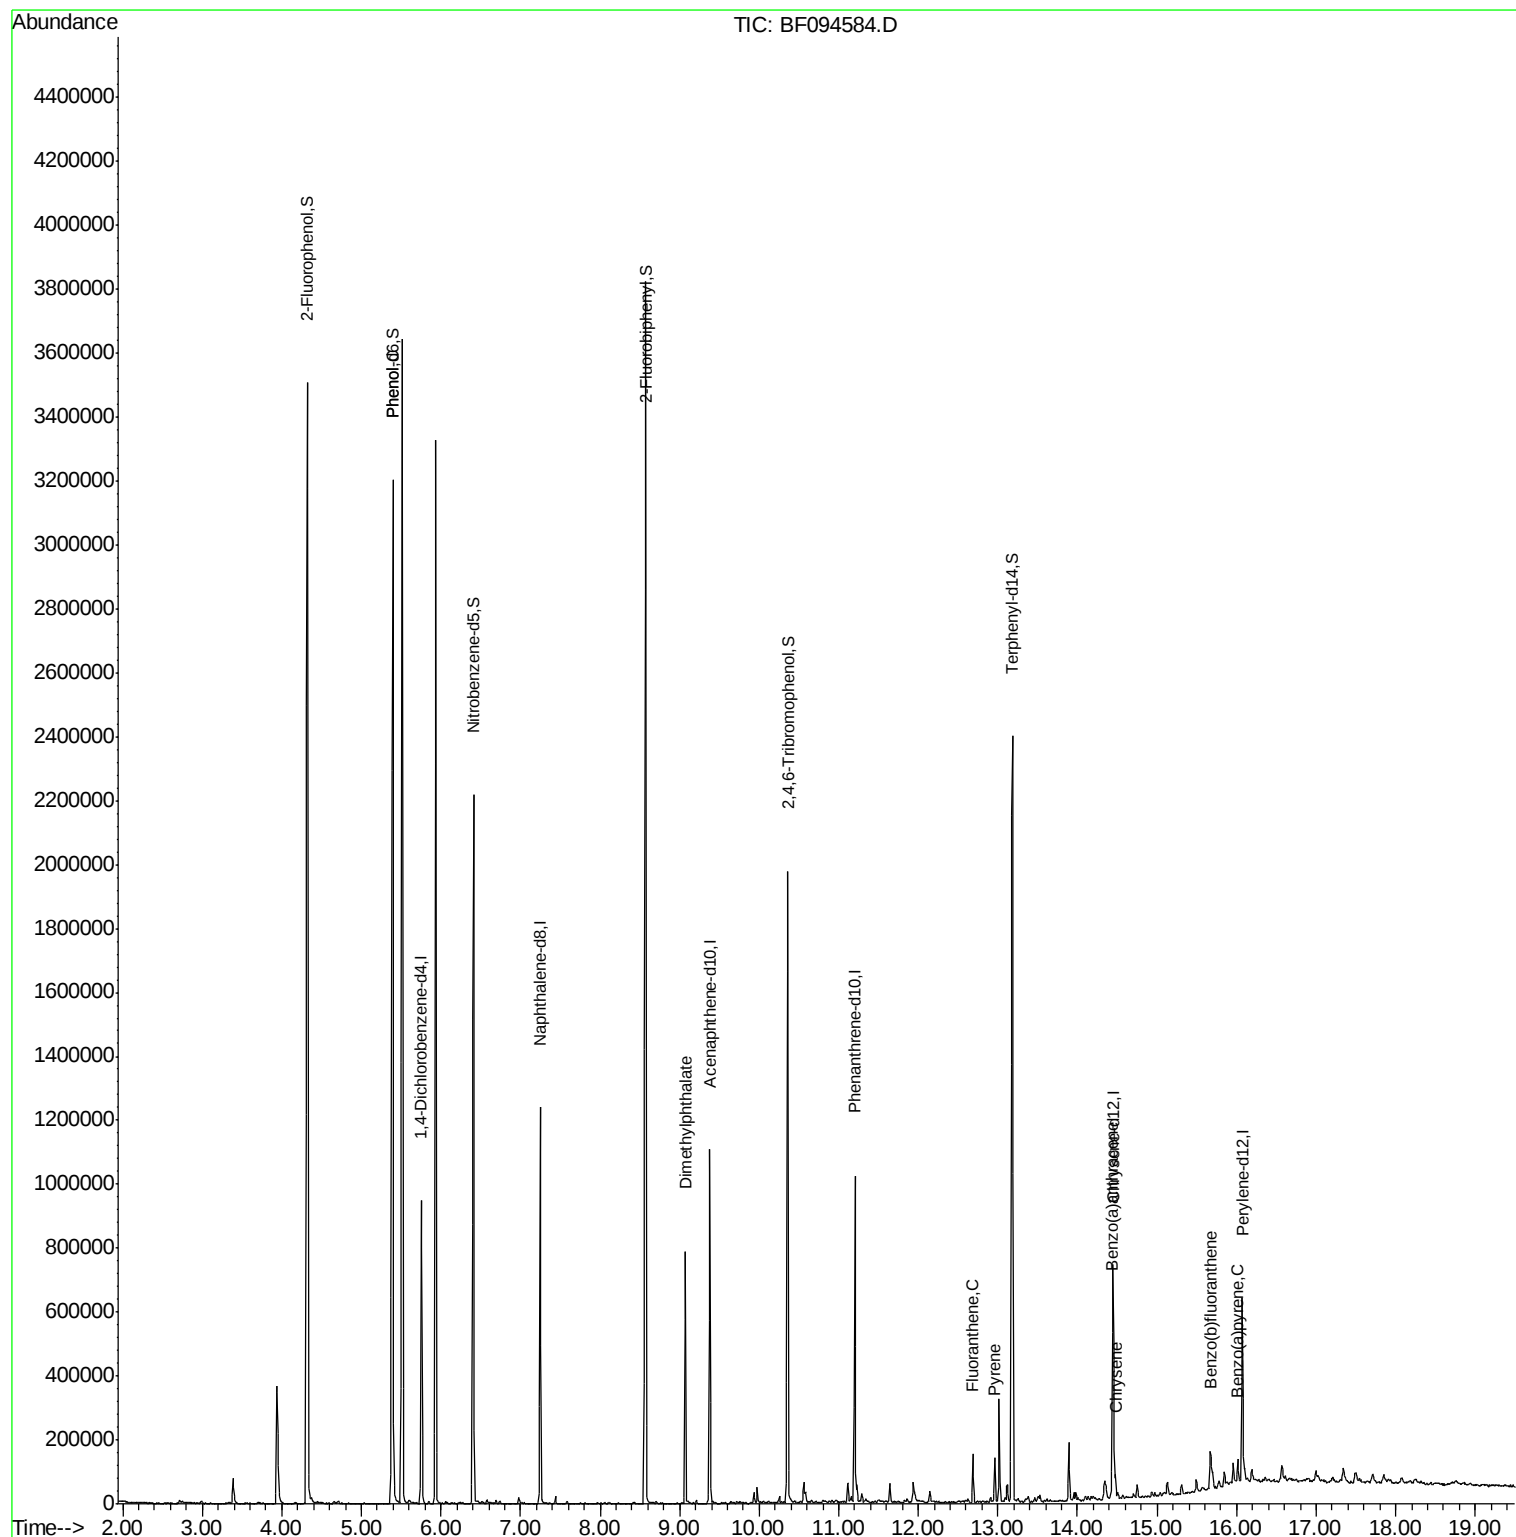




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 5.75 min Scan# 649
Delta R.T. -0.01 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Instrument :
BNA_F
ClientSampleId :
PE-5

Tot Ion:152 Resp: 149381
Ion Ratio Lower Upper
152 100
150 160.3 126.2 189.2
115 63.1 52.2 78.2




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

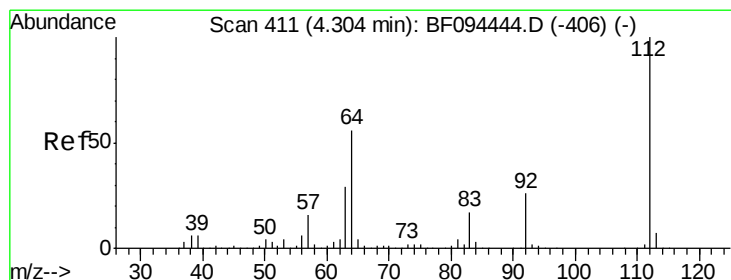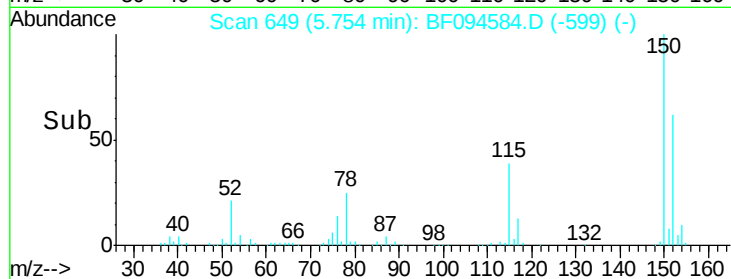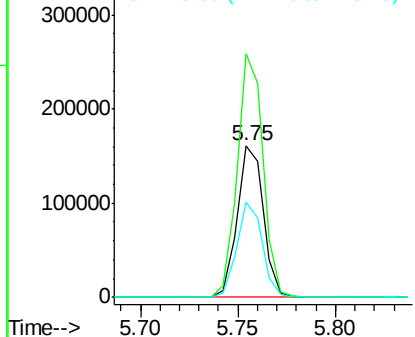



#5


2-Fluorophenol
Concen: 135.09 ng
RT: 4.32 min Scan# 405
Delta R.T. 0.01 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Tgt Ion:112 Resp: 1216359
Ion Ratio Lower Upper
112 100
64 58.3 46.0 69.0
63 28.7 23.4 35.0

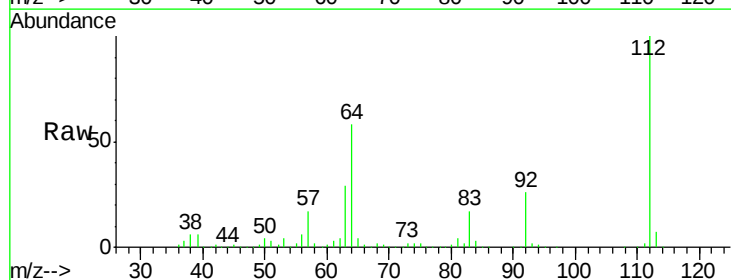

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

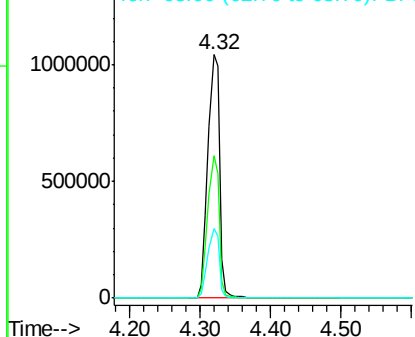

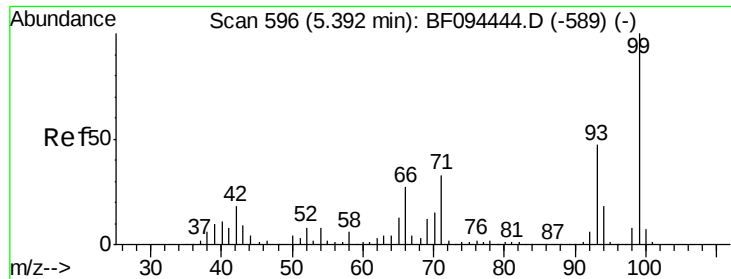

#7

Phenol-d6

Concen: 139.47 ng

RT: 5.40 min Scan# 588

Delta R.T. 0.00 min

Lab File: BF094584.D

Acq: 24 Apr 2017 14:44

Instrument :

BNA_F

ClientSampleId :

PE-5


Tot Ion: 99 Resp: 1480430

Ion Ratio Lower Upper

99 100

42 17.2 13.5 20.3




71 33.3 24.5 36.7

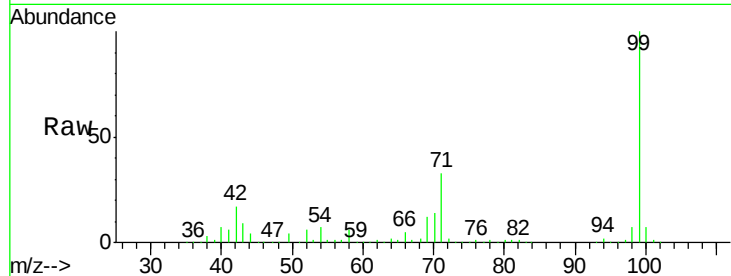

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

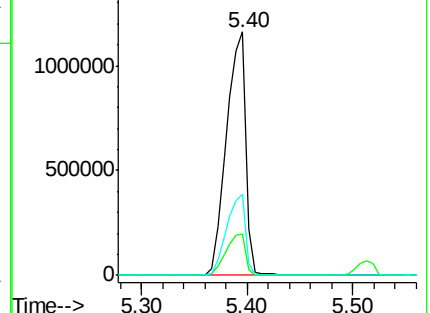

#10

Phenol

Concen: 7.19 ng

RT: 5.40 min Scan# 589

Delta R.T. -0.00 min

Lab File: BF094584.D

Acq: 24 Apr 2017 14:44


Tgt Ion: 94 Resp: 93718

Ion Ratio Lower Upper

94 100

65 27.1 9.9 49.9



66 40.4 23.1 63.1




Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

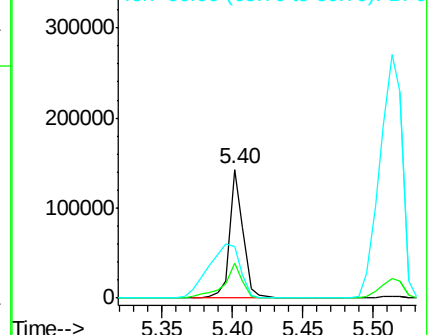


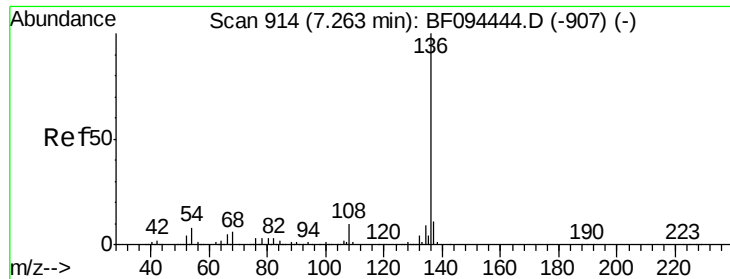




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.25 min Scan# 903
Delta R.T. -0.01 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Instrument :
BNA_F
ClientSampleId :
PE-5

Tot Ion:136	Resp:	571696
Ion	Ratio	Lower Upper
136	100	
137	10.7	8.5 12.7
54	7.1	4.9 7.3
68	5.9	4.1 6.1

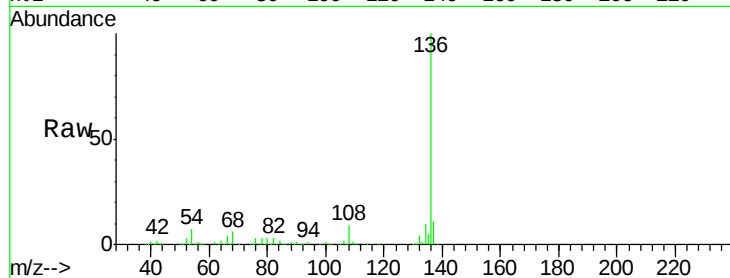


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

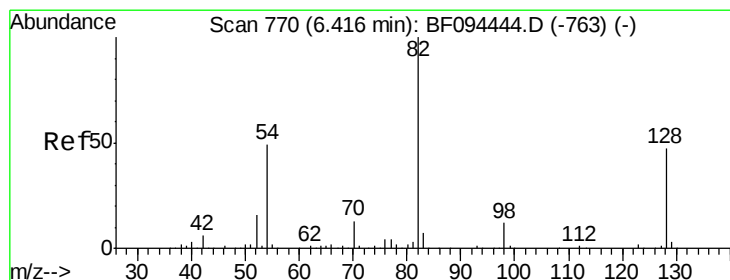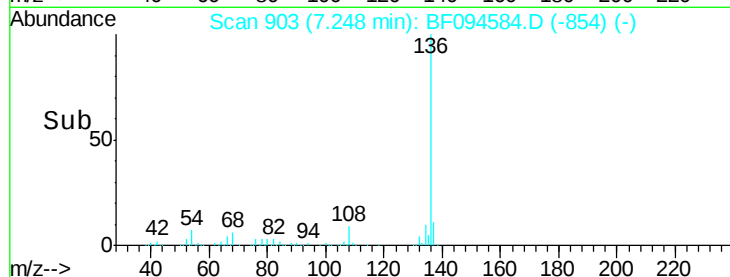
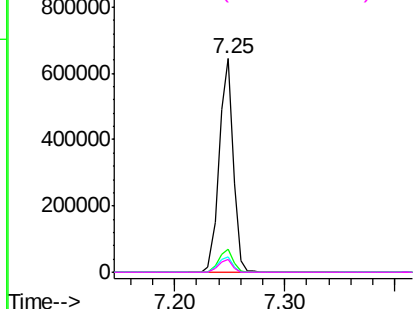



#23
Nitrobenzene-d5
Concen: 98.98 ng
RT: 6.41 min Scan# 761
Delta R.T. -0.00 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Tgt Ion: 82	Resp:	916412
Ion	Ratio	Lower Upper
82	100	
128	48.8	34.0 51.0
54	46.7	42.2 63.2

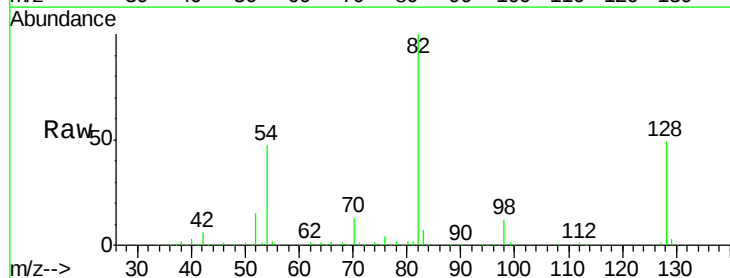

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

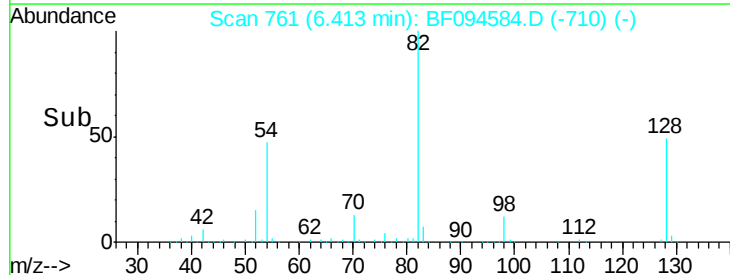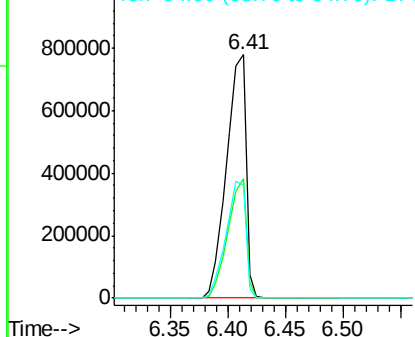


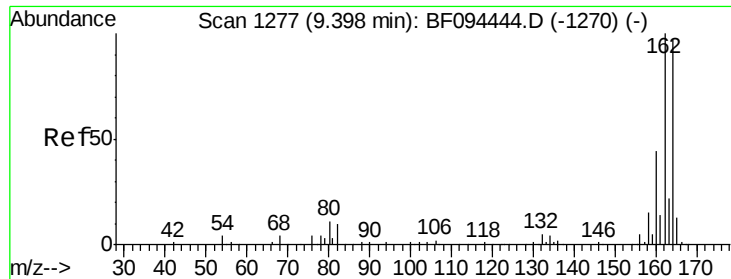




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.38 min Scan# 1265
 Delta R.T. -0.02 min
 Lab File: BF094584.D
 Acq: 24 Apr 2017 14:44

Instrument :
 BNA_F
 ClientSampleId :
 PE-5

Tot Ion:164 Resp: 242374
 Ion Ratio Lower Upper
 164 100
 162 106.1 82.6 123.8
 160 45.1 36.2 54.2

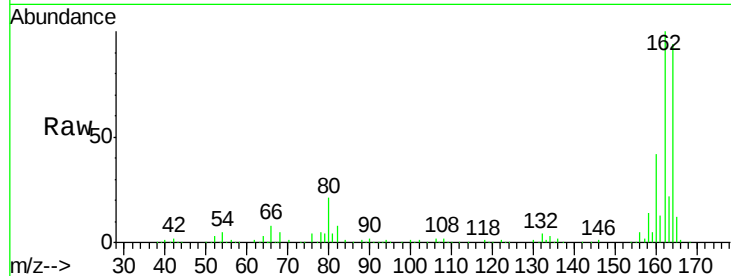


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E


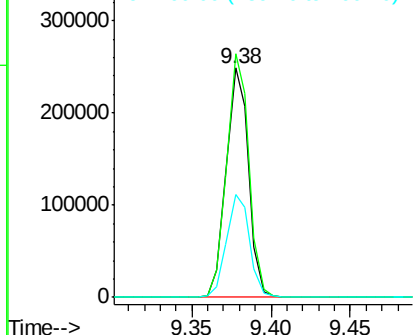



#41
 2,4,6-Tribromophenol
 Concen: 137.33 ng
 RT: 10.36 min Scan# 1432
 Delta R.T. -0.01 min
 Lab File: BF094584.D
 Acq: 24 Apr 2017 14:44

Tgt Ion:330 Resp: 260358
 Ion Ratio Lower Upper
 330 100
 332 97.7 76.6 115.0
 141 38.9 31.4 47.2



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

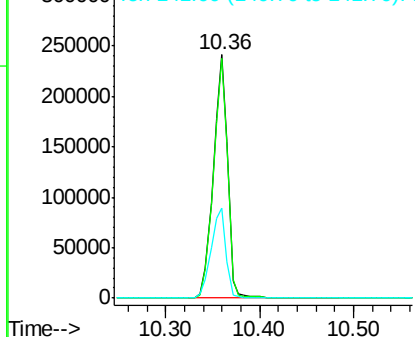







#44
2-Fluorobiphenyl
Concen: 85.38 ng
RT: 8.57 min Scan# 1128
Delta R.T. -0.01 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Instrument :
BNA_F
ClientSampleId :
PE-5

Tot Ion:172 Resp: 1406485
Ion Ratio Lower Upper
172 100
171 36.7 29.6 44.4
170 24.0 19.8 29.8




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

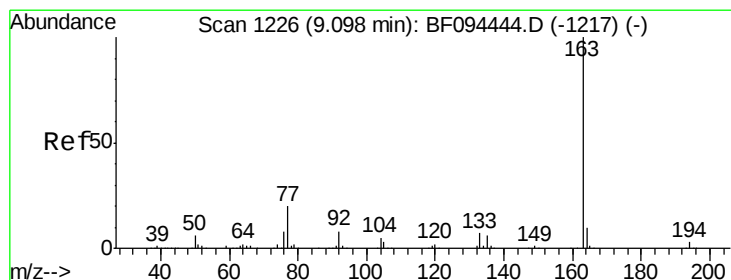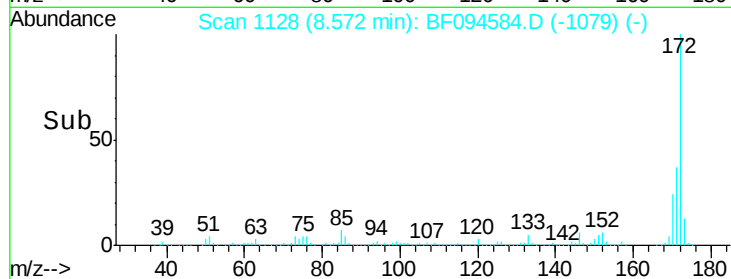
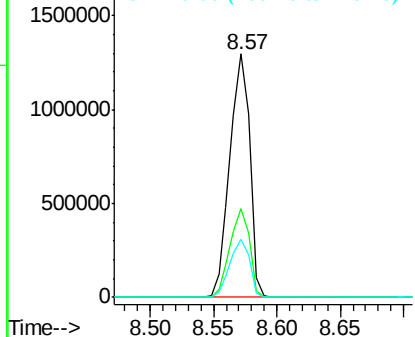



#49
Dimethylphthalate
Concen: 18.41 ng
RT: 9.07 min Scan# 1213
Delta R.T. -0.03 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Tgt Ion:163 Resp: 332568
Ion Ratio Lower Upper
163 100
194 3.5 2.6 4.0
164 9.6 8.4 12.6



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



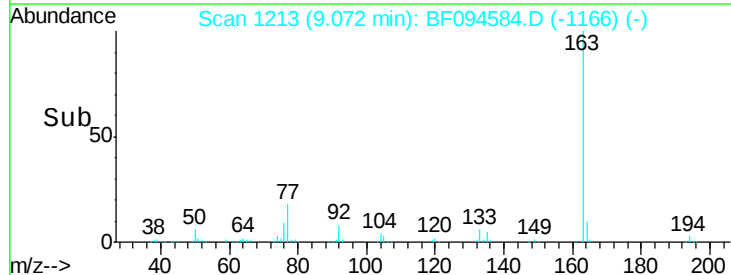
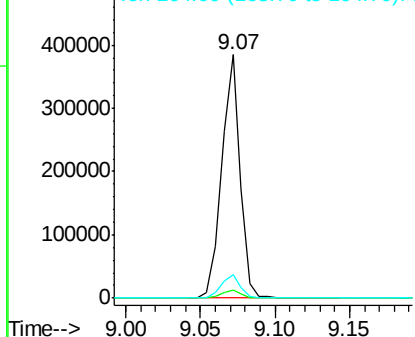


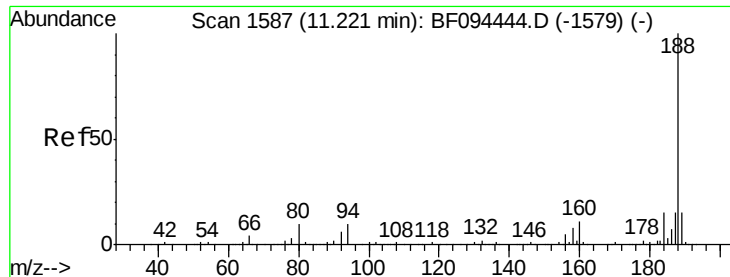

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.20 min Scan# 1575
Delta R.T. -0.02 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44




Instrument :
BNA_F
ClientSampleId :
PE-5


Tot Ion:188 Resp: 394893
Ion Ratio Lower Upper
188 100
94 10.4 9.4 14.2
80 11.1 10.2 15.2

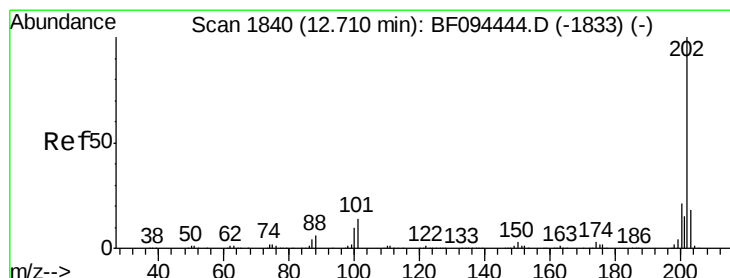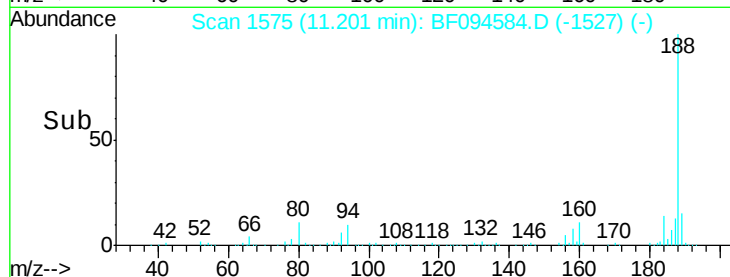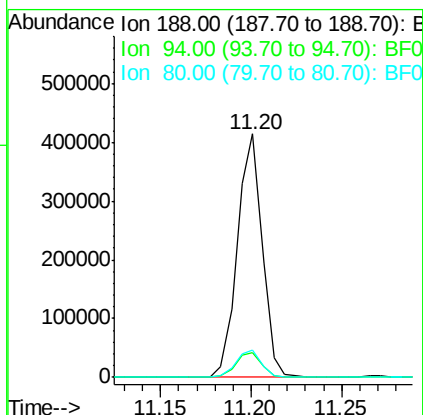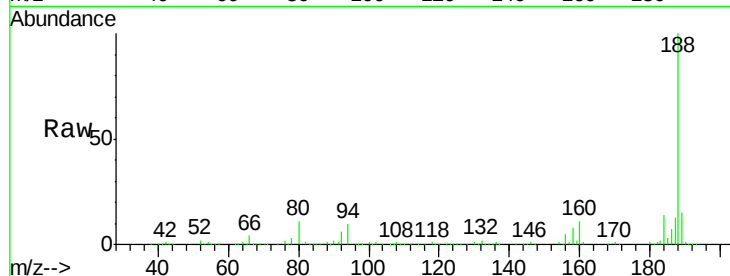

#74
Fluoranthene
Concen: 2.79 ng
RT: 12.69 min Scan# 1828
Delta R.T. -0.02 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Tgt Ion:202 Resp: 64241
Ion Ratio Lower Upper
202 100
101 12.0 0.0 33.2
203 16.9 0.0 38.1


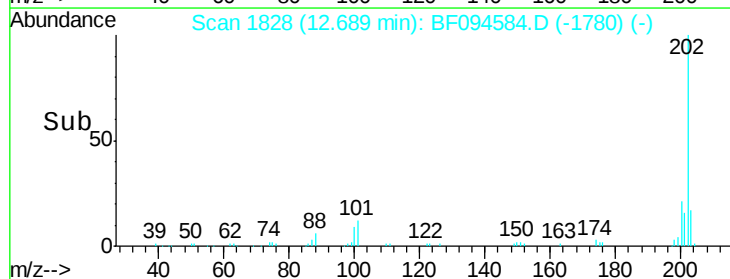
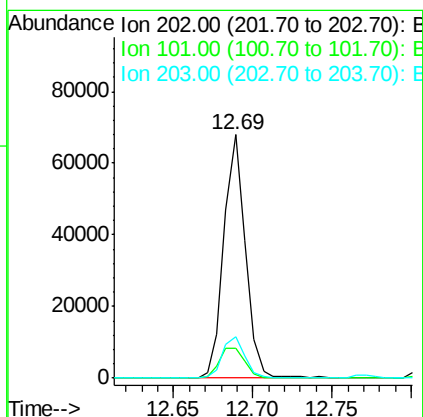
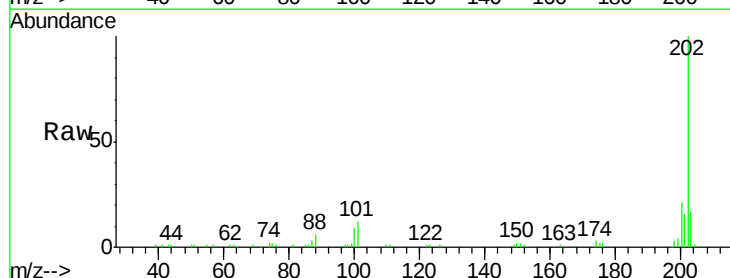


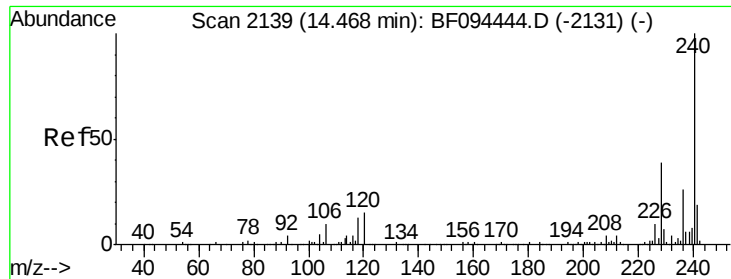

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.45 min Scan# 2127
Delta R.T. -0.02 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44




Instrument :
BNA_F
ClientSampleId :
PE-5


Tot Ion:240 Resp: 258033
Ion Ratio Lower Upper
240 100
120 14.5 5.8 8.8#
236 25.8 20.5 30.7

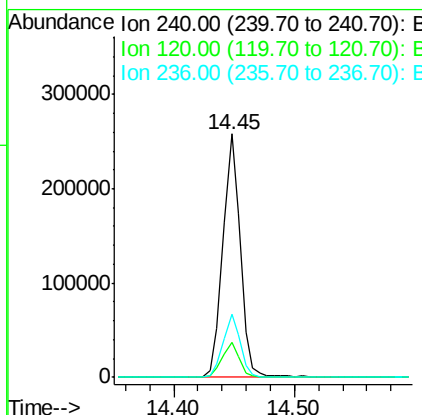

#77
Pyrene
Concen: 3.27 ng
RT: 12.97 min Scan# 1875
Delta R.T. -0.02 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Tgt Ion:202 Resp: 58946
Ion Ratio Lower Upper
202 100
200 19.9 17.6 26.4
203 20.2 14.4 21.6



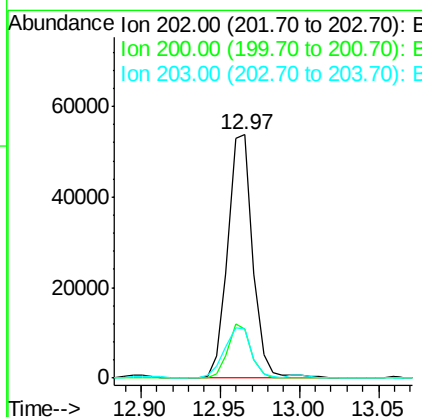



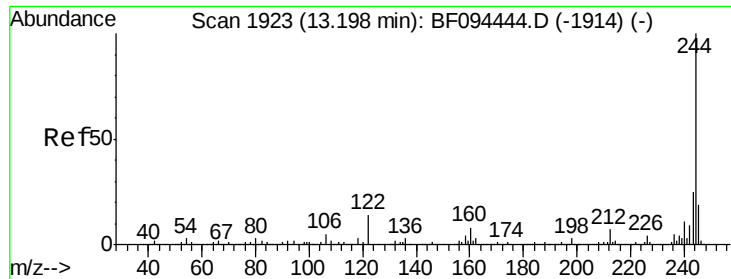

#78
 Terphenyl-d14
 Concen: 92.67 ng
 RT: 13.18 min Scan# 1912
 Delta R.T. -0.01 min
 Lab File: BF094584.D
 Acq: 24 Apr 2017 14:44




Instrument :
 BNA_F
 ClientSampleId :
 PE-5


Tot Ion:244 Resp: 894559
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.0 9.0
 122 13.2 10.3 15.5

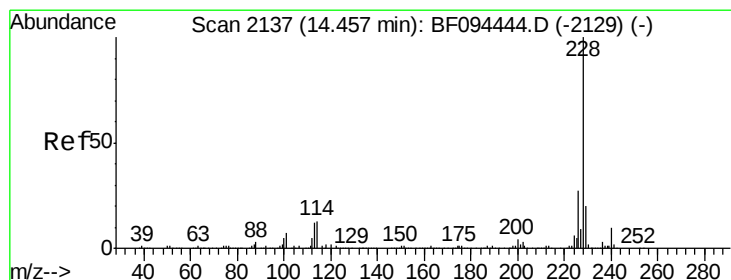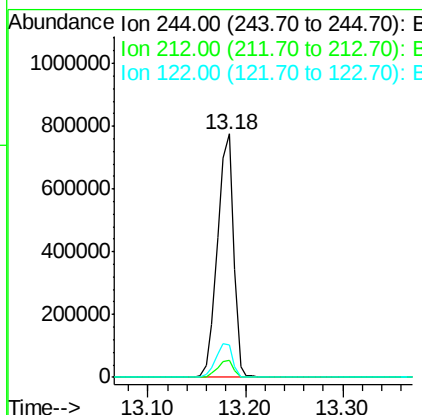

#80
 Benzo(a)anthracene
 Concen: 2.11 ng
 RT: 14.44 min Scan# 2125
 Delta R.T. -0.02 min
 Lab File: BF094584.D
 Acq: 24 Apr 2017 14:44

Tgt Ion:228 Resp: 31583
 Ion Ratio Lower Upper
 228 100
 226 28.6 22.6 33.8
 229 21.1 16.3 24.5


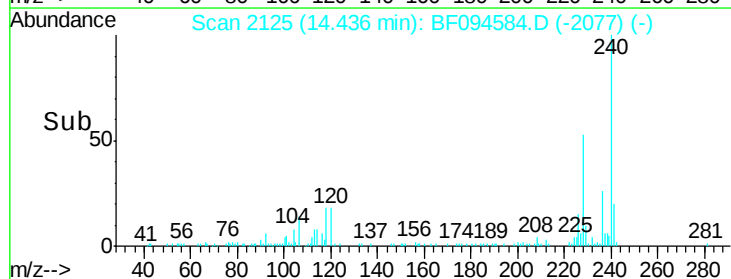
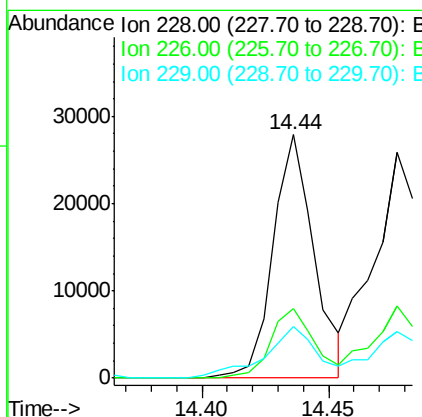
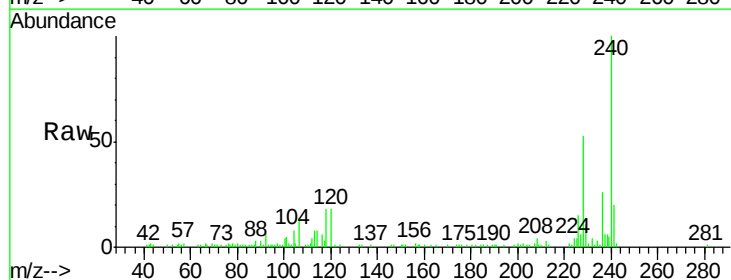




#82
Chrysene
Concen: 2.34 ng
RT: 14.48 min Scan# 2132
Delta R.T. -0.03 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44




Instrument :
BNA_F
ClientSampleId :
PE-5


Tot Ion:228 Resp: 32007
Ion Ratio Lower Upper
228 100
226 31.9 24.9 37.3
229 20.6 15.8 23.6

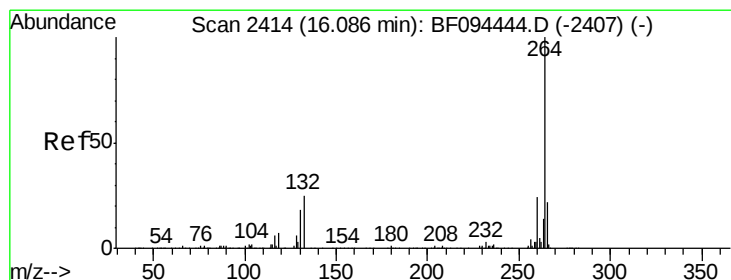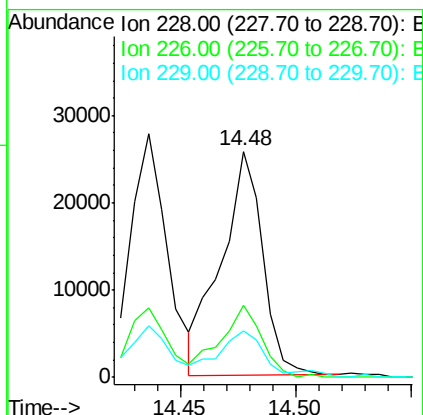

#86
Perylene-d12
Concen: 20.00 ng
RT: 16.08 min Scan# 2404
Delta R.T. -0.01 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Tgt Ion:264 Resp: 237551
Ion Ratio Lower Upper
264 100
260 24.1 19.5 29.3
265 21.2 17.2 25.8


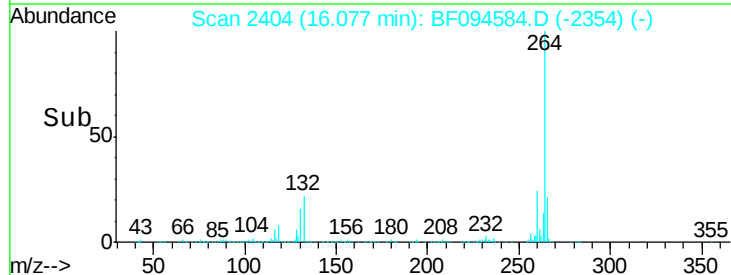
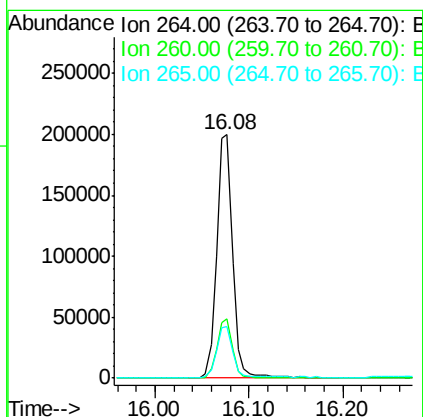



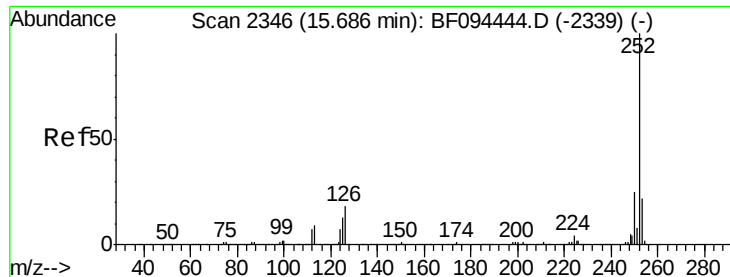

#87
Benzo(b)fluoranthene
Concen: 3.63 ng m
RT: 15.67 min Scan# 2335
Delta R.T. -0.01 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Instrument :
BNA_F
ClientSampleId :
PE-5

Tot Ion:252 Resp: 52706
Ion Ratio Lower Upper
252 100
253 21.3 18.1 27.1
125 12.8 9.8 14.8

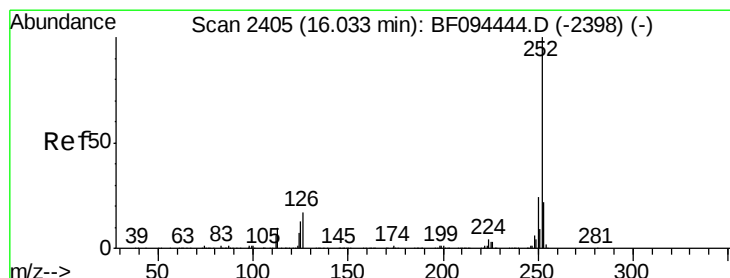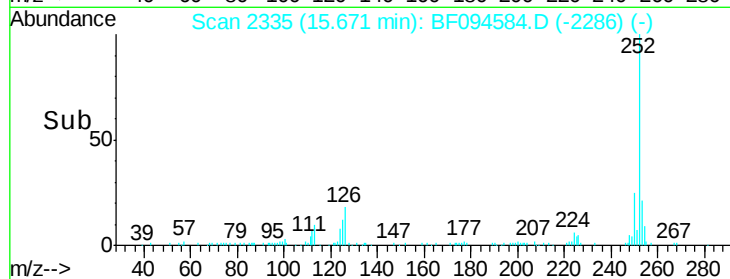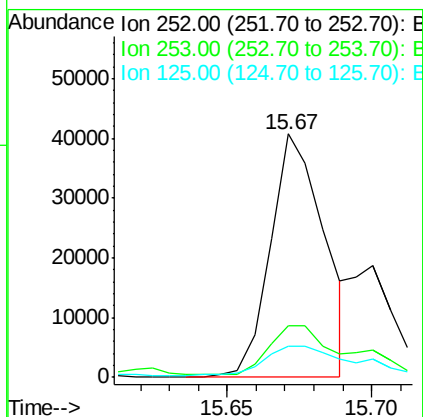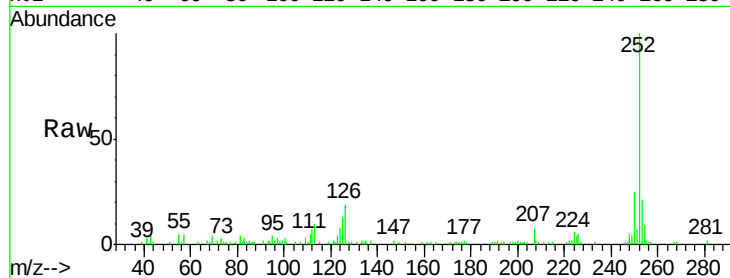

#89
Benzo(a)pyrene
Concen: 2.45 ng
RT: 16.02 min Scan# 2394
Delta R.T. -0.01 min
Lab File: BF094584.D
Acq: 24 Apr 2017 14:44

Tgt Ion:252 Resp: 33099
Ion Ratio Lower Upper
252 100
253 23.2 17.5 26.3
125 14.5 11.0 16.4

