


Data Path : Z:\HPCHEM1\BNA F\Data\BF042417\
 Data File : BF094576.D
 Acq On : 24 Apr 2017 10:49
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

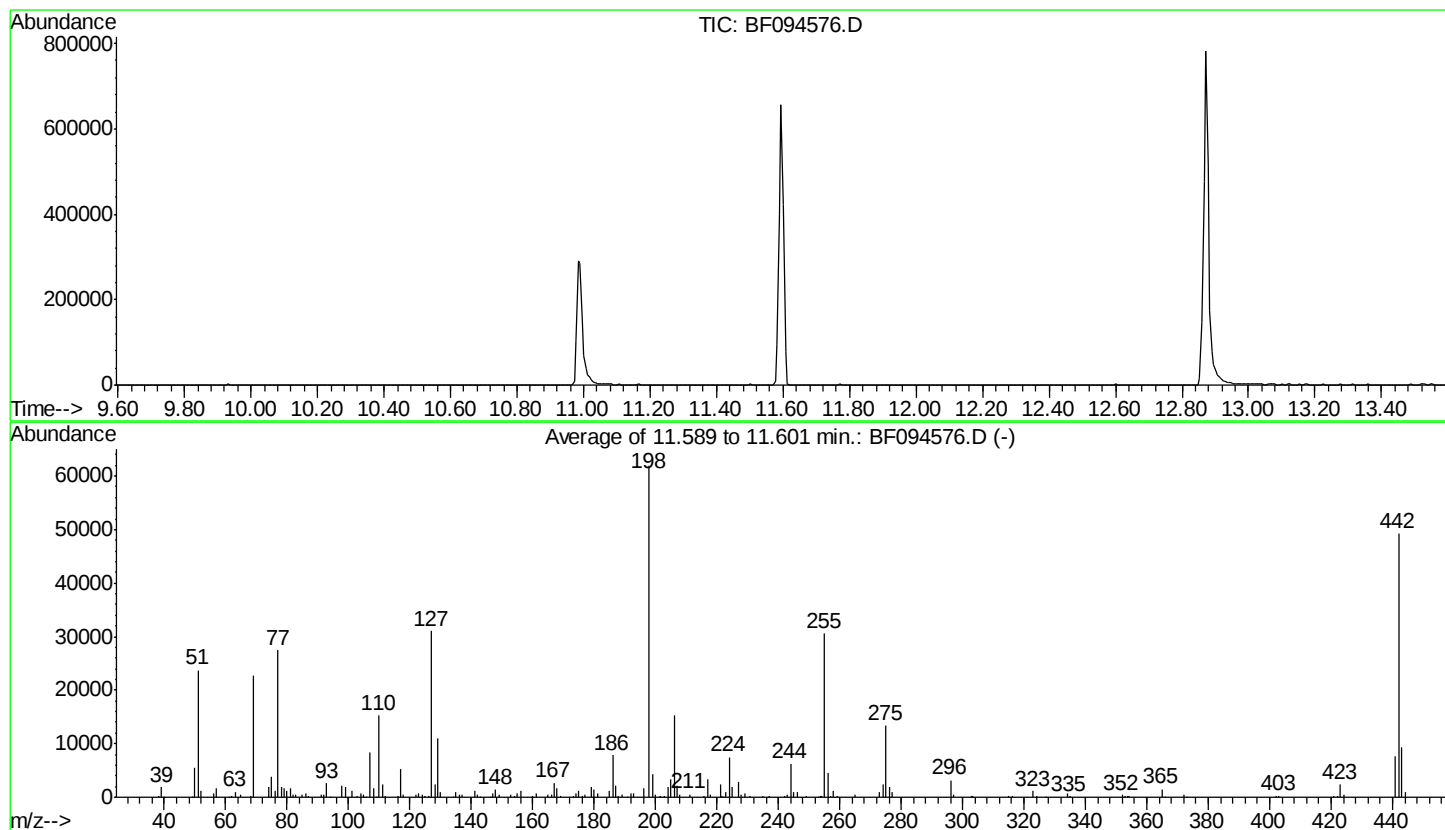

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	23687	PASS
68	69	0.00	2	1.1	258	PASS
69	198	0.00	100	36.5	22632	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	31072	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61933	PASS
199	198	5	9	7.0	4331	PASS
275	198	10	60	21.5	13325	PASS
365	198	1	100	2.3	1453	PASS
441	442	0.01	24	15.4	7583	PASS
442	198	50	100	79.4	49160	PASS
443	442	15	24	19.0	9331	PASS