
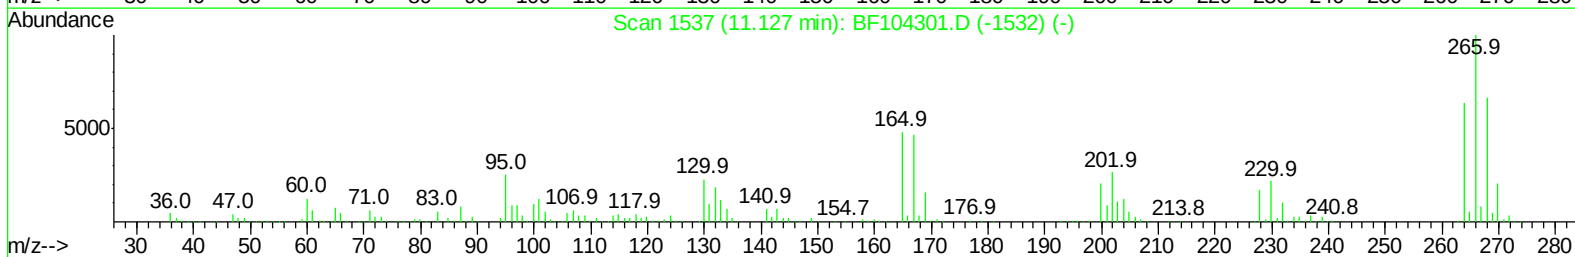
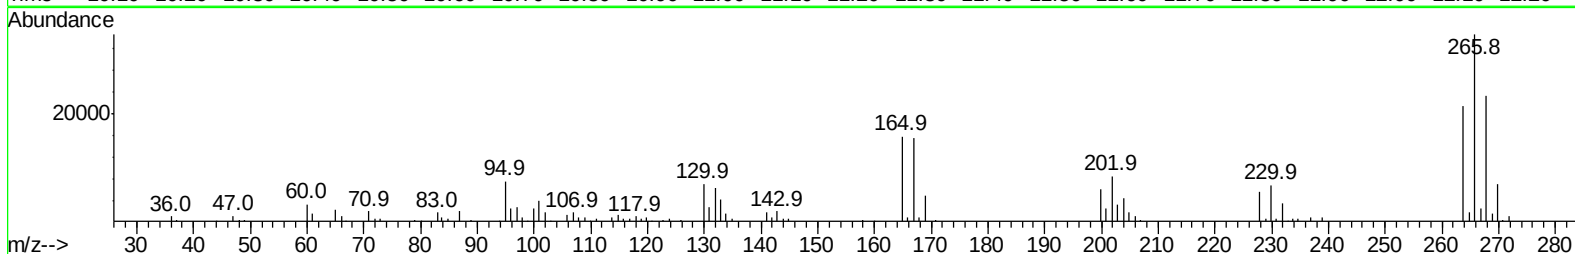


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042418\
Data File : BF104750.D
Acq On : 24 Apr 2018 12:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 04:37:26 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 15:38:25 2018
Response via : Initial Calibration

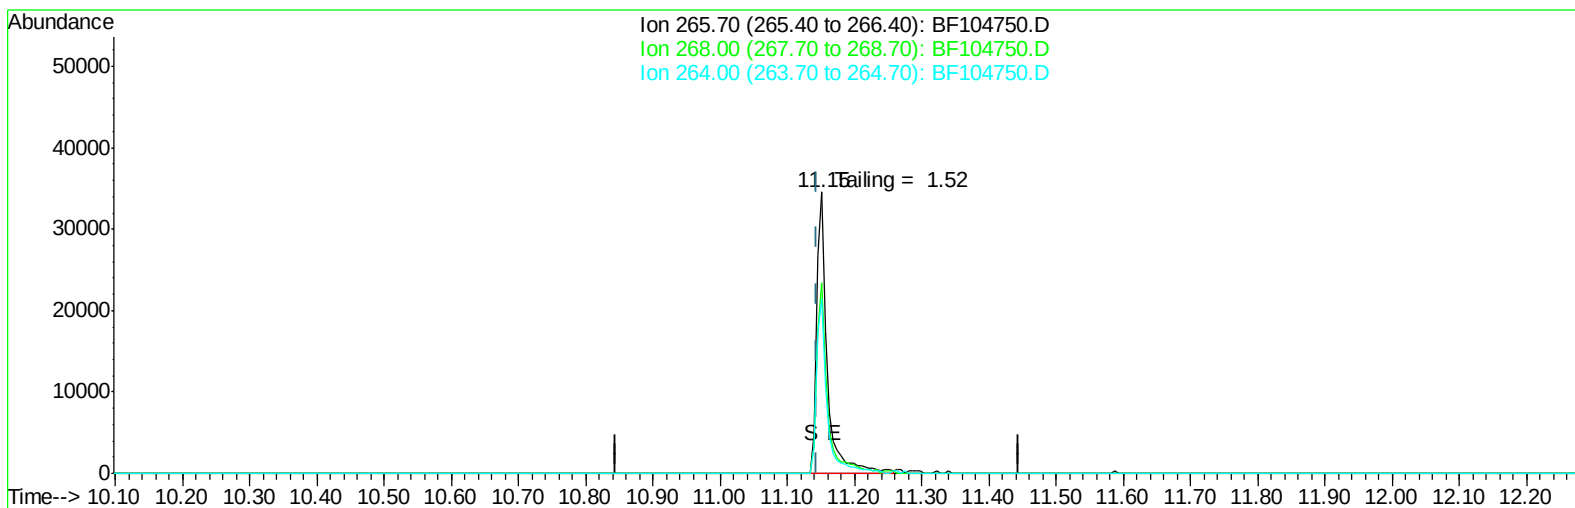

TIC: BF104750.D

(69) Pentachlorophenol (C)




11.151min (+0.006) 19864.17ng

response 39271

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.74
264.00	61.90	61.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042418\
Data File : BF104750.D
Acq On : 24 Apr 2018 12:00
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 04:37:26 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 15:38:25 2018
Response via : Initial Calibration

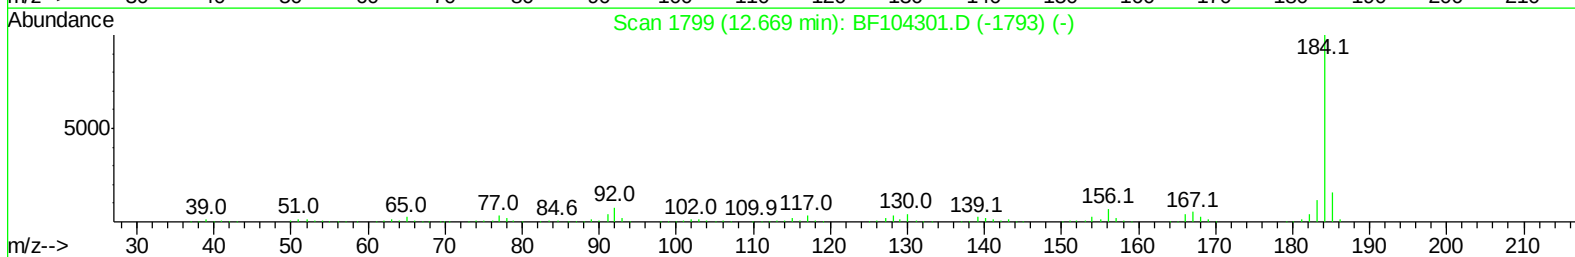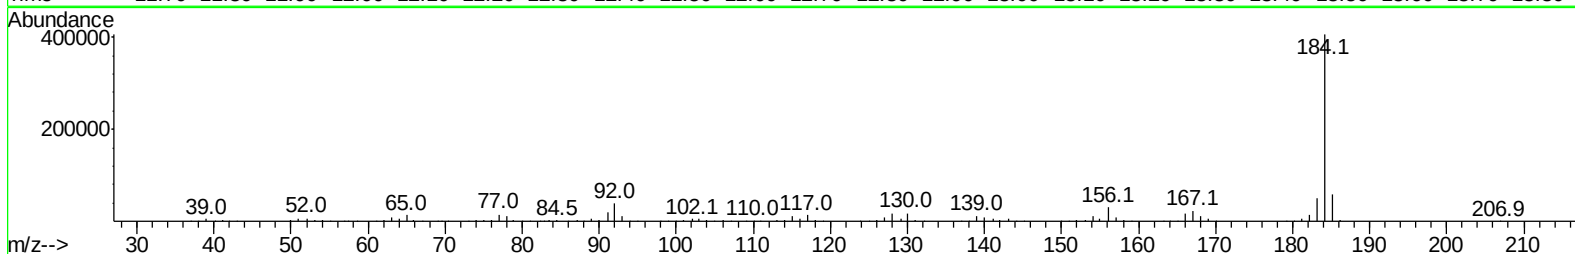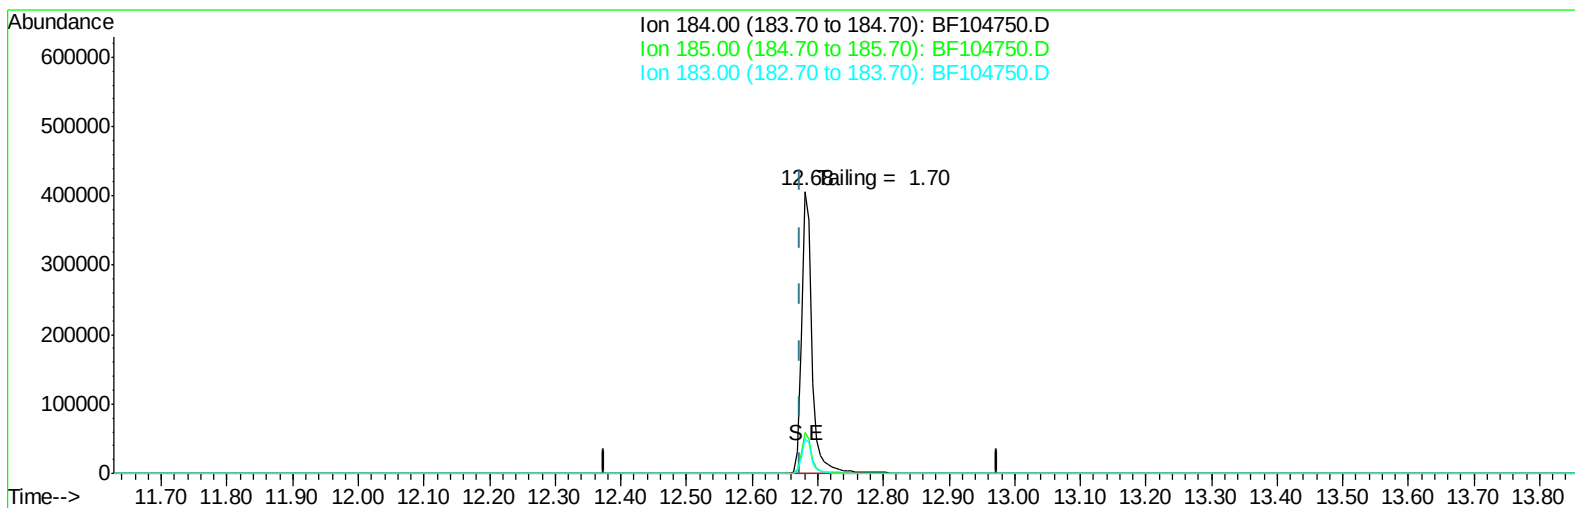

TIC: BF104750.D

(76) Benzidine

12.680min (+0.006) 0.00ng

response 451142

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.34
183.00	11.60	12.26
0.00	0.00	0.00