
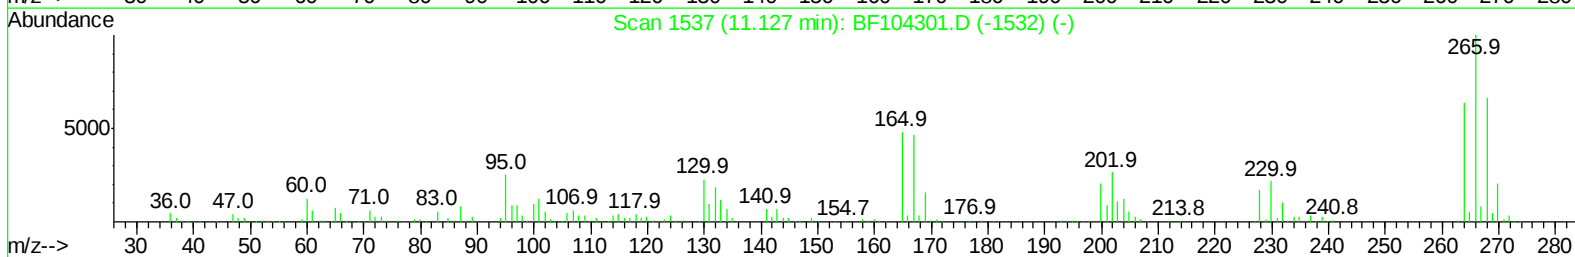
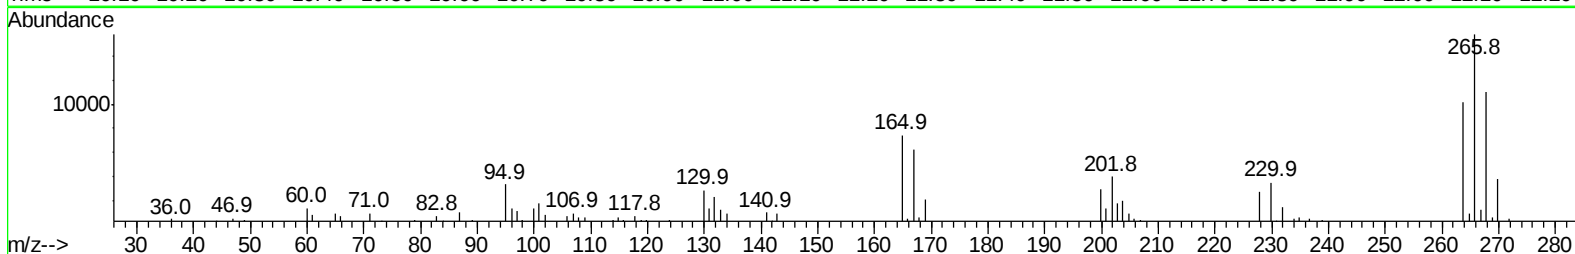


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042418\
Data File : BF104776.D
Acq On : 25 Apr 2018 1:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 04:39:29 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 15:38:25 2018
Response via : Initial Calibration

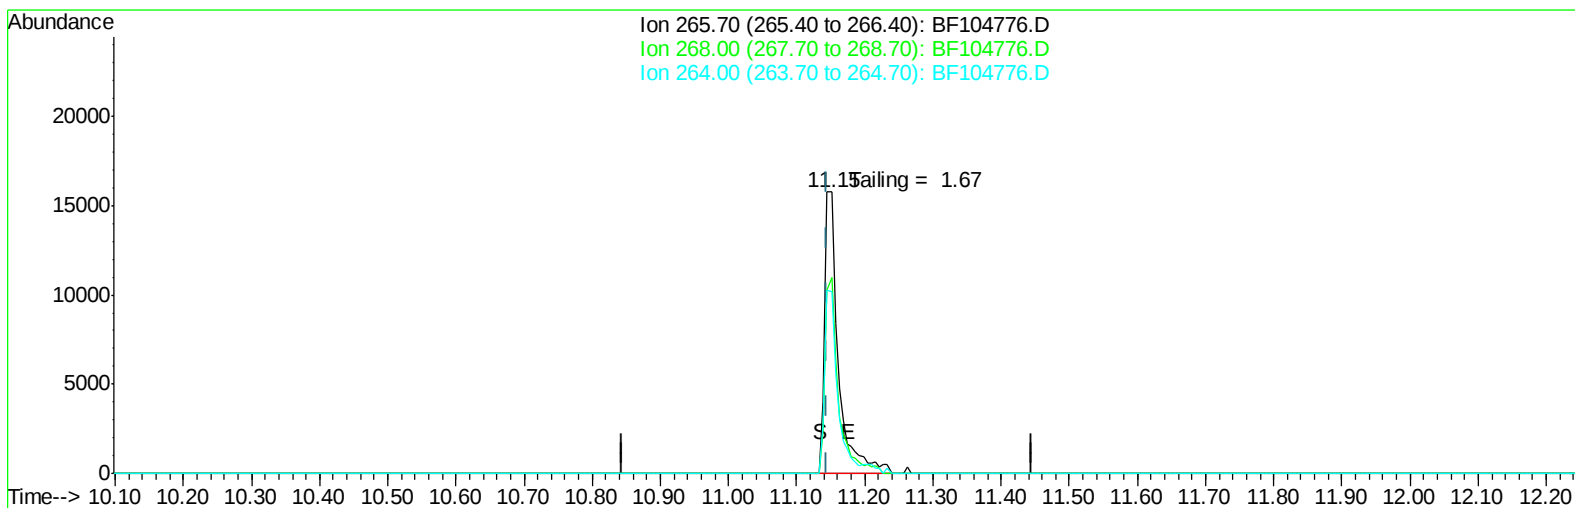

TIC: BF104776.D

(69) Pentachlorophenol (C)




11.151min (+0.006) 26178.71ng

response 21516

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.67
264.00	61.90	64.48
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\DATA\BF042418\  
Data File : BF104776.D  
Acq On    : 25 Apr 2018    1:03  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 25 04:39:29 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 23 15:38:25 2018
Response via : Initial Calibration

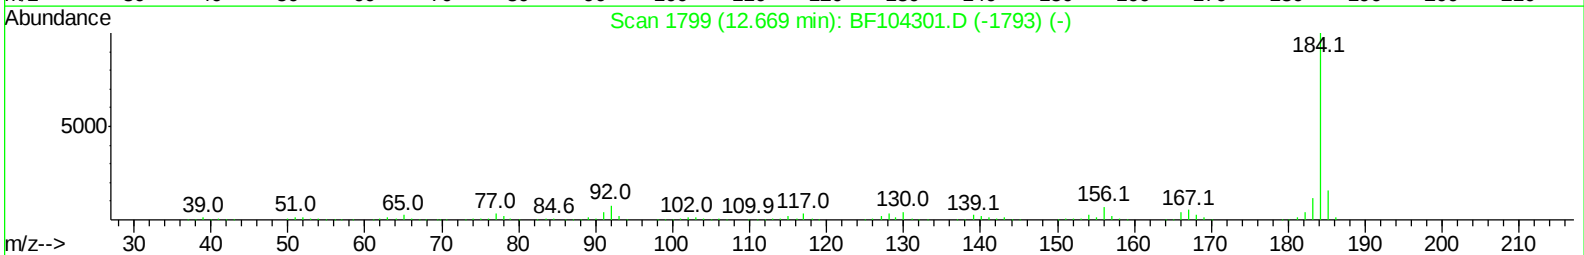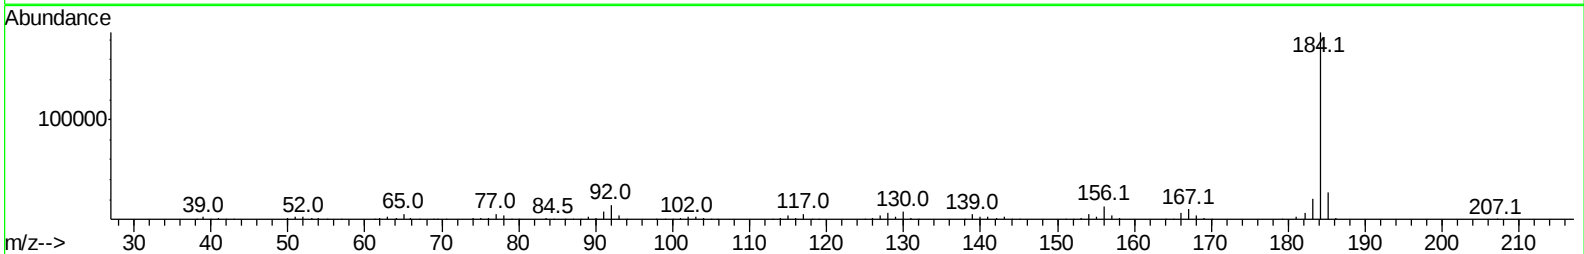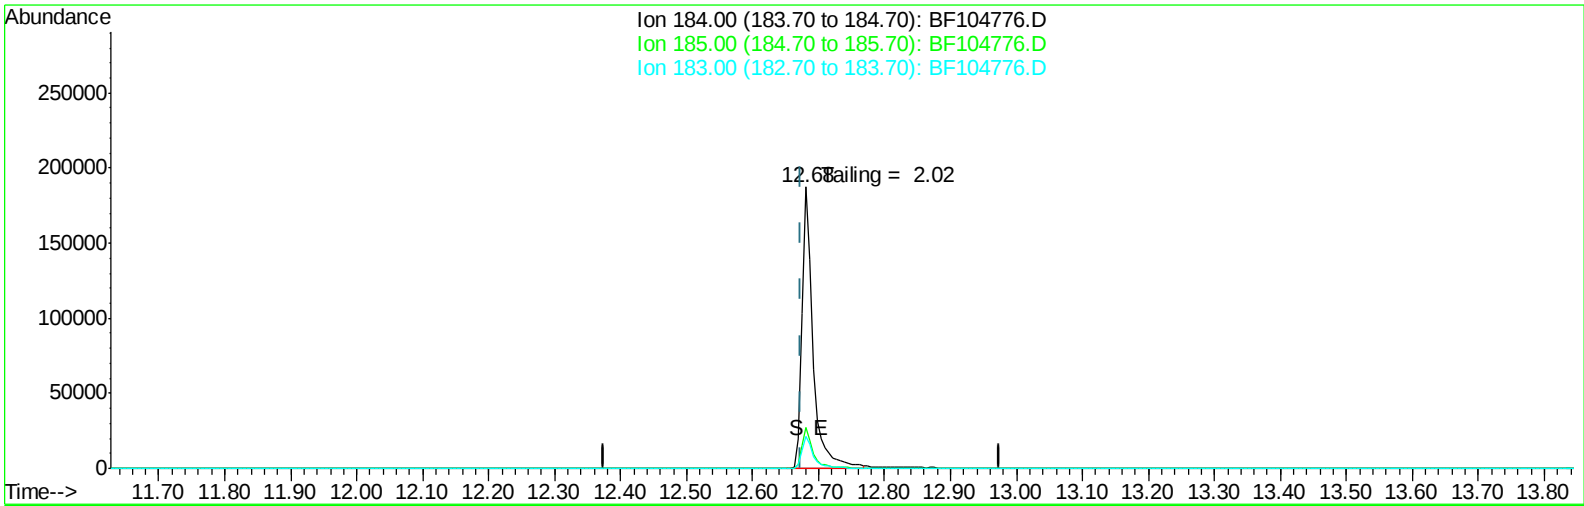

TIC: BF104776.D

(76) Benzidine

12.680min (+0.006) 0.00ng

response 225290

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.62
183.00	11.60	11.37
0.00	0.00	0.00