


Data Path : Z:\HPCHEM1\BNA F\Data\BF042418\
 Data File : BF104776.D
 Acq On : 25 Apr 2018 1:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 25 14:01:50 2018

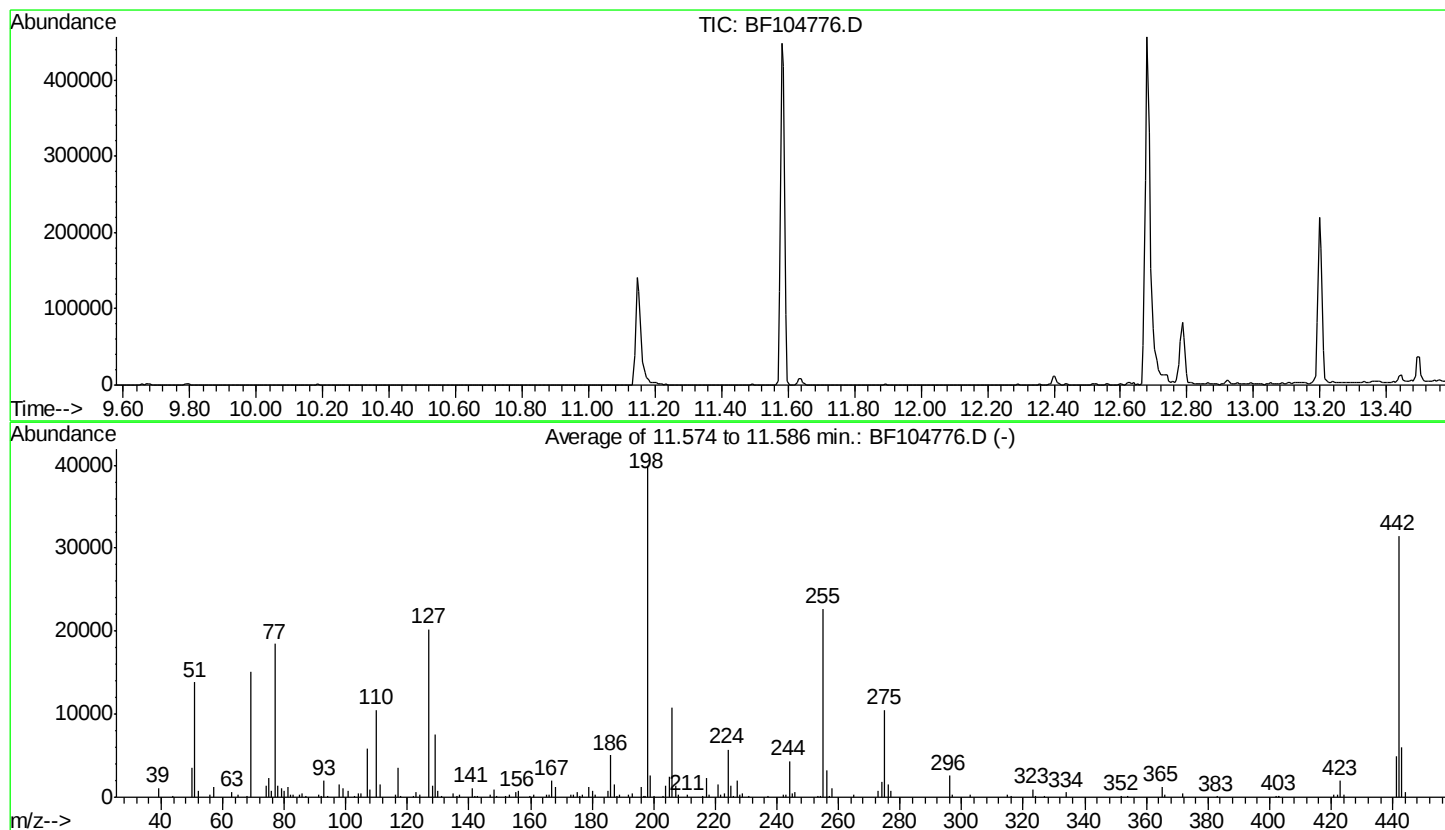

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	13812	PASS
68	69	0.00	2	0.9	137	PASS
69	198	0.00	100	37.8	15107	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.6	20232	PASS
197	198	0.00	2	0.5	202	PASS
198	198	100	100	100.0	39949	PASS
199	198	5	9	6.6	2645	PASS
275	198	10	60	26.3	10526	PASS
365	198	1	100	3.2	1259	PASS
441	443	0.01	100	83.7	5006	PASS
442	198	50	100	78.8	31466	PASS
443	442	15	24	19.0	5979	PASS