


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042419\
 Data File : BF113949.D
 Acq On : 24 Apr 2019 9:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 23 03:32:35 2019

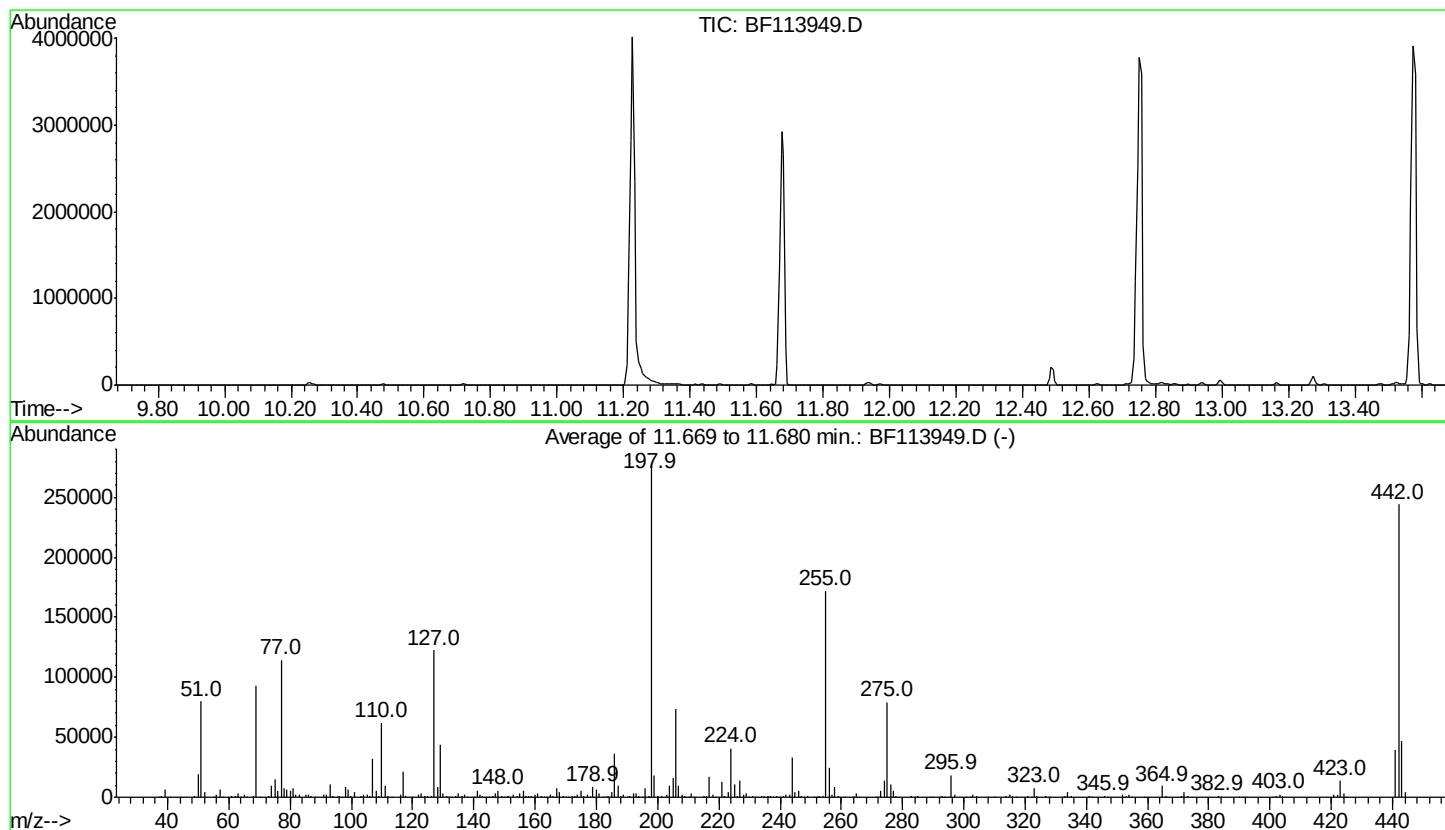

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	79605	PASS
68	69	0.00	2	1.7	1587	PASS
69	198	0.00	100	33.5	92621	PASS
70	69	0.00	2	0.5	481	PASS
127	198	10	80	44.3	122520	PASS
197	198	0.00	2	0.4	1035	PASS
198	198	100	100	100.0	276352	PASS
199	198	5	9	6.7	18502	PASS
275	198	10	60	28.7	79424	PASS
365	198	1	100	3.4	9303	PASS
441	198	0.01	100	14.3	39402	PASS
442	198	50	100	88.2	243832	PASS
443	442	15	24	19.2	46830	PASS