
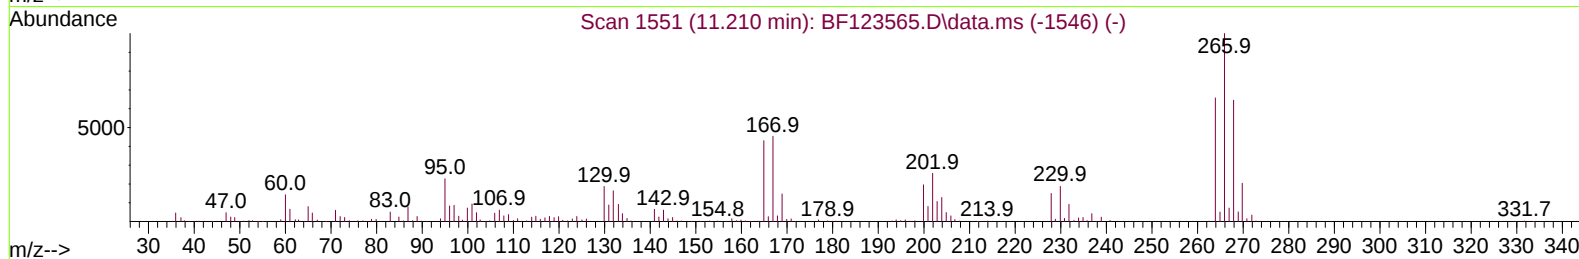
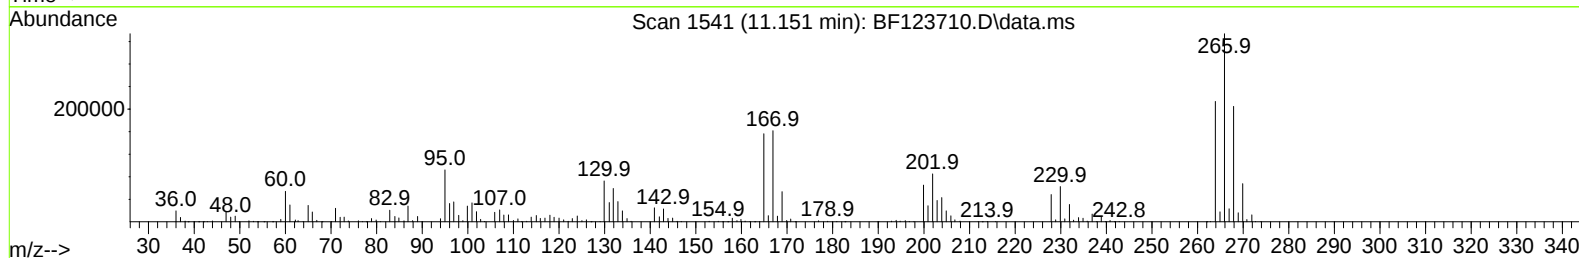


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042421\
Data File : BF123710.D
Acq On : 24 Apr 2021 10:34
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 08:56:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 05:40:49 2021
Response via : Initial Calibration

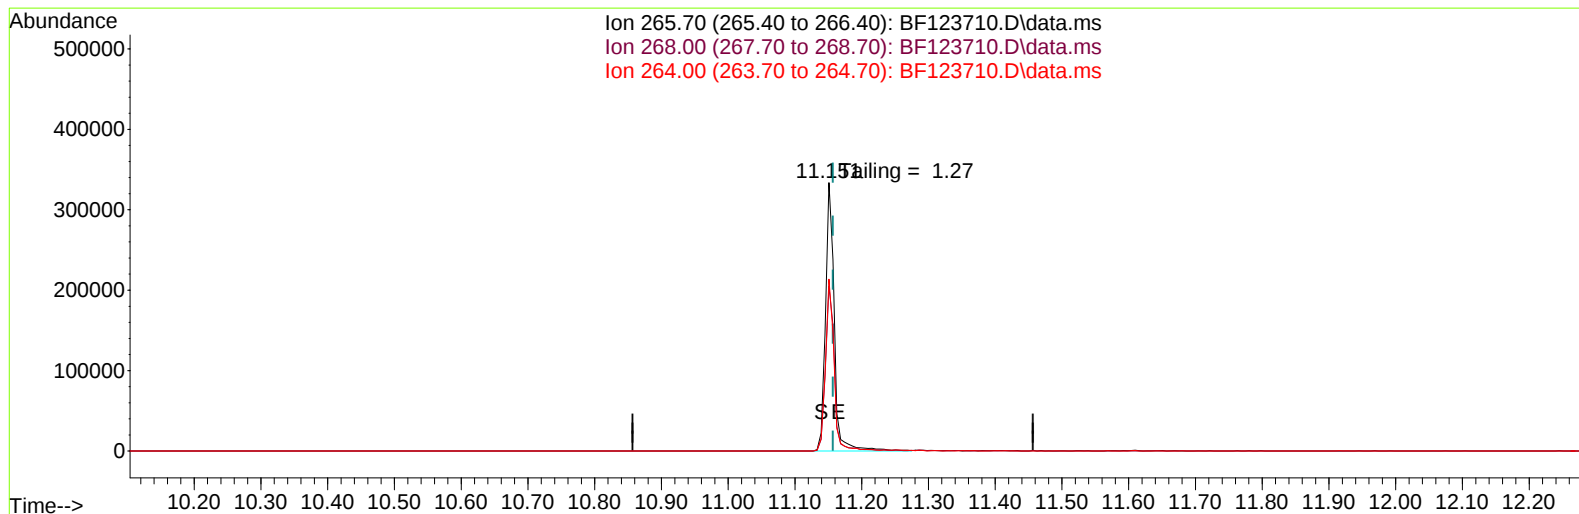

TIC: BF123710.D\data.ms

(70) Pentachlorophenol (C)




11.151min (-0.006) 28572.68 ng

response 303764

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	61.40
264.00	65.70	64.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042421\
Data File : BF123710.D
Acq On : 24 Apr 2021 10:34
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 08:56:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 05:40:49 2021
Response via : Initial Calibration

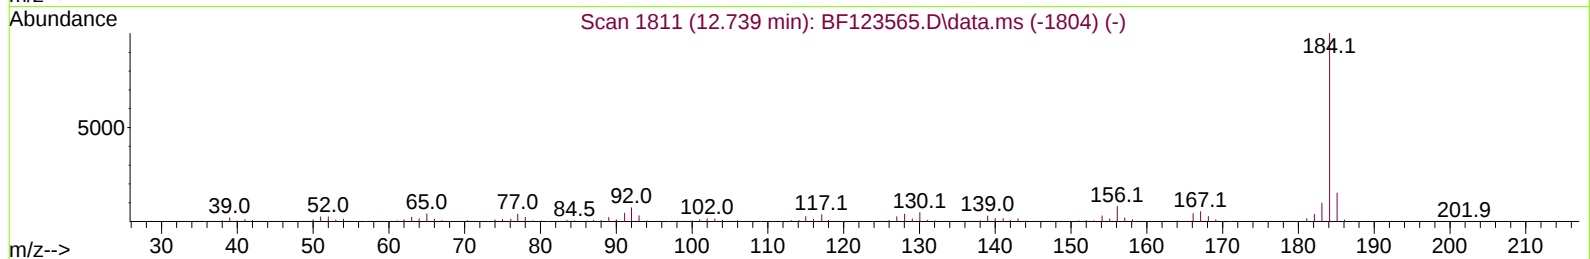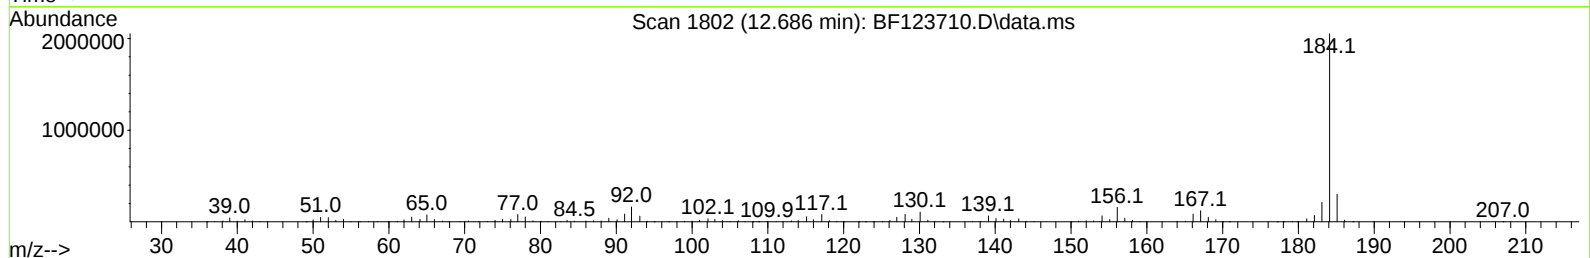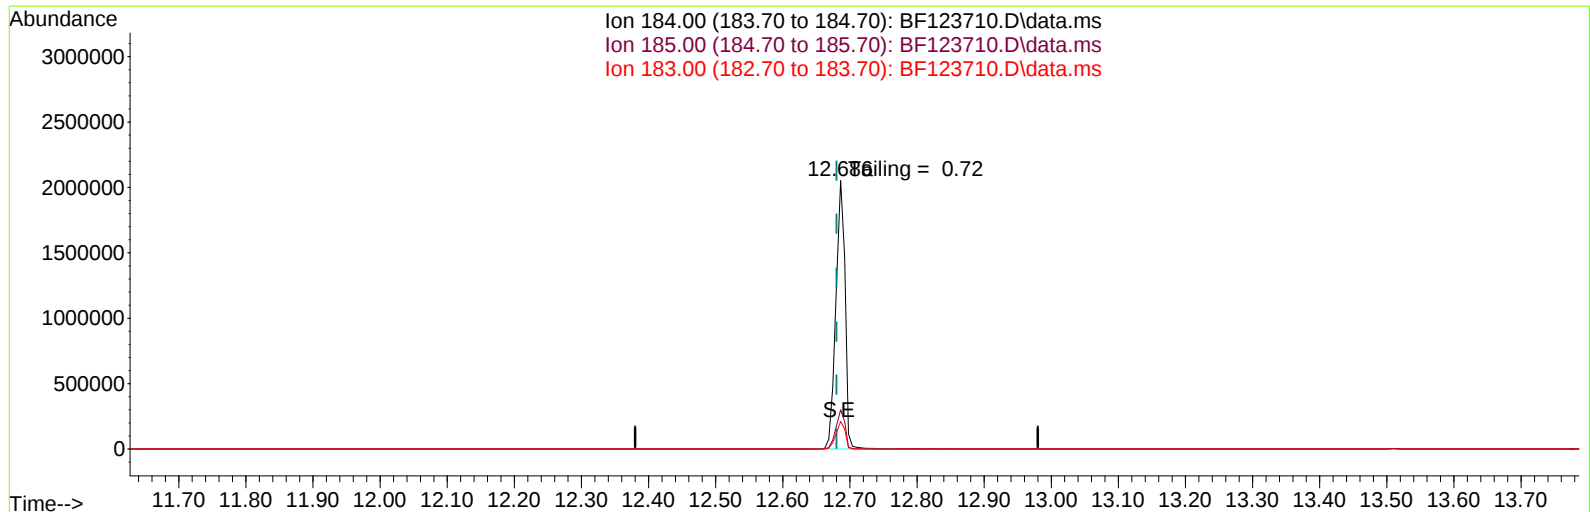

TIC: BF123710.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response 1964772

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.64
183.00	9.80	10.29
0.00	0.00	0.00