
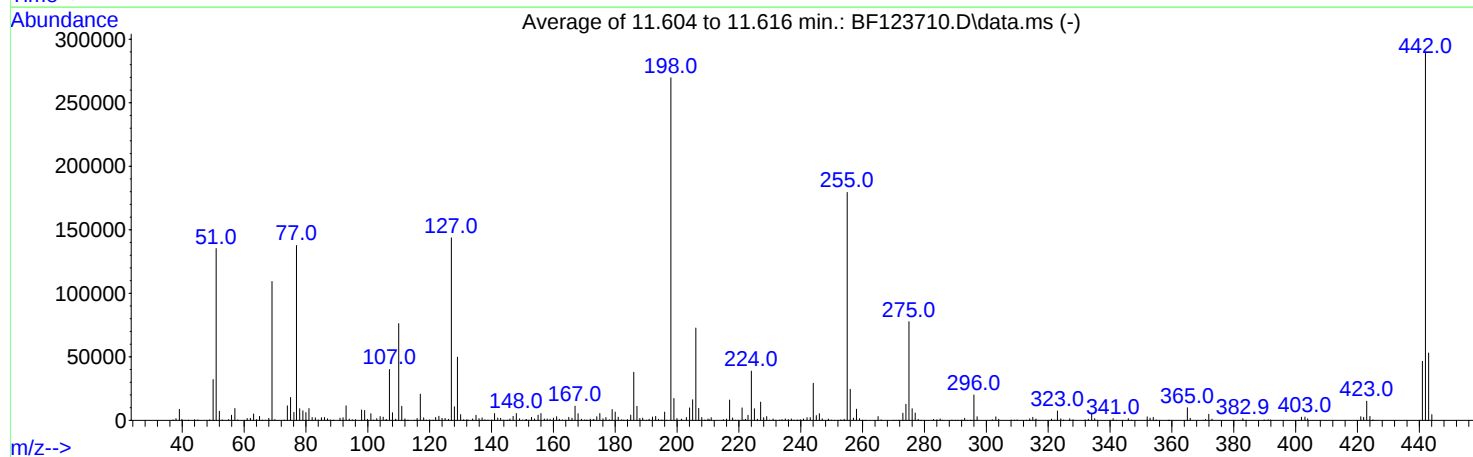


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042421\
 Data File : BF123710.D
 Acq On : 24 Apr 2021 10:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 26 05:40:49 2021

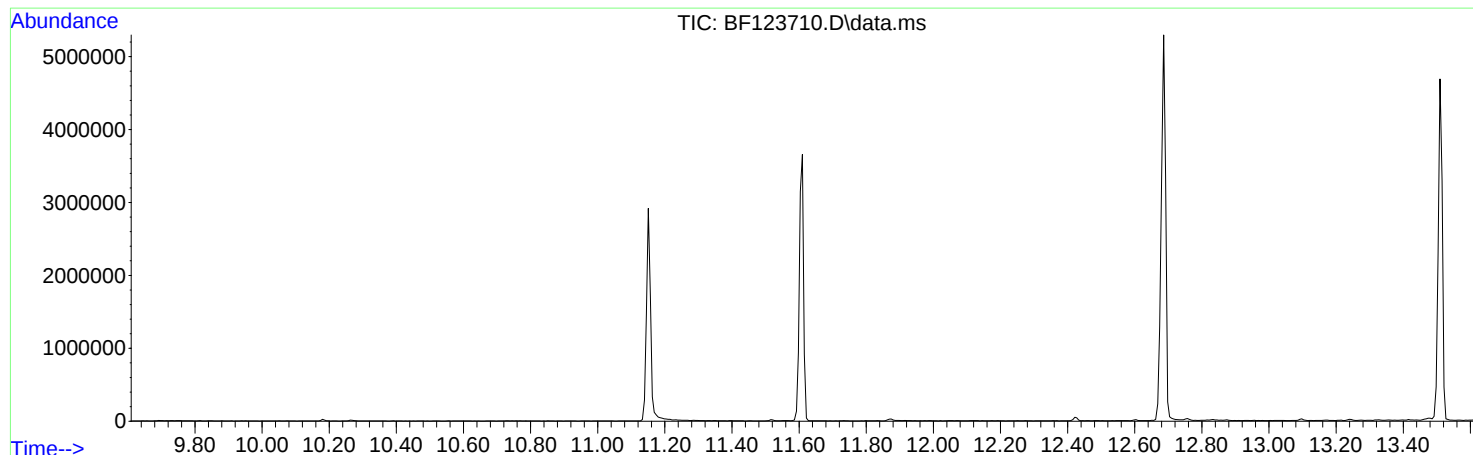




AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	135291	PASS
68	69	0.00	2	1.6	1703	PASS
69	198	0.00	100	40.6	109373	PASS
70	69	0.00	2	0.6	603	PASS
127	198	10	80	53.3	143765	PASS
197	198	0.00	2	0.0	120	PASS
198	198	100	100	100.0	269669	PASS
199	198	5	9	6.4	17282	PASS
275	198	10	60	28.8	77715	PASS
365	198	1	100	3.7	9947	PASS
441	198	0.01	100	17.2	46493	PASS
442	442	50	100	100.0	289557	PASS
443	442	15	24	18.3	53043	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042421\
Data File : BF123710.D
Acq On : 24 Apr 2021 10:34
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 26 08:56:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 05:40:49 2021
Response via : Initial Calibration

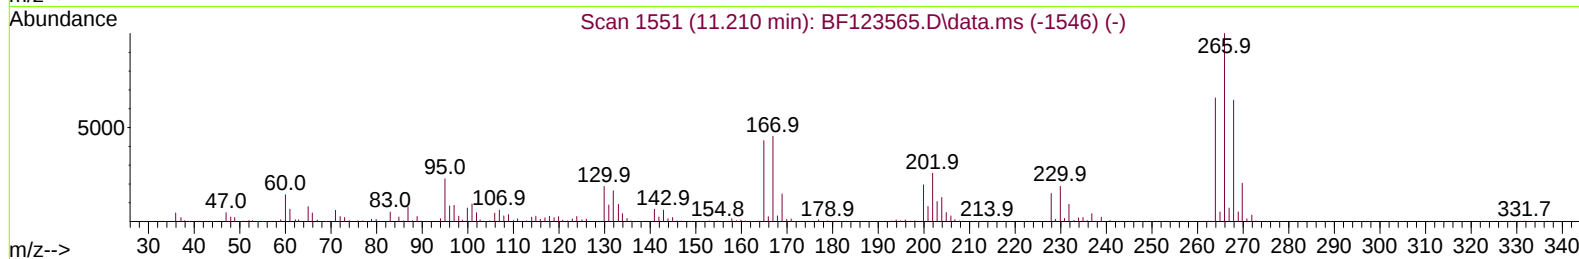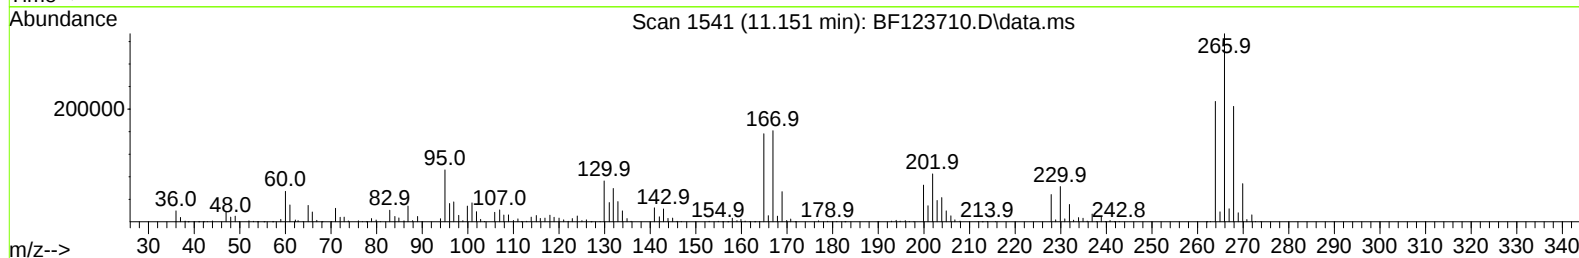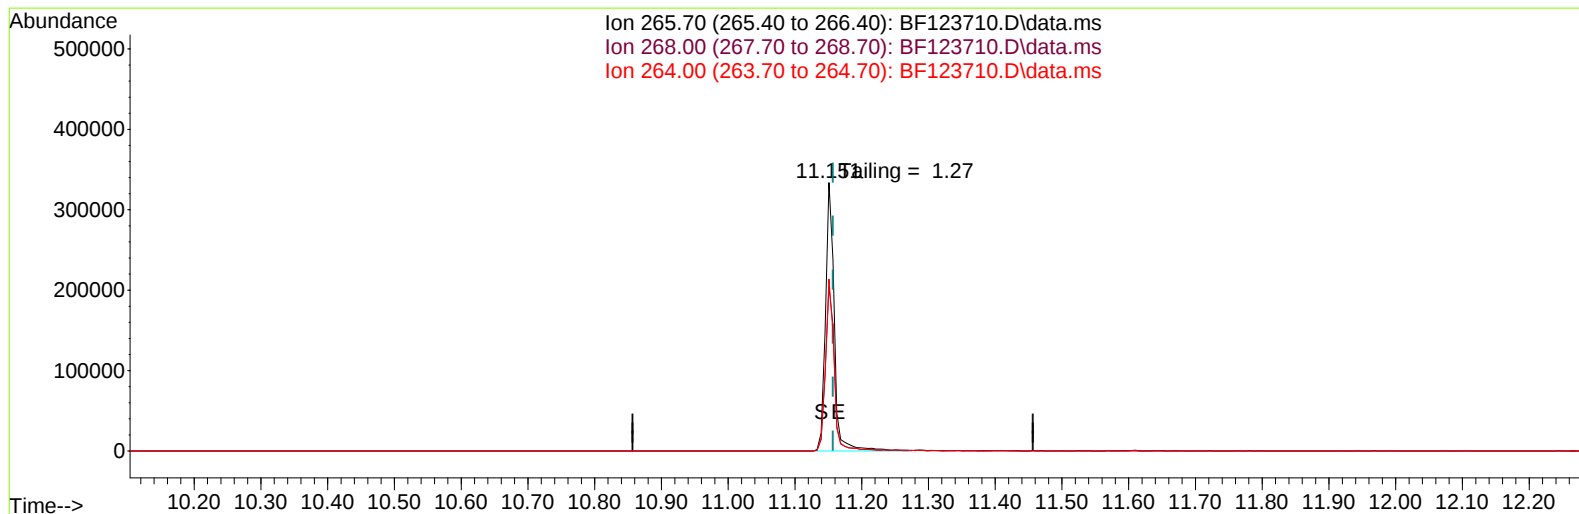

TIC: BF123710.D\data.ms




(70) Pentachlorophenol (C)

11.151min (-0.006) 28572.68 ng

response 303764

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	61.40
264.00	65.70	64.05
0.00	0.00	0.00

Quant Time: Apr 26 08:56:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF041521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 05:40:49 2021
Response via : Initial Calibration

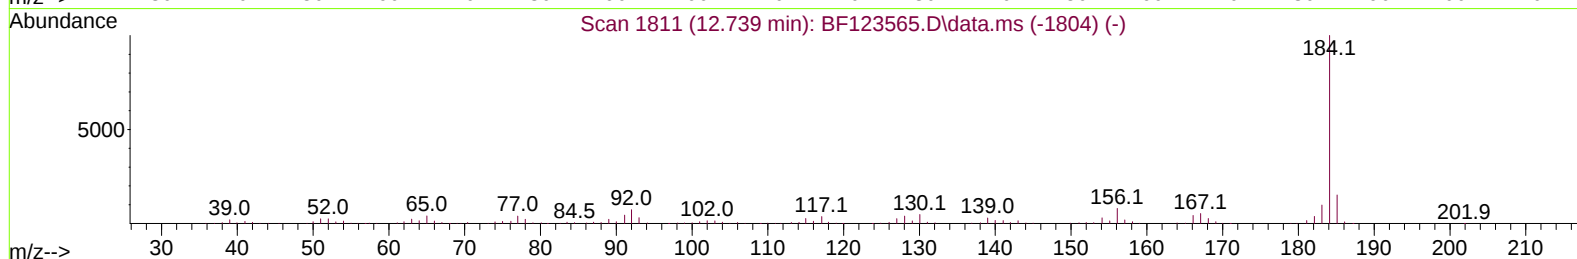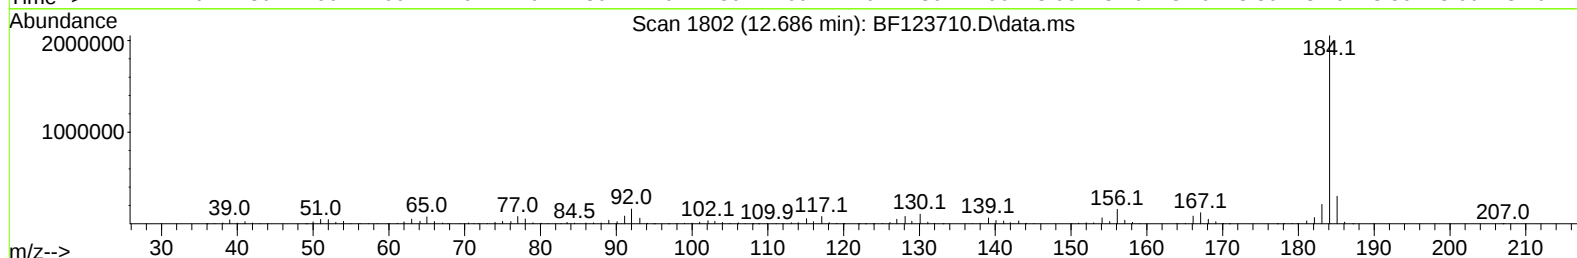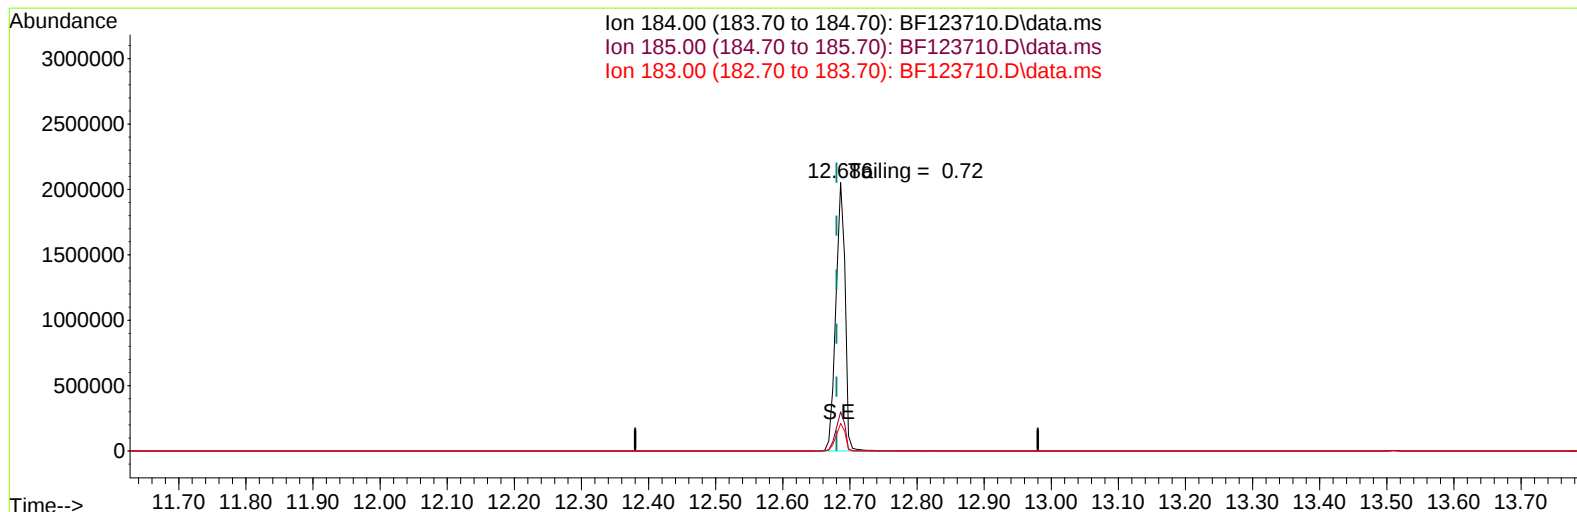

TIC: BF123710.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 0.00 ng

response **1964772**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.64
183.00	9.80	10.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/24/2021	BNA_F	<u>BF123710.D</u>
Compound Name	Response	Retention Time
DDT	443935	13.51
DDD	3396	13.239
DDE	1035	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4431	448366	0.99