
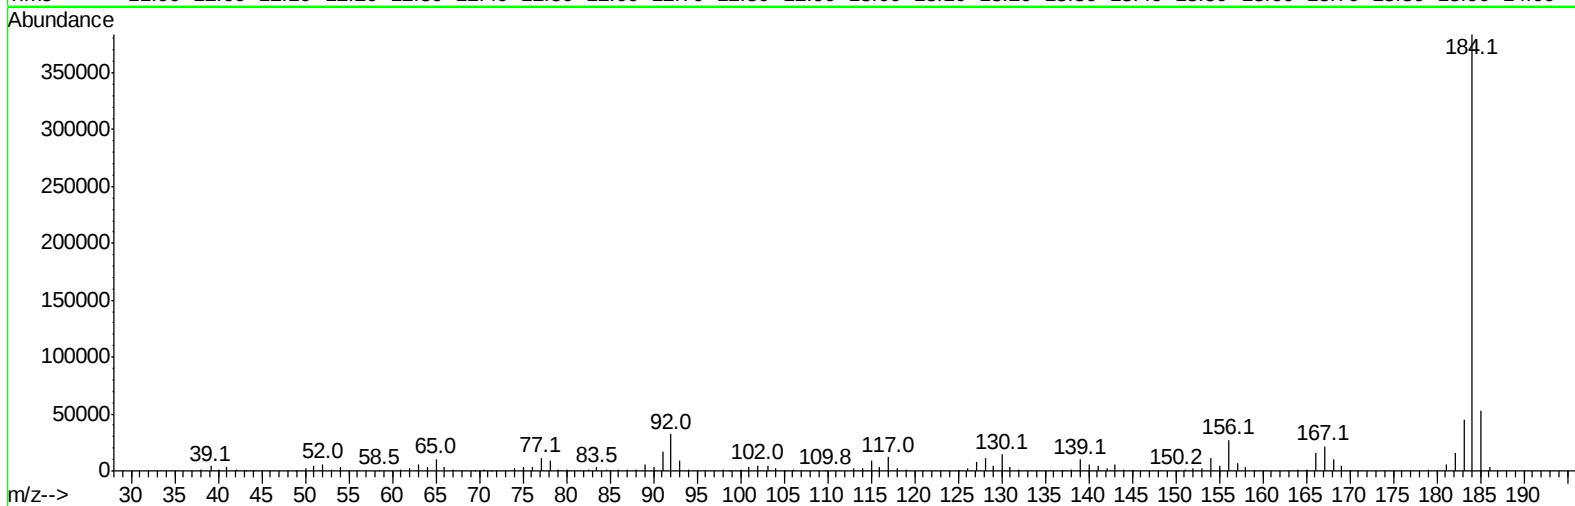


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042517\
Data File : BF094596.D
Acq On : 25 Apr 2017 10:52
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 08:57:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

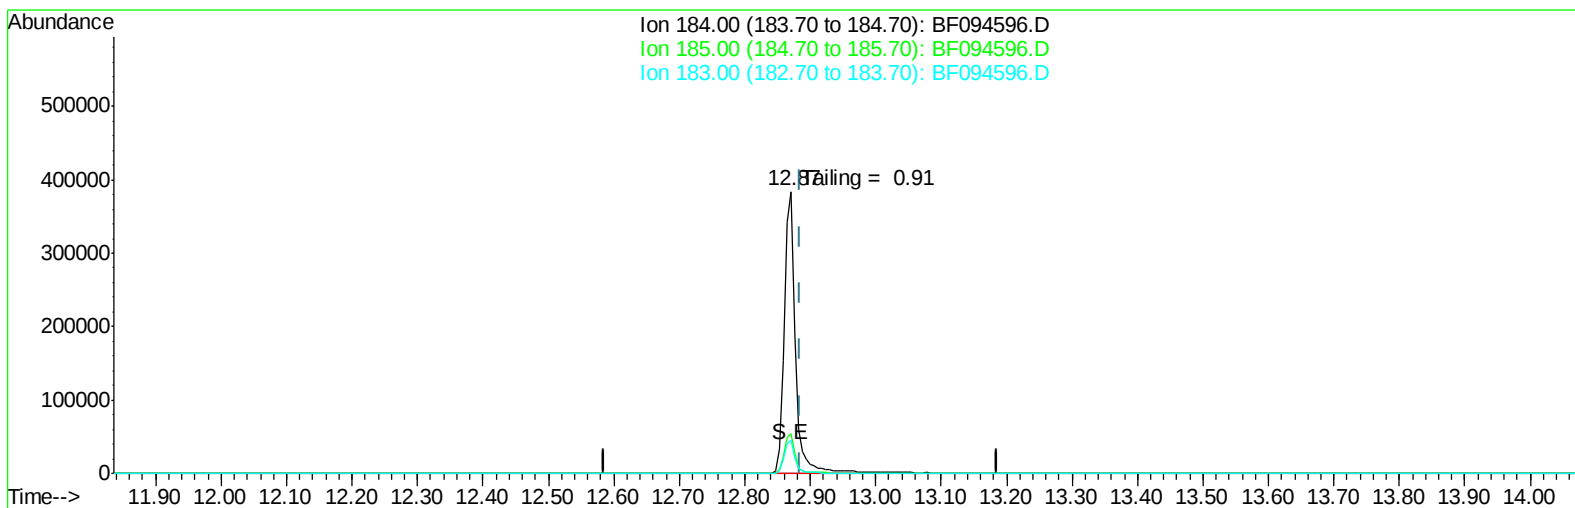

TIC: BF094596.D

(76) Benzidine



12.871min (-0.015) 0.00ng

response 462518

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.92#
183.00	12.20	11.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042517\
Data File : BF094596.D
Acq On : 25 Apr 2017 10:52
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 08:57:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

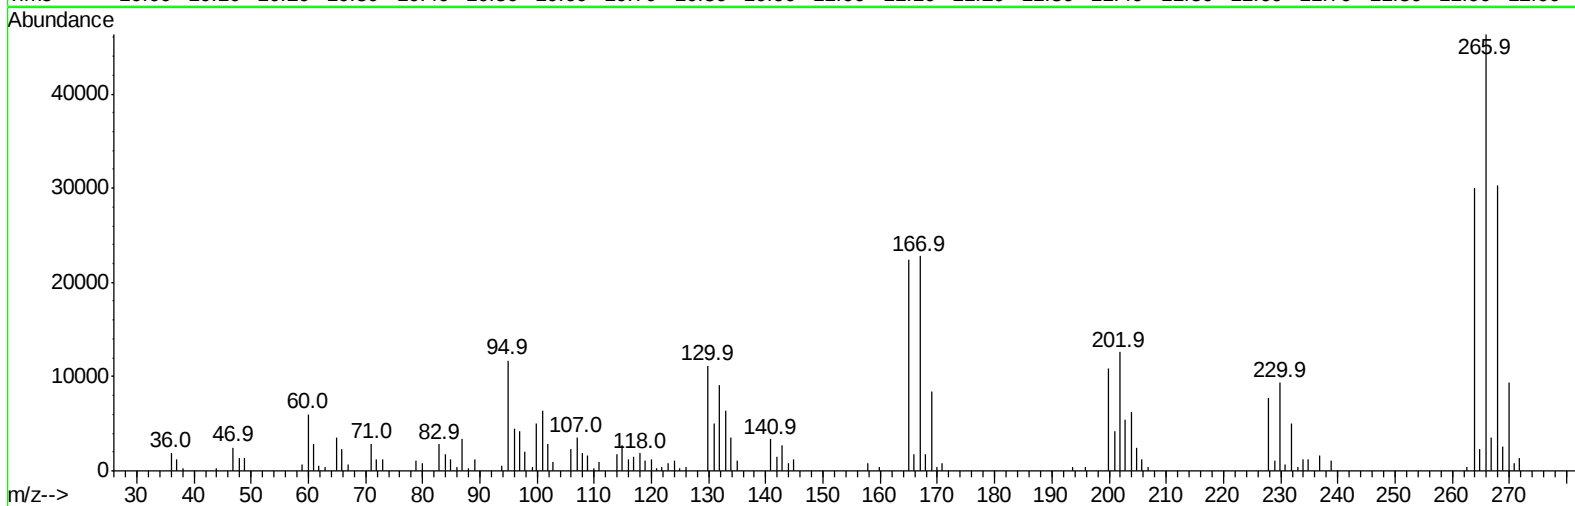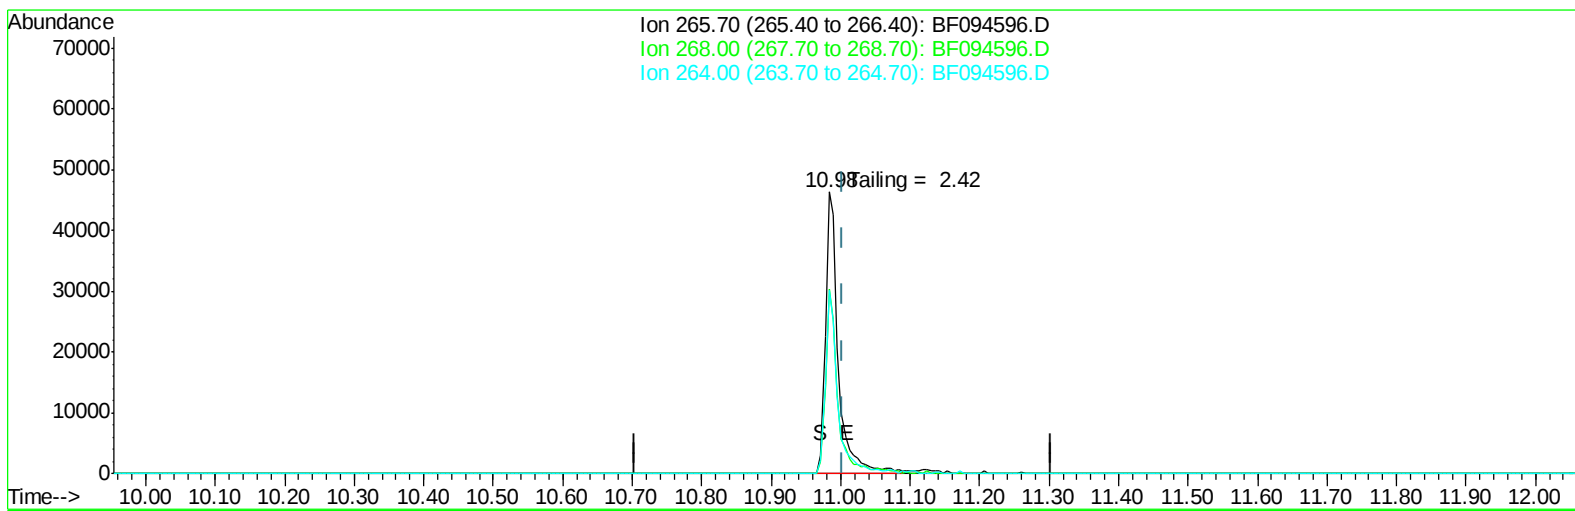

TIC: BF094596.D

(69) Pentachlorophenol (C)

10.983min (-0.021) 0.00ng

response 58962

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.26
264.00	64.60	64.80
0.00	0.00	0.00