
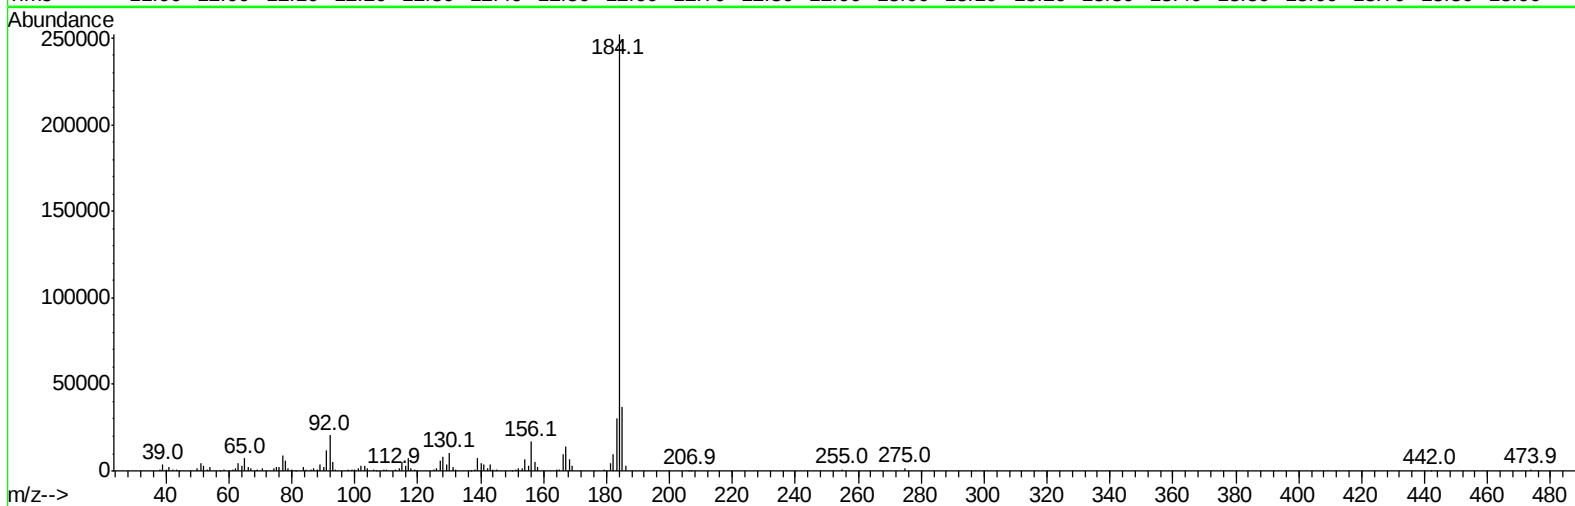


Data Path : Z:\HPCHEM1\BNA F\DATA\BF042517\
Data File : BF094622.D
Acq On : 26 Apr 2017 00:13
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 09:00:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

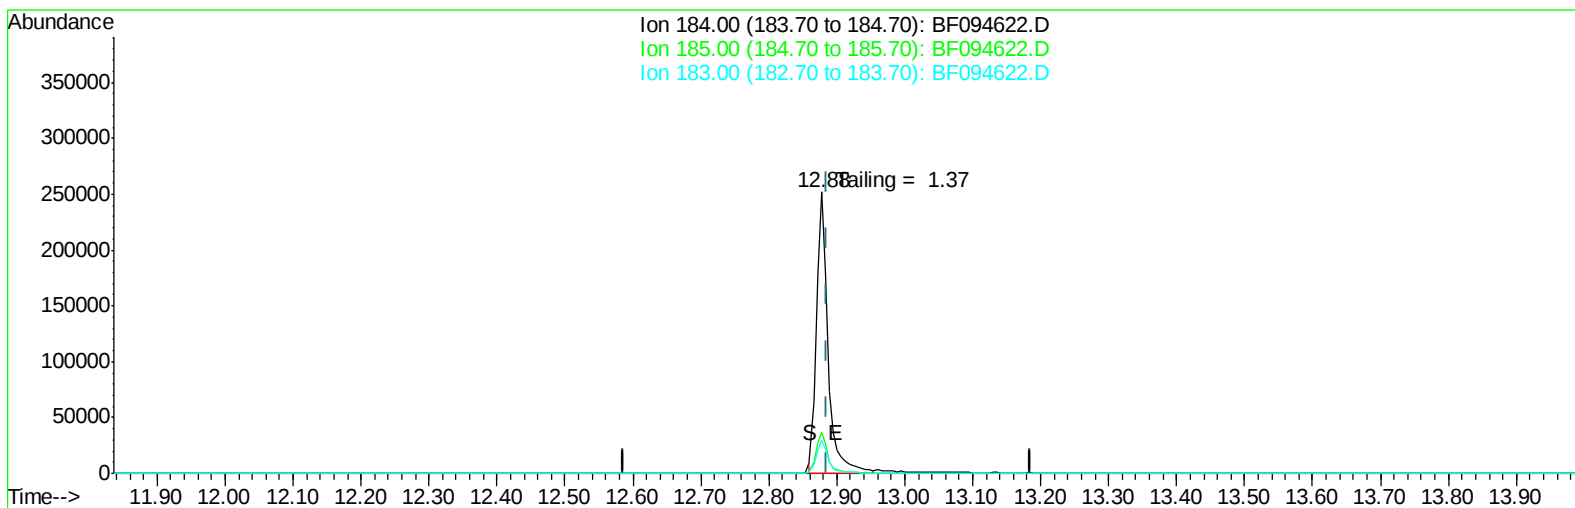

TIC: BF094622.D

(76) Benzidine



12.877min (-0.009) 0.00ng

response 312549

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.54#
183.00	12.20	11.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042517\
Data File : BF094622.D
Acq On : 26 Apr 2017 00:13
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 09:00:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF041717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 17 14:59:23 2017
Response via : Initial Calibration

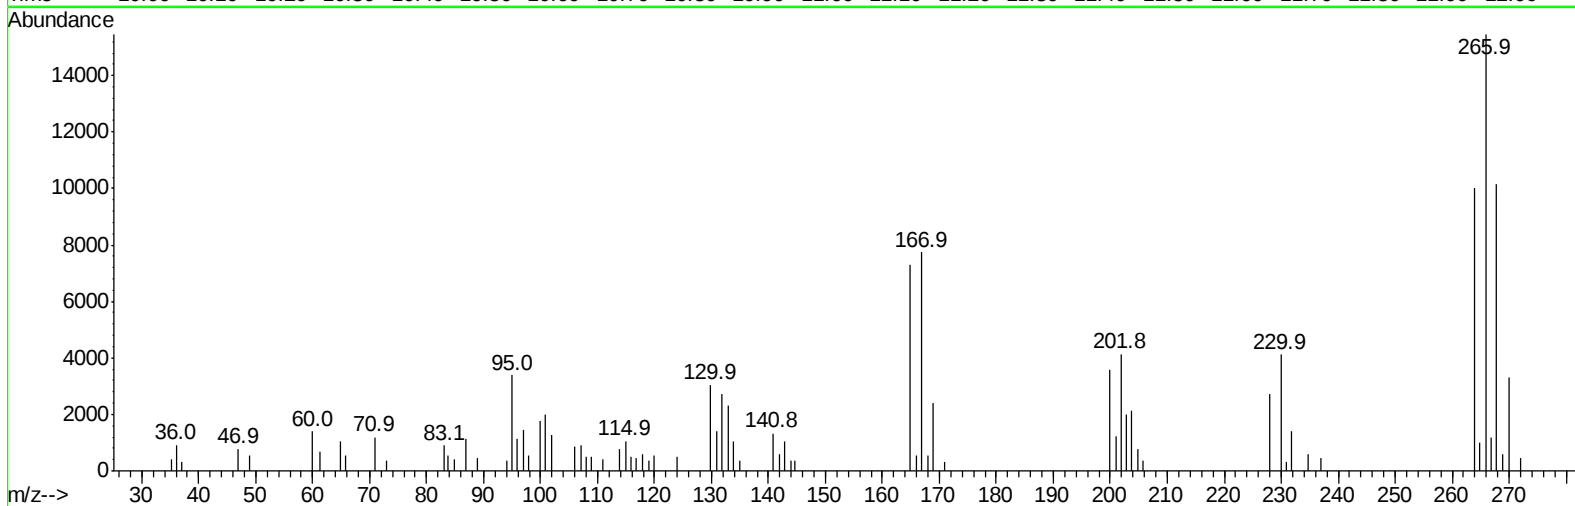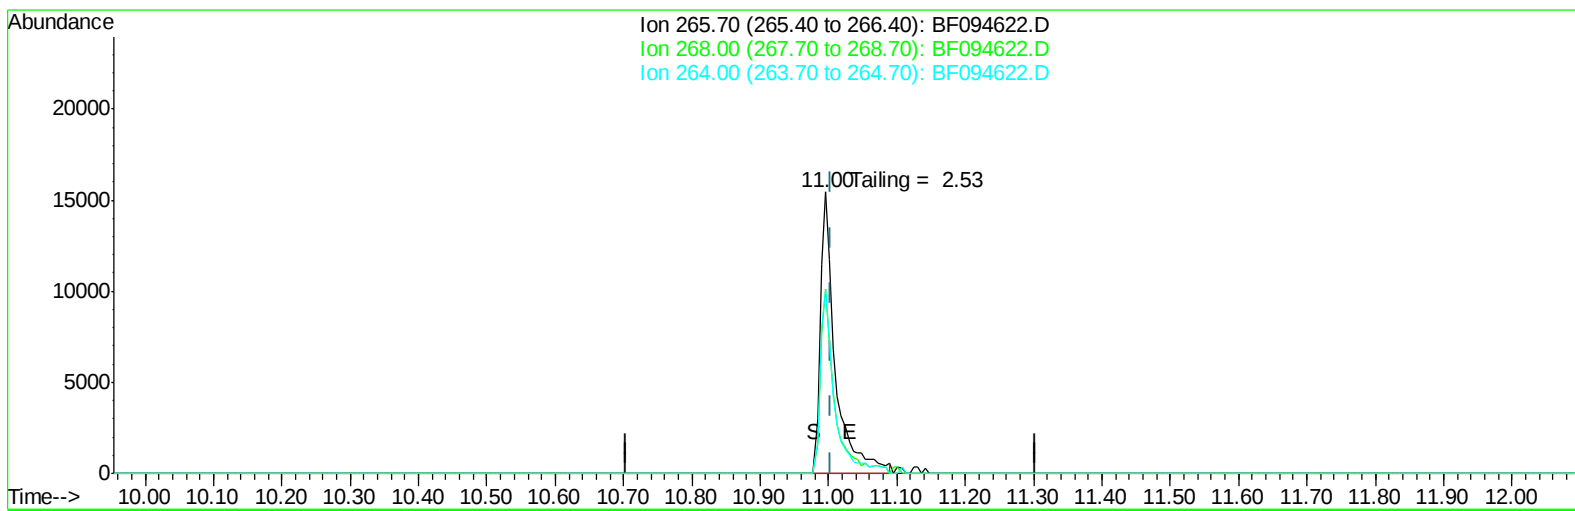

TIC: BF094622.D

(69) Pentachlorophenol (C)

10.995min (-0.009) 0.00ng

response 23882

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.62
264.00	64.60	64.86
0.00	0.00	0.00