


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF042517\
 Data File : BF094622.D
 Acq On : 26 Apr 2017 00:13
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF041717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 17 14:59:23 2017

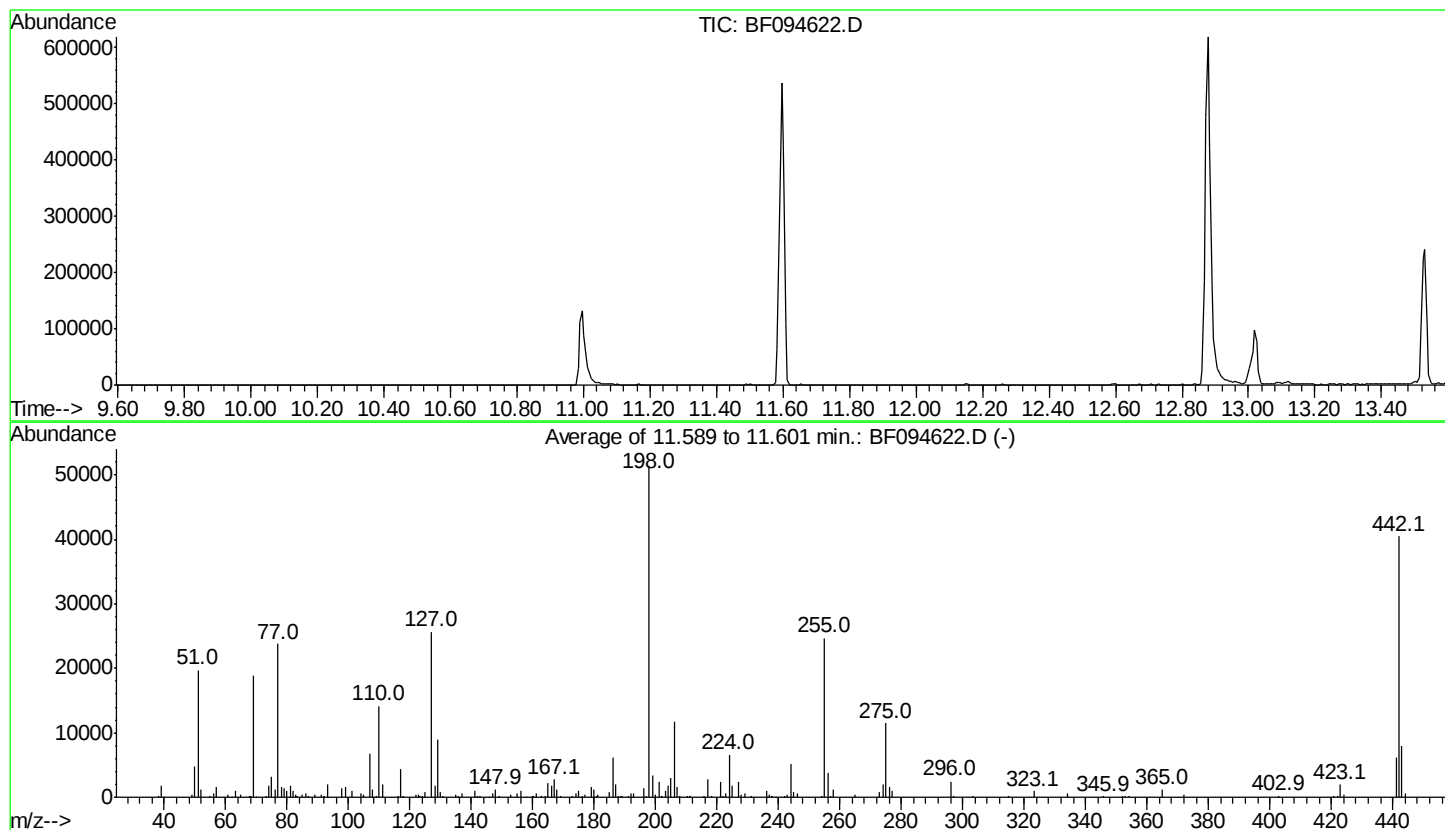

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	19661	PASS
68	69	0.00	2	1.1	202	PASS
69	198	0.00	100	36.7	18861	PASS
70	69	0.00	2	0.5	101	PASS
127	198	10	80	49.9	25682	PASS
197	198	0.00	2	0.4	210	PASS
198	198	100	100	100.0	51421	PASS
199	198	5	9	6.8	3474	PASS
275	198	10	60	22.3	11486	PASS
365	198	1	100	2.2	1112	PASS
441	442	0.01	24	15.1	6096	PASS
442	198	50	100	78.7	40493	PASS
443	442	15	24	19.6	7954	PASS