

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042518\
 Data File : BF104792.D
 Acq On : 25 Apr 2018 16:46
 Operator : JU/SJ
 Sample : J2505-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 26 08:13:13 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 25 14:01:50 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	122693	20.00	ng	0.00
21) Naphthalene-d8	8.08	136	495739	20.00	ng	0.00
38) Acenaphthene-d10	9.84	164	217002	20.00	ng	0.00
63) Phenanthrene-d10	11.33	188	341766	20.00	ng	0.00
75) Chrysene-d12	13.98	240	215335	20.00	ng	0.00
86) Perylene-d12	15.45	264	186907	20.00	ng	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.42	112	843592	105.13	ng	0.00
7) Phenol-d6	6.45	99	1032763	104.75	ng	0.00
23) Nitrobenzene-d5	7.37	82	648257	85.39	ng	0.00
41) 2,4,6-Tribromophenol	10.64	330	230142	102.24	ng	0.00
44) 2-Fluorobiphenyl	9.16	172	982033	71.49	ng	0.00
78) Terphenyl-d14	12.92	244	730608	77.35	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.35	77	4942	Below Cal		# 1
18) Hexachloroethane	7.33	117	16101	4.722	ng	# 1
19) n-Nitroso-di-n-propylamine	7.37	70	89571	13.903	ng	# 75
22) Acetophenone	7.19	105	35219	2.886	ng	# 59
25) Isophorone	7.37	82	646833	40.291	ng	# 64
37) 2-Methylnaphthalene	8.80	142	53989	3.381	ng	97
49) Dimethylphthalate	9.55	163	170283	9.951	ng	99
57) Fluorene	10.39	166	29114	2.082	ng	94
64) 4,6-Dinitro-2-methylphenol	10.63	198	514	7.609	ng	# 1
66) 4-Bromophenyl-phenylether	10.63	248	14128	3.886	ng	# 1
70) Phenanthrene	11.36	178	176366	9.266	ng	96
71) Anthracene	11.40	178	47853	2.473	ng	97
74) Fluoranthene	12.55	202	181962	9.150	ng	98
76) Benzidine	12.92	184	11274	Below Cal		95
77) Pyrene	12.78	202	162100	10.156	ng	99
80) Benzo(a)anthracene	13.97	228	78183	6.077	ng	97
82) Chrysene	13.97	228	78183	5.917	ng	96
85) Indeno(1,2,3-cd)pyrene	16.91	276	24962	2.224	ng	93
87) Benzo(b)fluoranthene	15.02	252	96892	8.208	ng	# 80
88) Benzo(k)fluoranthene	15.02	252	96892	8.694	ng	# 83
89) Benzo(a)pyrene	15.39	252	51845	4.909	ng	# 83
91) Benzo(g,h,i)perylene	17.36	276	26839	3.193	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF042518\
Data File : BF104792.D
Acq On : 25 Apr 2018 16:46
Operator : JU/SJ
Sample : J2505-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 26 08:13:13 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 25 14:01:50 2018
Response via : Initial Calibration






#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.80 min Scan# 801
 Delta R.T. -0.00 min
 Lab File: BF104792.D
 Acq: 25 Apr 2018 16:46

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 122693
 Ion Ratio Lower Upper
 152 100
 150 152.7 124.6 186.8
 115 61.9 50.1 75.1




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

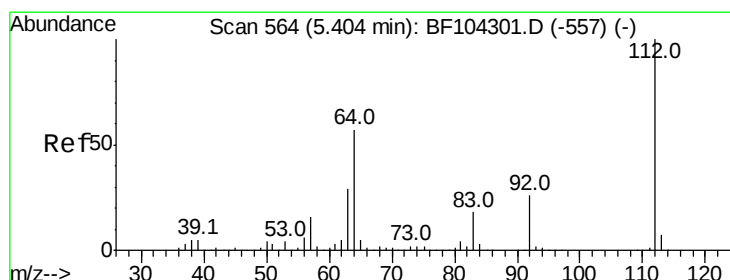



#5

2-Fluorophenol
 Concen: 105.132 ng
 RT: 5.42 min Scan# 567
 Delta R.T. 0.01 min
 Lab File: BF104792.D
 Acq: 25 Apr 2018 16:46

Tgt Ion:112 Resp: 843592
 Ion Ratio Lower Upper
 112 100
 64 55.4 47.9 71.9
 63 28.9 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1





#7

Phenol-d6

Concen: 104.753 ng

RT: 6.45 min Scan# 741

Delta R.T. -0.00 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 1032763

Ion Ratio Lower Upper

99 100

42 16.4 14.5 21.7

71 34.8 25.4 38.0



#18

Hexachloroethane

Concen: 4.722 ng

RT: 7.33 min Scan# 891

Delta R.T. 0.02 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46




Tgt Ion: 117 Resp: 16101

Ion Ratio Lower Upper

117 100

119 557.9 75.8 113.8#

201 0.0 75.7 113.5#









#19
n-Nitroso-di-n-propylamine
Concen: 13.903 ng
RT: 7.37 min Scan# 898
Delta R.T. 0.15 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46

Instrument :
BNA_F
ClientSampleId :

Tot Ion: 70 Resp: 89571
Ion Ratio Lower Upper
70 100
42 44.2 47.5 71.3#
101 0.0 7.4 11.2#
130 2.1 16.6 25.0#




Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): BF1
Ion 130.00 (129.70 to 130.70): BF1






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.08 min Scan# 1019
Delta R.T. -0.01 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46

Tgt Ion:136 Resp: 495739
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 6.8 6.6 9.8
68 6.0 5.0 7.4



Abundance Ion 136.00 (135.70 to 136.70): BF1
Ion 137.00 (136.70 to 137.70): BF1
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1









#22
Acetophenone
Concen: 2.886 ng
RT: 7.19 min Scan# 867
Delta R.T. -0.03 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46




Instrument :
BNA_F
ClientSampleId :


Tot Ion:105 Resp: 35219
Ion Ratio Lower Upper
105 100
71 3.5 4.4 6.6#
51 4.2 22.3 33.5#
120 0.0 16.9 25.3#



#23
Nitrobenzene-d5
Concen: 85.388 ng
RT: 7.37 min Scan# 898
Delta R.T. -0.01 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46

Tgt Ion: 82 Resp: 648257
Ion Ratio Lower Upper
82 100
128 45.4 36.1 54.1
54 44.4 41.4 62.2





#25

Isophorone

Concen: 40.291 ng

RT: 7.37 min Scan# 898

Delta R.T. -0.26 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 646833

Ion Ratio Lower Upper




82 100

95 0.1 5.2 7.8#

138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1



#37

2-Methylnaphthalene

Concen: 3.381 ng

RT: 8.80 min Scan# 1141

Delta R.T. -0.00 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion: 142 Resp: 53989

Ion Ratio Lower Upper



142 100


141 92.4 70.8 106.2

115 32.7 26.1 39.1



Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E
Ion 115.00 (114.70 to 115.70): E





#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.84 min Scan# 1318

Delta R.T. -0.01 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 217002

Ion Ratio Lower Upper

164 100

162 104.6 86.1 129.1




160 45.7 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



#41

2,4,6-Tribromophenol

Concen: 102.239 ng

RT: 10.64 min Scan# 1454

Delta R.T. -0.00 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion:330 Resp: 230142

Ion Ratio Lower Upper

330 100

332 96.1 77.0 115.6



141 33.8 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E









#44
 2-Fluorobiphenyl
 Concen: 71.491 ng
 RT: 9.16 min Scan# 1203
 Delta R.T. -0.00 min
 Lab File: BF104792.D
 Acq: 25 Apr 2018 16:46

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:172 Resp: 982033
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.7 44.5
 170 23.9 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E






#49
 Dimethylphthalate
 Concen: 9.951 ng
 RT: 9.55 min Scan# 1269
 Delta R.T. -0.02 min
 Lab File: BF104792.D
 Acq: 25 Apr 2018 16:46

Tgt Ion:163 Resp: 170283
 Ion Ratio Lower Upper
 163 100
 194 3.3 2.7 4.1
 164 9.8 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E









#57
Fluorene
 Concen: 2.082 ng
 RT: 10.39 min Scan# 1411
 Delta R.T. -0.01 min
 Lab File: BF104792.D
 Acq: 25 Apr 2018 16:46




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:166 Resp: 29114
 Ion Ratio Lower Upper
 166 100
 165 93.3 79.8 119.8
 167 14.1 10.6 16.0



#63
Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.33 min Scan# 1572
 Delta R.T. -0.00 min
 Lab File: BF104792.D
 Acq: 25 Apr 2018 16:46

Tgt Ion:188 Resp: 341766
 Ion Ratio Lower Upper
 188 100
 94 9.1 8.5 12.7
 80 9.6 9.2 13.8





#64

4,6-Dinitro-2-methylphenol

Concen: 7.609 ng

RT: 10.63 min Scan# 1453

Delta R.T. 0.18 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion:198 Resp: 514

Ion Ratio Lower Upper

198 100

51 175.4 37.7 77.7#




105 215.6 36.3 76.3#



Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E



#66

4-Bromophenyl-phenylether

Concen: 3.886 ng

RT: 10.63 min Scan# 1453

Delta R.T. -0.24 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion:248 Resp: 14128

Ion Ratio Lower Upper

248 100

250 193.0 76.9 115.3#



141 568.0 74.4 111.6#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E





#70

Phenanthrene

Concen: 9.266 ng

RT: 11.36 min Scan# 1576

Delta R.T. -0.01 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampled :


Tot Ion:178 Resp: 176366

Ion Ratio Lower Upper

178 100

176 17.6 15.8 23.8




179 14.8 13.0 19.6



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E



#71

Anthracene

Concen: 2.473 ng

RT: 11.40 min Scan# 1584

Delta R.T. -0.01 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion:178 Resp: 47853

Ion Ratio Lower Upper

178 100

176 17.9 15.4 23.2



179 16.7 12.6 19.0




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E





#74

Fluoranthene

Concen: 9.150 ng

RT: 12.55 min Scan# 1778

Delta R.T. -0.01 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 181962

Ion Ratio Lower Upper

202 100

101 12.6 0.0 34.1




203 18.1 0.0 38.1



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.98 min Scan# 2022

Delta R.T. -0.01 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion:240 Resp: 215335

Ion Ratio Lower Upper

240 100

120 12.3 9.5 14.3



236 26.4 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E





#77

Pvrene

Concen: 10.156 ng

RT: 12.78 min Scan# 1818

Delta R.T. -0.00 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 162100

Ion Ratio Lower Upper

202 100

200 20.9 17.4 26.2




203 17.7 14.3 21.5



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



#78

Terphenyl-d14

Concen: 77.352 ng

RT: 12.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion:244 Resp: 730608

Ion Ratio Lower Upper

244 100

212 6.8 5.4 8.0



122 11.8 11.0 16.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E









#80
Benzo(a)anthracene
Concen: 6.077 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.01 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 78183
Ion Ratio Lower Upper
228 100
226 29.2 22.6 33.8
229 21.8 15.8 23.6



#82
Chrysene
Concen: 5.917 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.05 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46

Tgt Ion:228 Resp: 78183
Ion Ratio Lower Upper
228 100
226 29.2 25.0 37.6
229 21.8 16.2 24.4





#85

Indeno(1,2,3-cd)pyrene

Concen: 2.224 ng

RT: 16.91 min Scan# 2520

Delta R.T. -0.02 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion:276 Resp: 24962

Ion Ratio Lower Upper

276 100

138 27.8 25.0 37.6




277 28.5 20.1 30.1



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



#86

Perylene-d12

Concen: 20.000 ng

RT: 15.45 min Scan# 2272

Delta R.T. -0.01 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion:264 Resp: 186907

Ion Ratio Lower Upper

264 100

260 22.9 19.2 28.8



265 21.3 17.5 26.3




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E





#87

Benzo(b)fluoranthene

Concen: 8.208 ng

RT: 15.02 min Scan# 2199

Delta R.T. -0.02 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46

Instrument :

BNA_F

ClientSampleId :


Tot Ion:252 Resp: 96892

Ion Ratio Lower Upper

252 100

253 27.9 17.0 25.6#




125 23.6 9.0 13.6#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



#88

Benzo(k)fluoranthene

Concen: 8.694 ng

RT: 15.02 min Scan# 2199

Delta R.T. -0.05 min

Lab File: BF104792.D

Acq: 25 Apr 2018 16:46


Tgt Ion:252 Resp: 96892

Ion Ratio Lower Upper

252 100

253 27.9 17.9 26.9#



125 23.6 10.2 15.2#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E









#89
Benzo(a)pyrene
Concen: 4.909 ng
RT: 15.39 min Scan# 2261
Delta R.T. -0.02 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46

Instrument :
BNA_F
ClientSampleId :

Tot Ion:252 Resp: 51845
Ion Ratio Lower Upper
252 100
253 24.3 17.1 25.7
125 26.0 9.8 14.6#



#91
Benzo(g,h,i)perylene
Concen: 3.193 ng
RT: 17.36 min Scan# 2596
Delta R.T. -0.02 min
Lab File: BF104792.D
Acq: 25 Apr 2018 16:46

Tgt Ion:276 Resp: 26839
Ion Ratio Lower Upper
276 100
277 27.8 17.9 26.9#
138 29.6 21.8 32.8

