


Data Path : Z:\HPCHEM1\BNA F\Data\BF042518\
 Data File : BF104807.D
 Acq On : 26 Apr 2018 00:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 25 14:01:50 2018

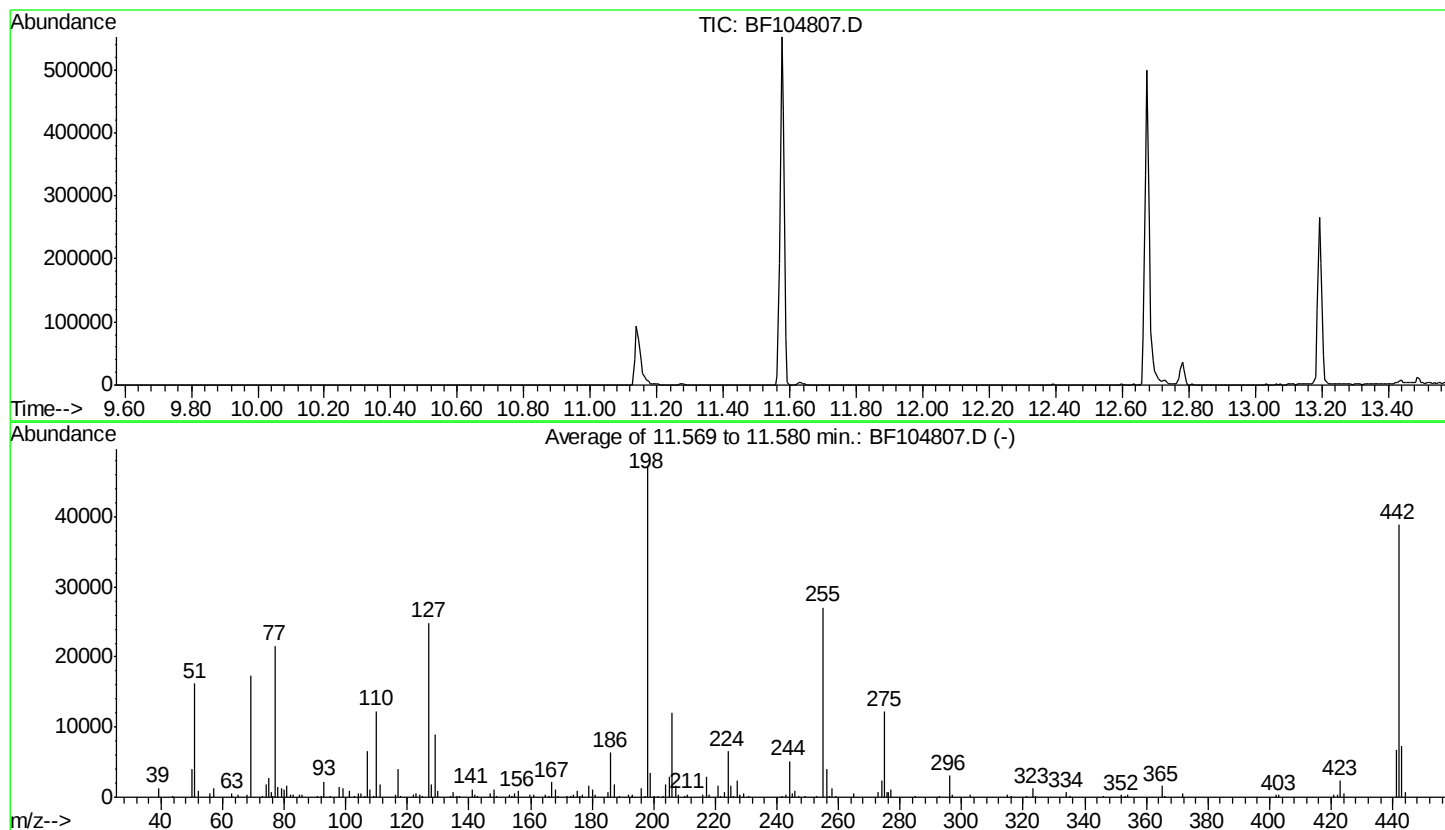

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	16201	PASS
68	69	0.00	2	1.9	325	PASS
69	198	0.00	100	36.6	17292	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	24903	PASS
197	198	0.00	2	0.5	244	PASS
198	198	100	100	100.0	47293	PASS
199	198	5	9	7.2	3422	PASS
275	198	10	60	25.7	12153	PASS
365	198	1	100	3.3	1558	PASS
441	443	0.01	100	91.6	6717	PASS
442	198	50	100	82.2	38859	PASS
443	442	15	24	18.9	7336	PASS