
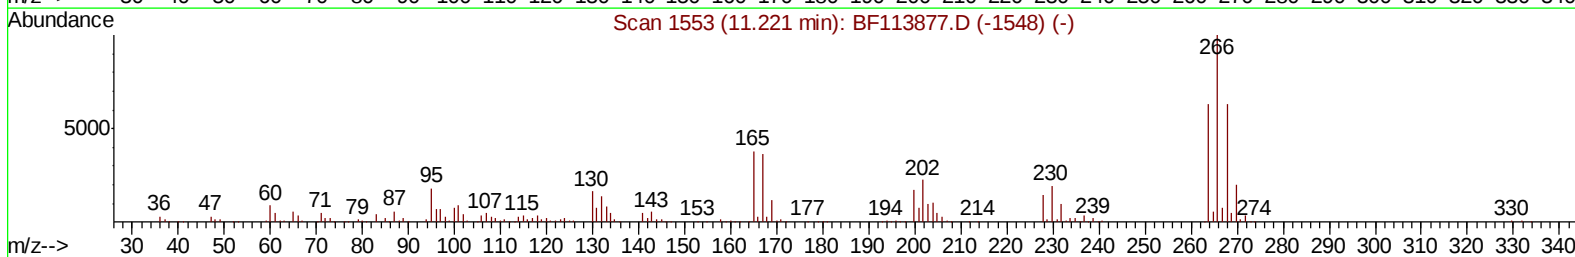
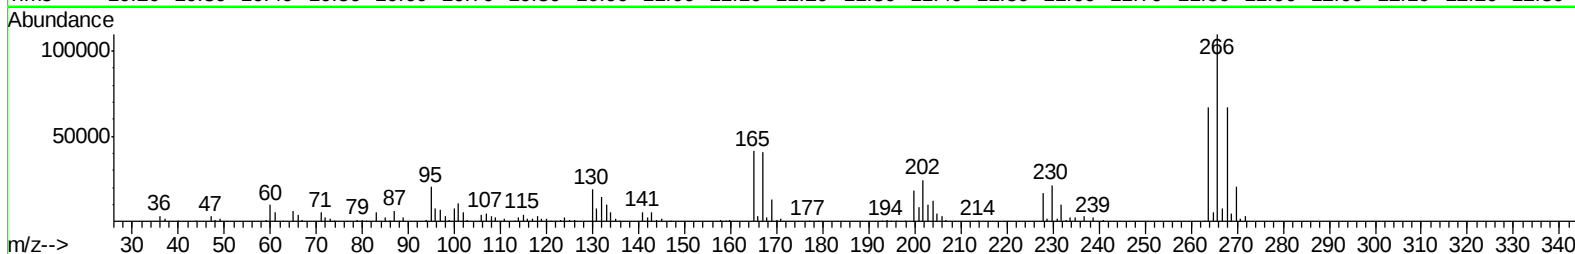


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042519\
Data File : BF113974.D
Acq On : 25 Apr 2019 13:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:24:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 03:32:35 2019
Response via : Initial Calibration

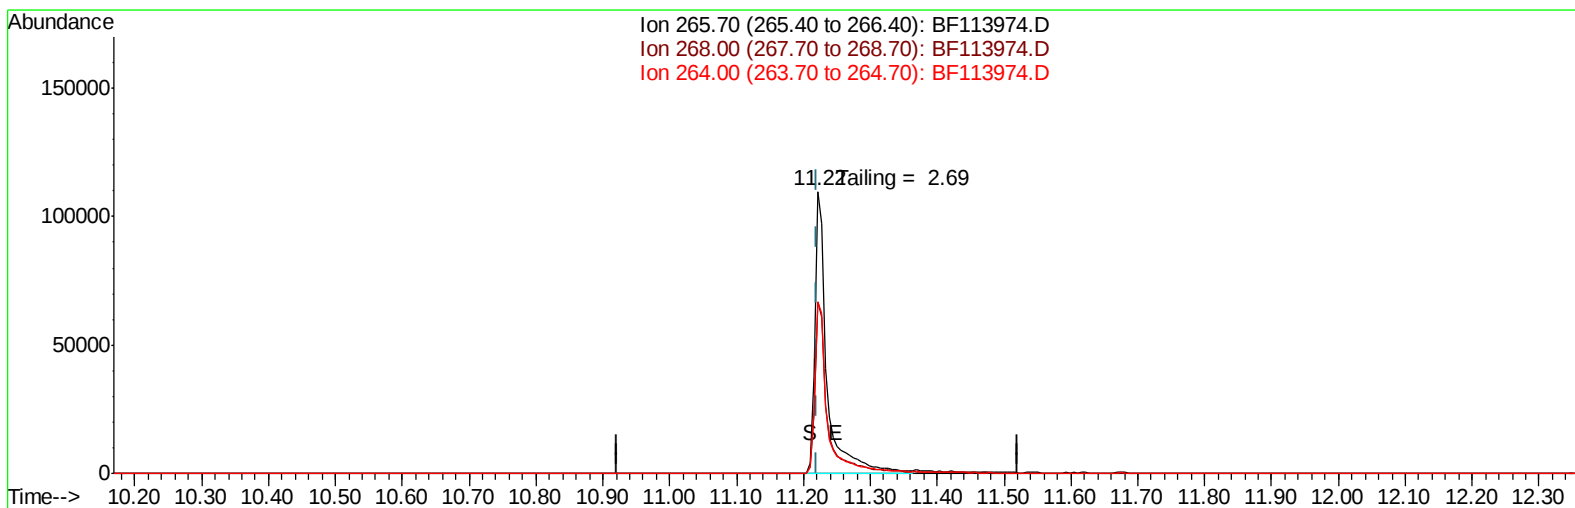

TIC: BF113974.D

(70) Pentachlorophenol (C)




11.221min (0.000) 33547.94ng

response 141206

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	60.86
264.00	63.80	60.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042519\
 Data File : BF113974.D
 Acq On : 25 Apr 2019 13:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:24:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 03:32:35 2019
 Response via : Initial Calibration

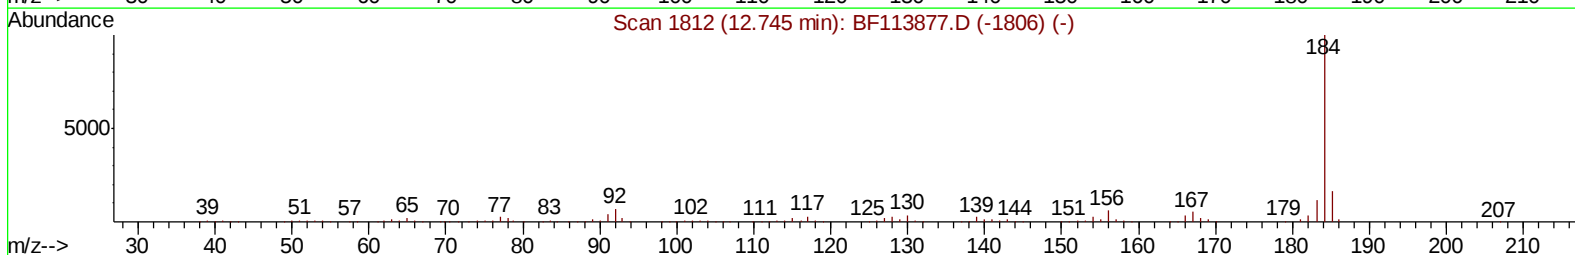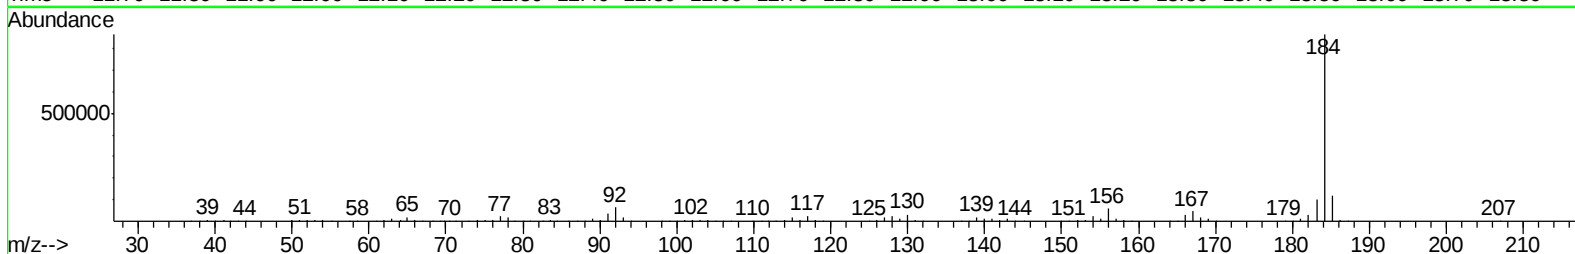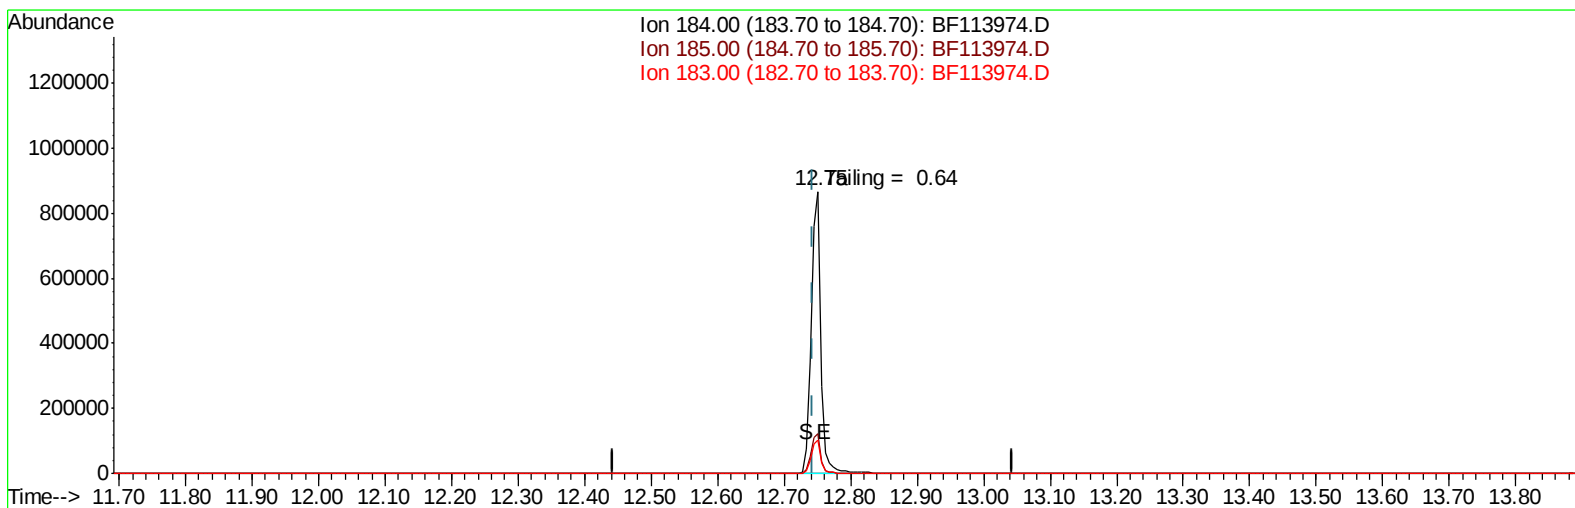

TIC: BF113974.D

(77) Benzidine

12.751min (+0.007) 0.00ng

response 879747

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.96
183.00	11.70	11.89
0.00	0.00	0.00