

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042519\
 Data File : BF113989.D
 Acq On : 25 Apr 2019 20:28
 Operator : JU/SJ
 Sample : K2555-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BLIND-DUPLICATE

Quant Time: Apr 26 05:47:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 23 03:32:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.89	152	101577	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	387472	20.00	ng	0.00
39) Acenaphthene-d10	9.93	164	207472	20.00	ng	0.00
64) Phenanthrene-d10	11.42	188	446577	20.00	ng	0.00
76) Chrysene-d12	14.05	240	427416	20.00	ng	-0.02
87) Perylene-d12	15.54	264	442106	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	365498	61.54	ng	0.00
7) Phenol-d6	6.52	99	343044	46.04	ng	0.00
23) Nitrobenzene-d5	7.45	82	624283	99.48	ng	0.00
42) 2,4,6-Tribromophenol	10.72	330	372568	147.41	ng	0.00
45) 2-Fluorobiphenyl	9.25	172	1264053	95.29	ng	0.00
79) Terphenyl-d14	13.00	244	1780527	85.40	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042519\
Data File : BF113989.D
Acq On : 25 Apr 2019 20:28
Operator : JU/SJ
Sample : K2555-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE

Quant Time: Apr 26 05:47:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 23 03:32:35 2019
Response via : Initial Calibration

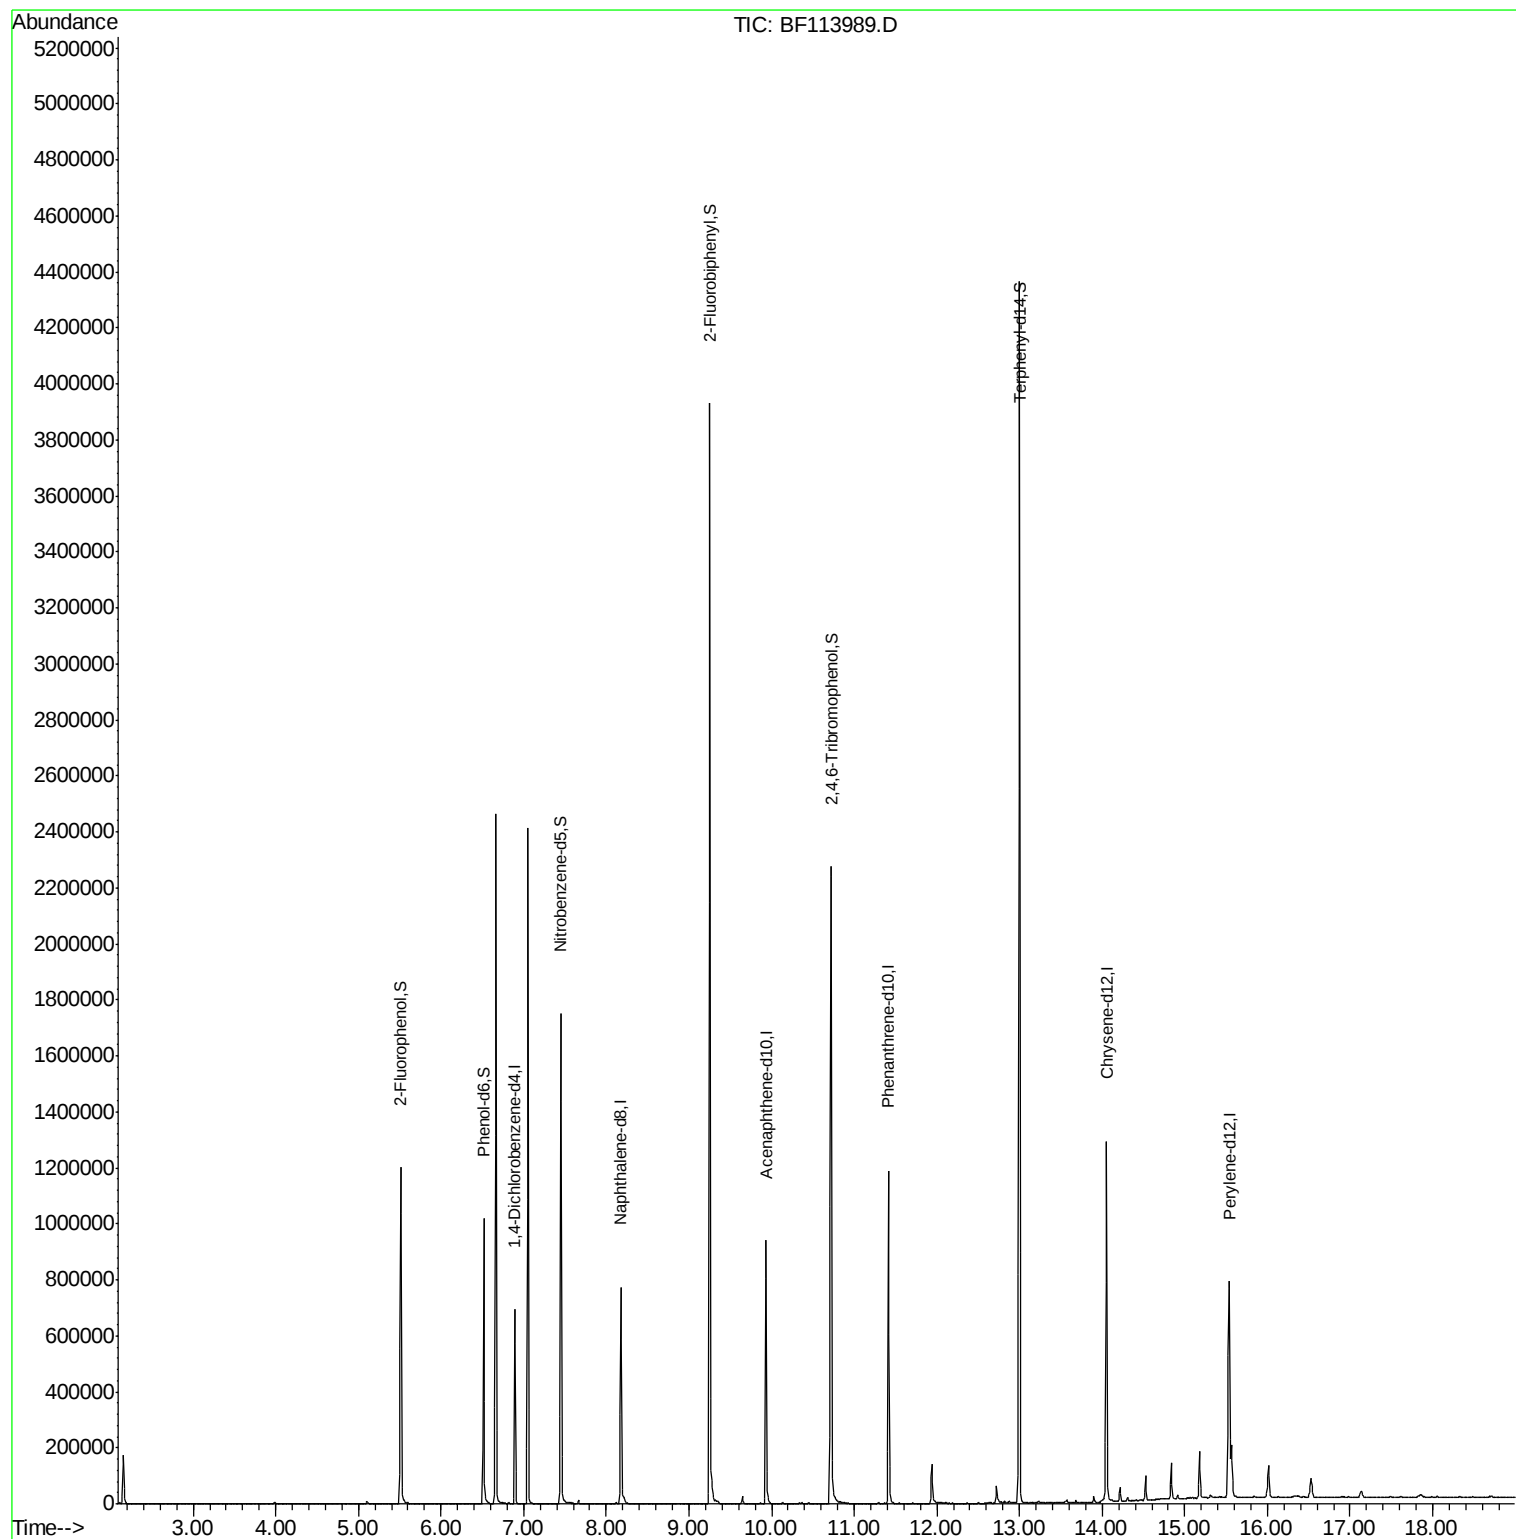

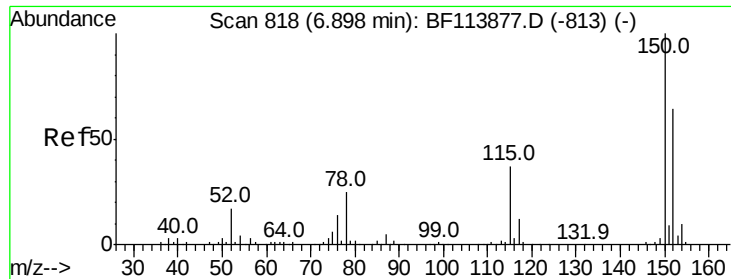


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.89 min Scan# 817
Delta R.T. -0.01 min
Lab File: BF113989.D
Acq: 25 Apr 2019 20:28

Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE

Tot Ion:152 Resp: 101577
Ion Ratio Lower Upper
152 100
150 157.7 125.9 188.9
115 62.2 45.9 68.9

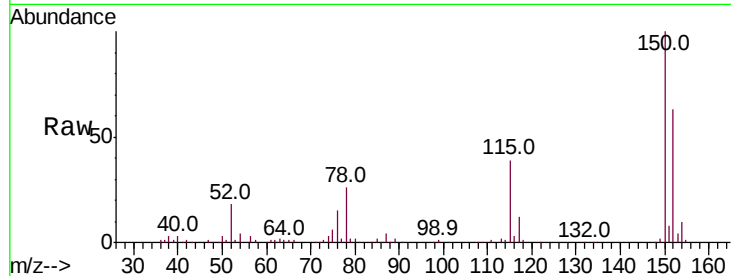


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

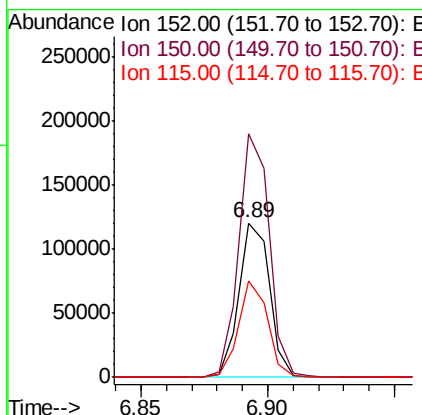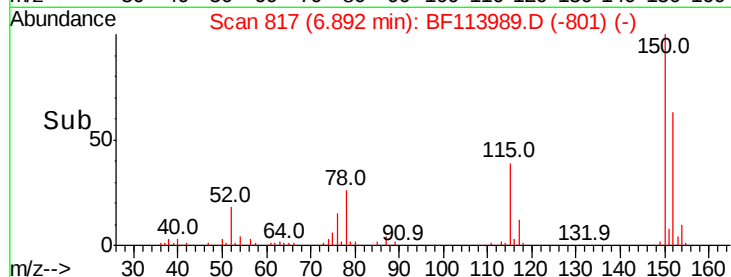



#5


2-Fluorophenol
Concen: 61.543 ng
RT: 5.51 min Scan# 582
Delta R.T. -0.01 min
Lab File: BF113989.D
Acq: 25 Apr 2019 20:28

Tgt Ion:112 Resp: 365498
Ion Ratio Lower Upper
112 100
64 57.4 46.6 69.8
63 28.6 23.1 34.7



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

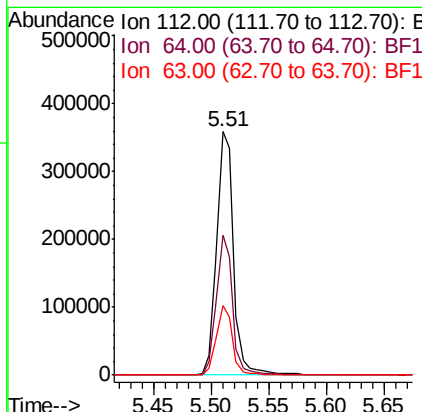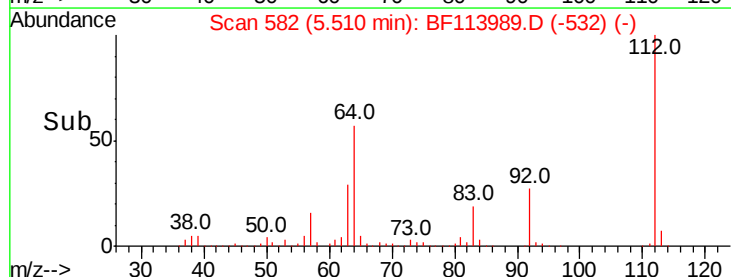

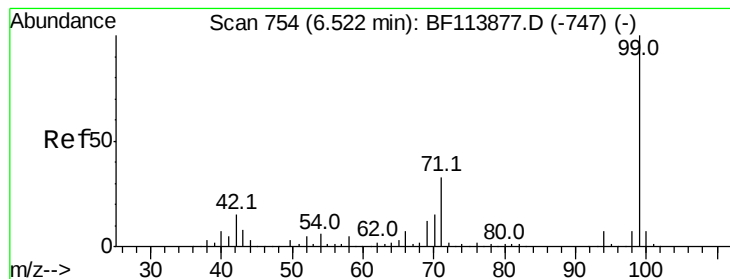

#7

Phenol-d6

Concen: 46.039 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.01 min

Lab File: BF113989.D

Acq: 25 Apr 2019 20:28

Instrument :

BNA_F

ClientSampleId :

BLIND-DUPLICATE


Tot Ion: 99 Resp: 343044

Ion Ratio Lower Upper

99 100

42 14.3 12.5 18.7




71 32.8 26.9 40.3

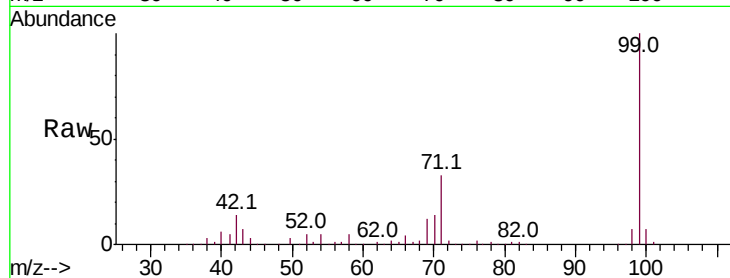

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

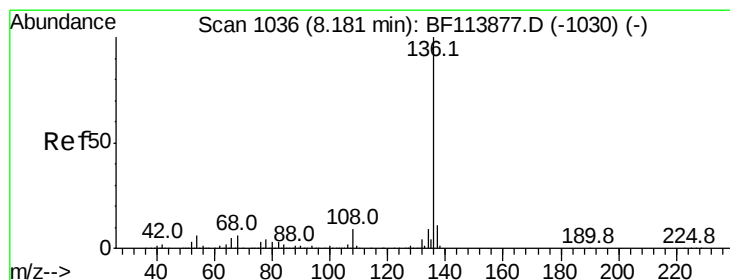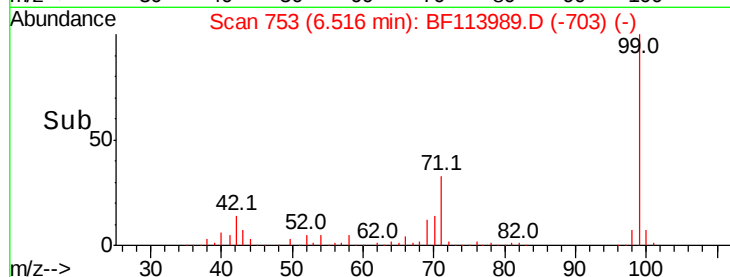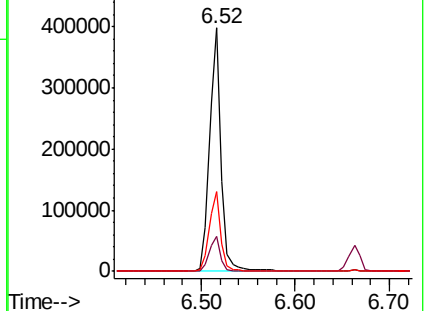

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.17 min Scan# 1035

Delta R.T. -0.01 min

Lab File: BF113989.D

Acq: 25 Apr 2019 20:28

Tgt Ion: 136 Resp: 387472


Ion Ratio Lower Upper

136 100

137 11.2 8.6 12.8

54 6.4 5.0 7.6

68 6.0 4.9 7.3


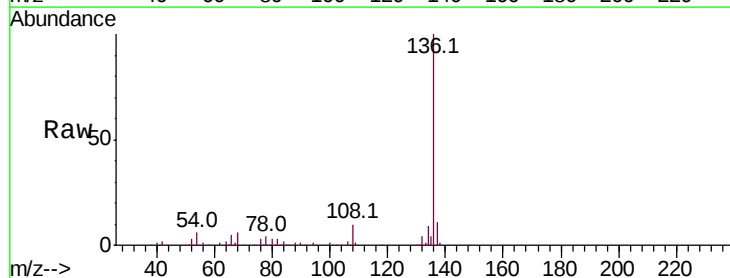



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

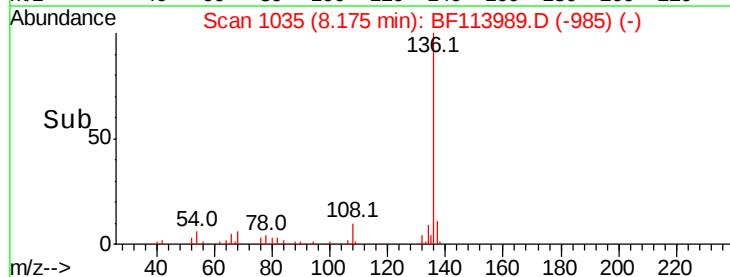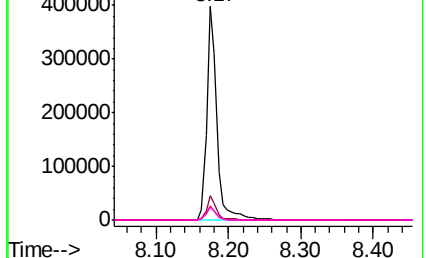


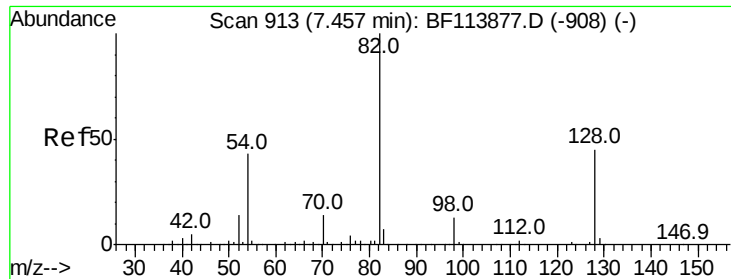




#23
 Nitrobenzene-d5
 Concen: 99.480 ng
 RT: 7.45 min Scan# 912
 Delta R.T. -0.01 min
 Lab File: BF113989.D
 Acq: 25 Apr 2019 20:28

Instrument :
 BNA_F
 ClientSampleId :
 BLIND-DUPLICATE

Tot Ion	82	Resp	624283
Ion Ratio	Lower	Upper	
82	100		
128	45.3	36.8	55.2
54	43.3	33.8	50.6

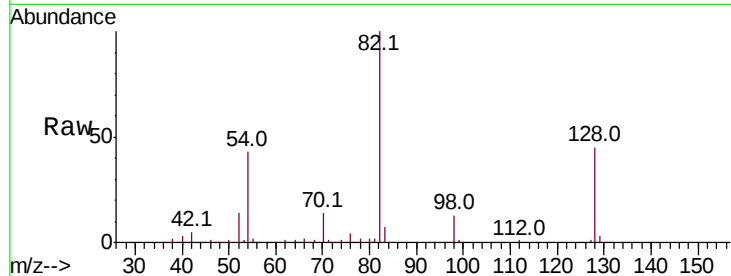


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

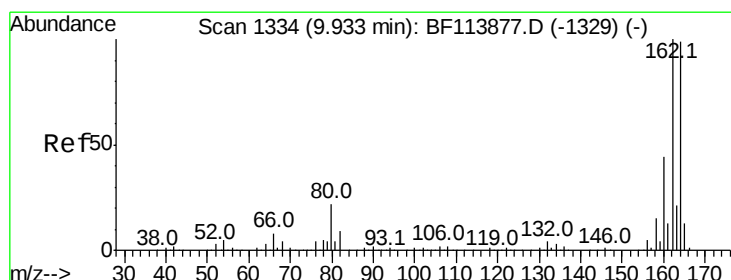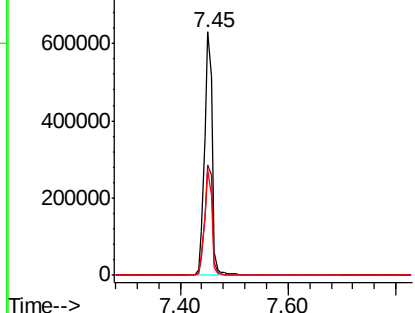
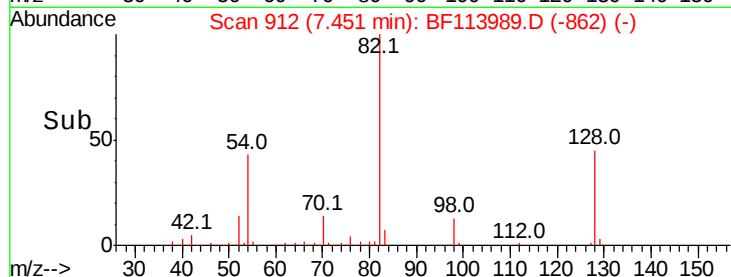



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. 0.00 min
 Lab File: BF113989.D
 Acq: 25 Apr 2019 20:28

Tgt Ion	164	Resp	207472
Ion Ratio	Lower	Upper	
164	100		
162	103.6	81.1	121.7
160	44.9	35.8	53.6



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

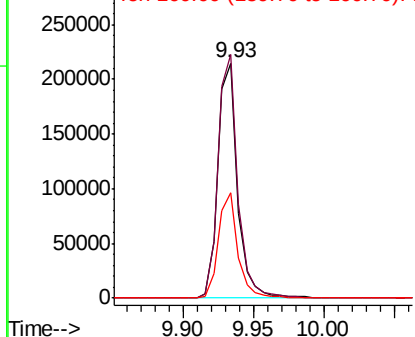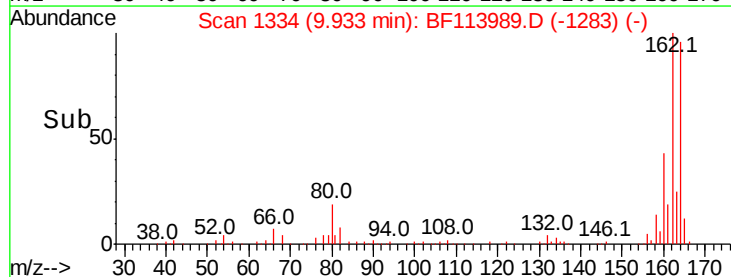


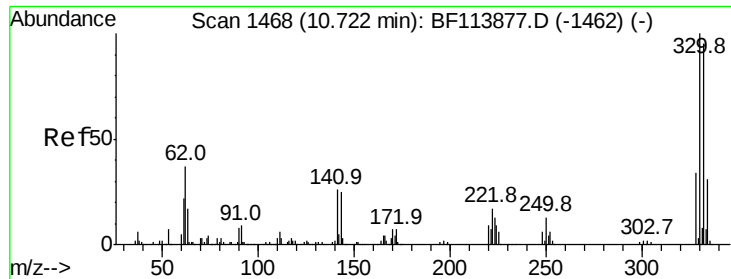




#42
 2,4,6-Tribromophenol
 Concen: 147.410 ng
 RT: 10.72 min Scan# 1468
 Delta R.T. 0.00 min
 Lab File: BF113989.D
 Acq: 25 Apr 2019 20:28

Instrument :
 BNA_F
 ClientSampleId :
 BLIND-DUPLICATE

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.7	77.5	116.3
141	26.5	22.2	33.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

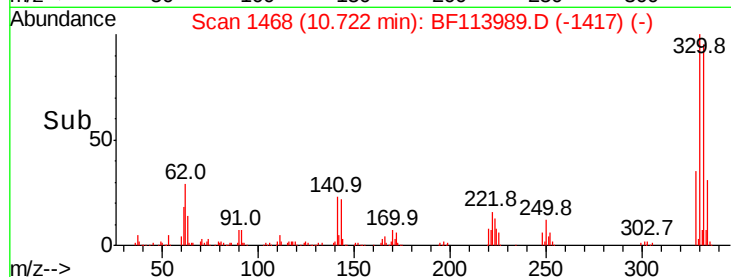
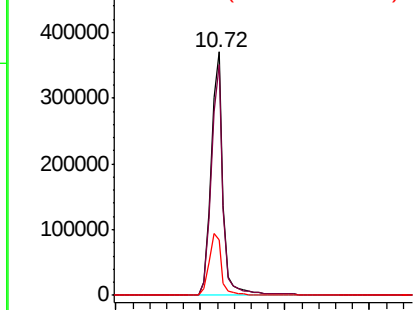



#45
 2-Fluorobiphenyl
 Concen: 95.290 ng
 RT: 9.25 min Scan# 1218
 Delta R.T. -0.00 min
 Lab File: BF113989.D
 Acq: 25 Apr 2019 20:28

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.4	44.0
170	24.8	19.9	29.9



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



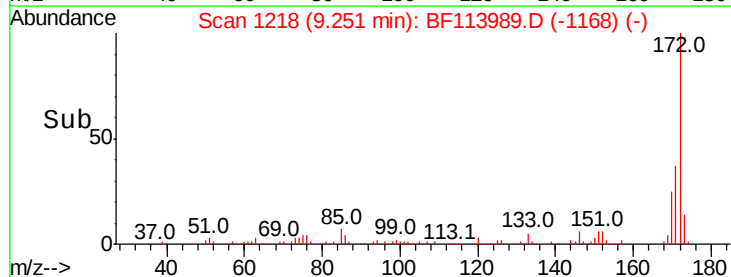
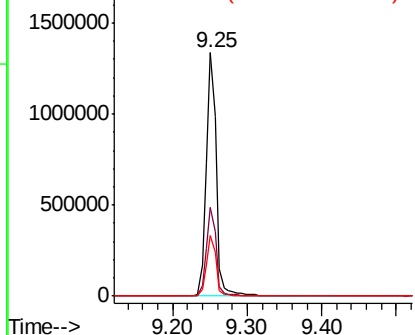


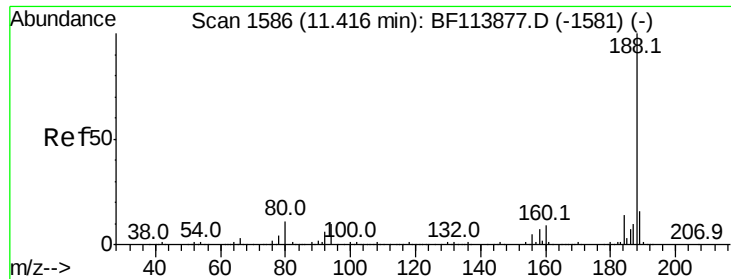

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.42 min Scan# 1586
Delta R.T. 0.00 min
Lab File: BF113989.D
Acq: 25 Apr 2019 20:28




Instrument :
BNA_F
ClientSampleId :
BLIND-DUPLICATE


Tot Ion:188 Resp: 446577
Ion Ratio Lower Upper
188 100
94 8.8 8.2 12.4
80 9.8 9.0 13.6

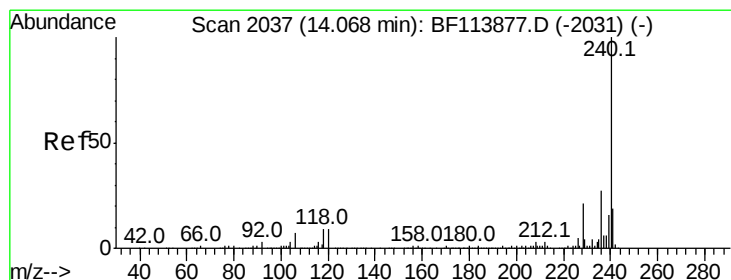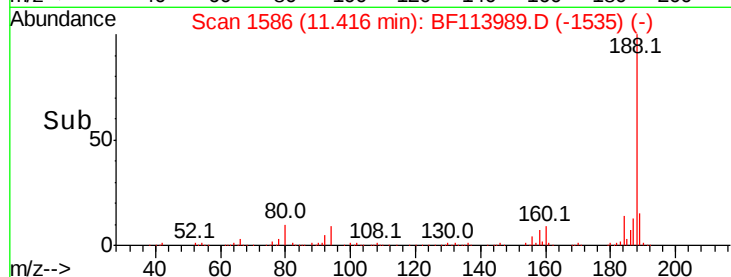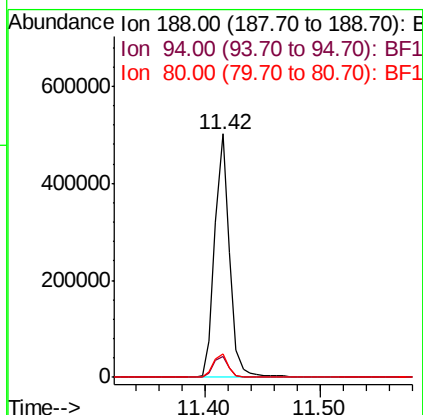

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.05 min Scan# 2034
Delta R.T. -0.02 min
Lab File: BF113989.D
Acq: 25 Apr 2019 20:28

Tgt Ion:240 Resp: 427416
Ion Ratio Lower Upper
240 100
120 10.1 9.3 13.9
236 26.5 21.2 31.8

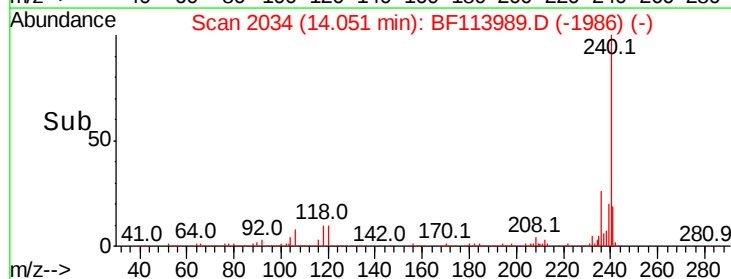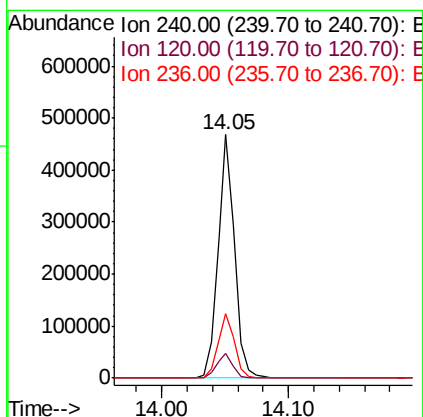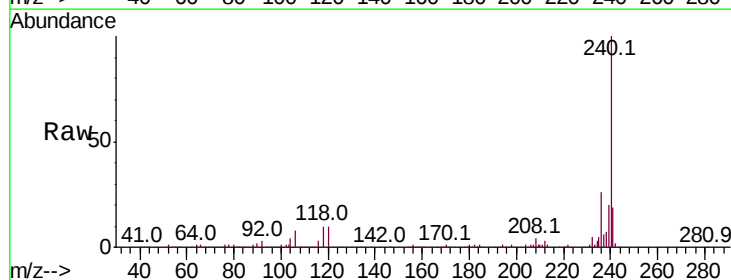

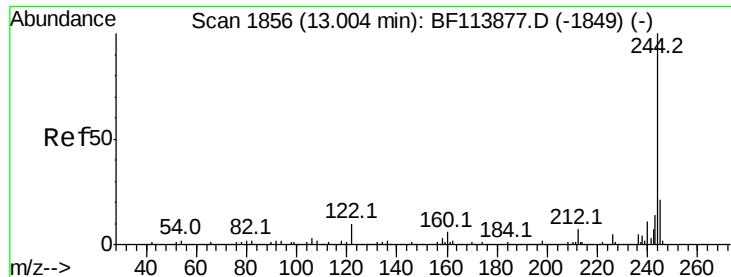

#79

Terphenyl-d14

Concen: 85.404 ng

RT: 13.00 min Scan# 1856

Delta R.T. 0.00 min

Lab File: BF113989.D

Acq: 25 Apr 2019 20:28

Instrument :

BNA_F

ClientSampleId :

BLIND-DUPLICATE


Tot Ion:244 Resp: 1780527

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.2




122 9.2 7.6 11.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

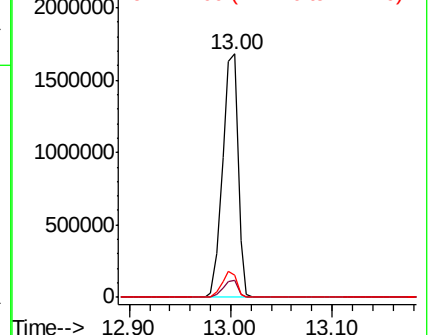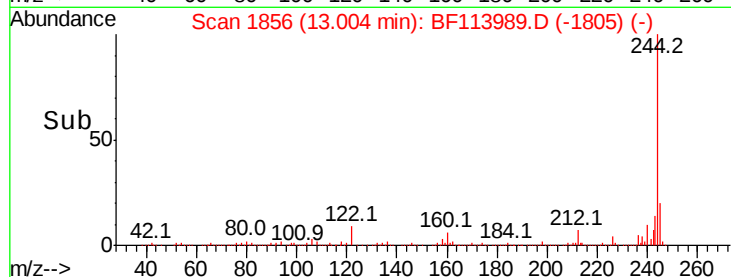

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.54 min Scan# 2287

Delta R.T. -0.03 min

Lab File: BF113989.D

Acq: 25 Apr 2019 20:28


Tgt Ion:264 Resp: 442106

Ion Ratio Lower Upper

264 100

260 23.3 18.9 28.3

265 21.3 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

