

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042519\
 Data File : BF113993.D
 Acq On : 25 Apr 2019 22:13
 Operator : JU/SJ
 Sample : K2566-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S37-0019

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.152	5	11	19	rVB	155694	203141	4.80%	0.910%
2	5.510	578	582	601	rBV	948928	901309	21.31%	4.040%
3	6.516	749	753	766	rBV	585949	550184	13.01%	2.466%
4	6.663	774	778	781	rBV	2271273	1947683	46.05%	8.729%
5	6.892	814	817	821	rBV	682176	571184	13.50%	2.560%
6	7.051	840	844	848	rBV	2244799	1986674	46.97%	8.904%
7	7.451	907	912	915	rBV	1639103	1524216	36.04%	6.831%
8	8.175	1032	1035	1053	rBV	762670	728384	17.22%	3.265%
9	9.251	1214	1218	1221	rBV	3710401	3181786	75.23%	14.261%
10	9.933	1330	1334	1347	rBV	906514	904330	21.38%	4.053%
11	10.716	1463	1467	1488	rBV	2130102	2242477	53.02%	10.051%
12	11.416	1582	1586	1600	rBV	1114460	1031703	24.39%	4.624%
13	12.998	1851	1855	1859	rBV	4119951	4229487	100.00%	18.956%
14	14.051	2030	2034	2045	rVB	1187328	1144110	27.05%	5.128%
15	15.174	2221	2225	2231	rBV	39274	43384	1.03%	0.194%
16	15.533	2280	2286	2299	rBV	743246	1121782	26.52%	5.028%


Sum of corrected areas: 22311834

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042519\
Data File : BF113993.D
Acq On : 25 Apr 2019 22:13
Operator : JU/SJ
Sample : K2566-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S37-0019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

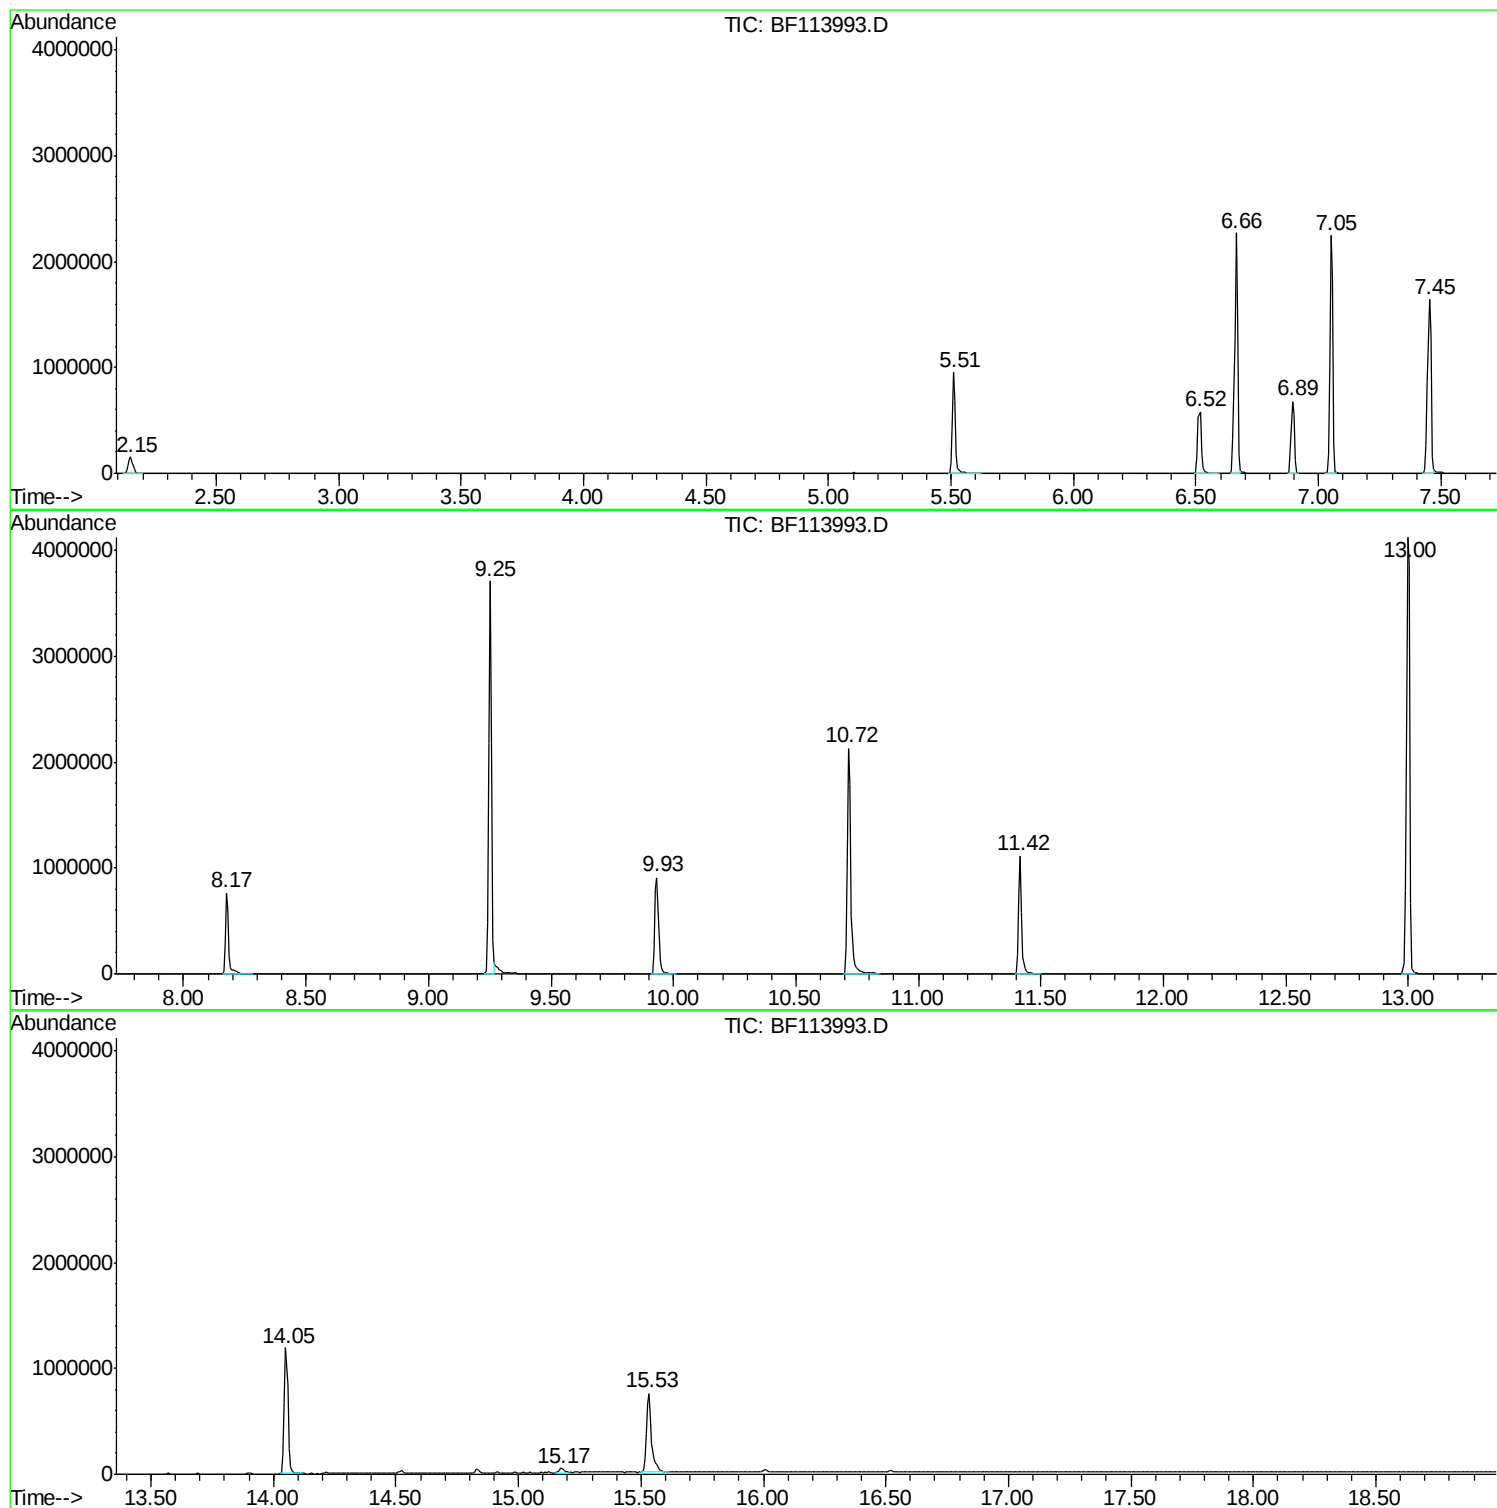

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042519\
Data File : BF113993.D
Acq On : 25 Apr 2019 22:13
Operator : JU/SJ
Sample : K2566-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S37-0019










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.15	7.11 ng	203141	1,4-Dichlorobenzene-d4	6.89

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			N-Ethylformamide	73	C3H7NO	000627-45-2	9
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

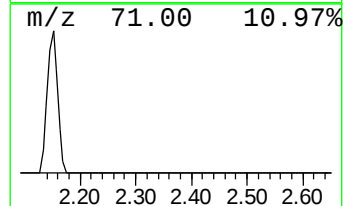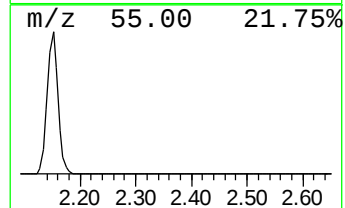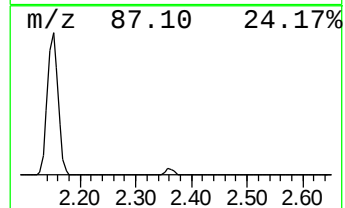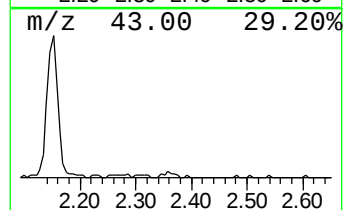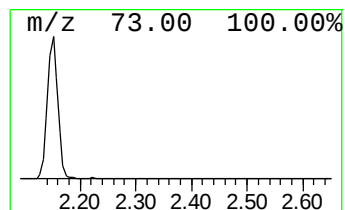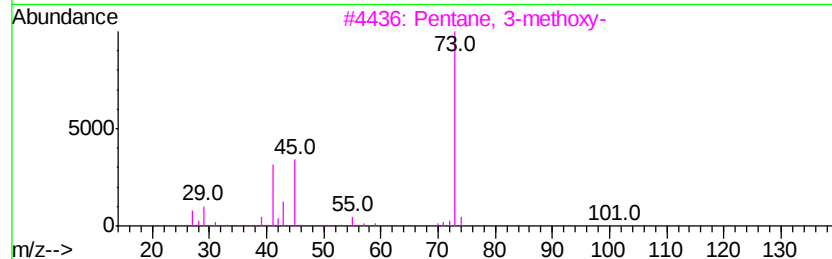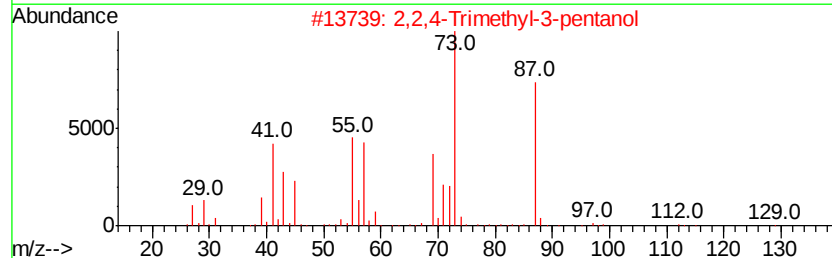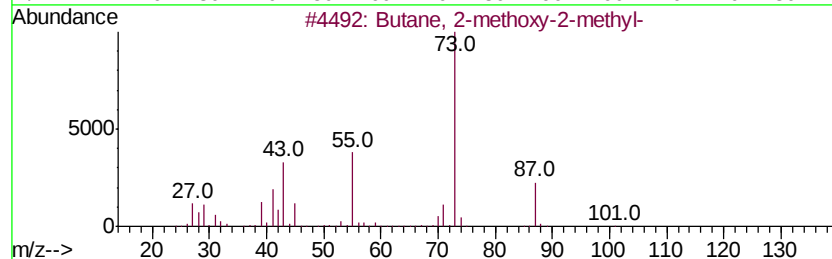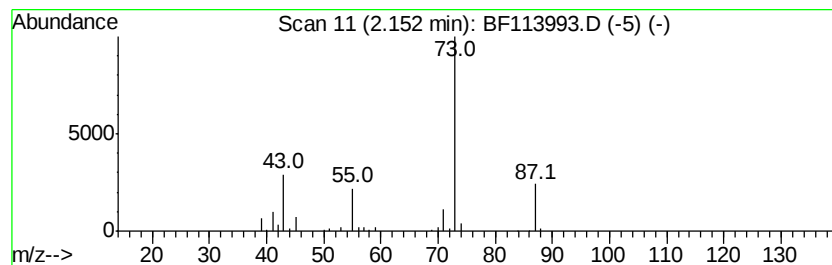

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF042519\
Data File : BF113993.D
Acq On : 25 Apr 2019 22:13
Operator : JU/SJ
Sample : K2566-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S37-0019










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.66 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	68.20 ng	1947680	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	9
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

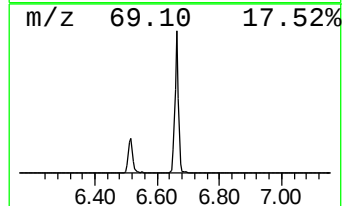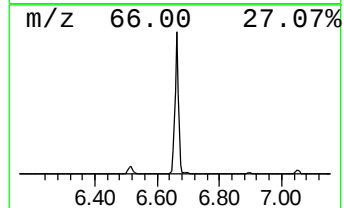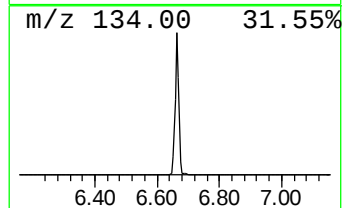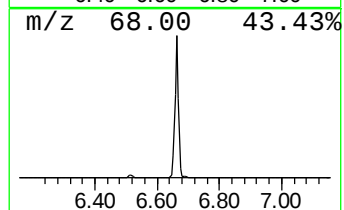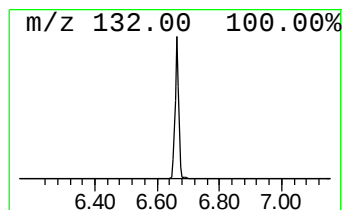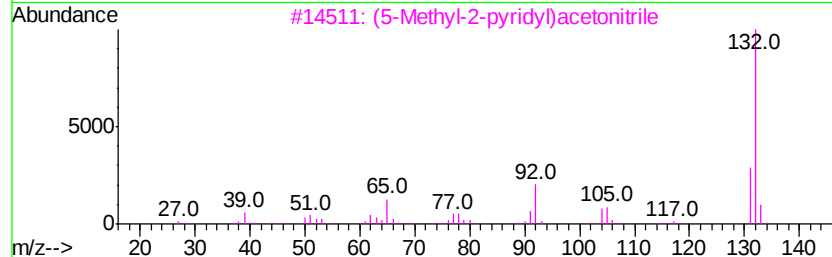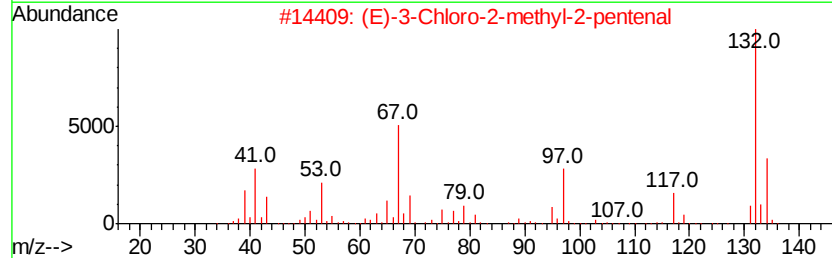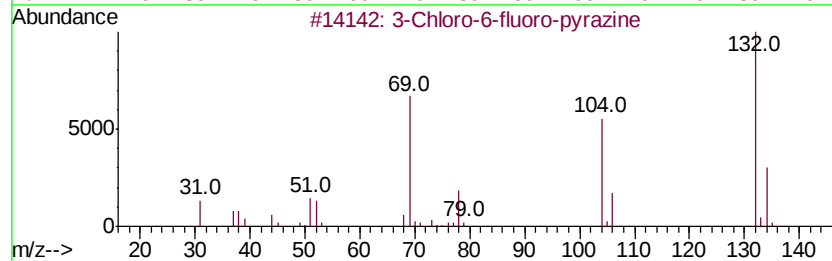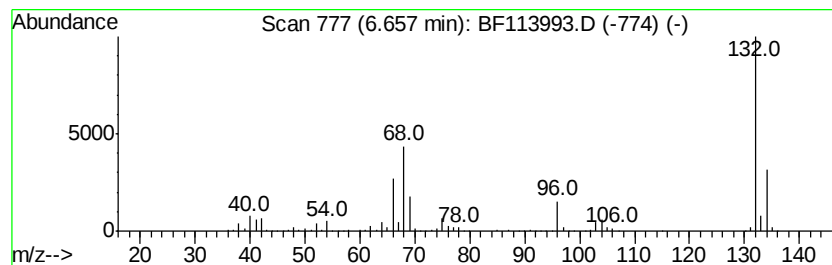

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF042519\
Data File : BF113993.D
Acq On : 25 Apr 2019 22:13
Operator : JU/SJ
Sample : K2566-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S37-0019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown	2.15	7.1	ng	203141	1	6.89	571184	20.0
unknown6.66	6.66	68.2	ng	1947680	1	6.89	571184	20.0