
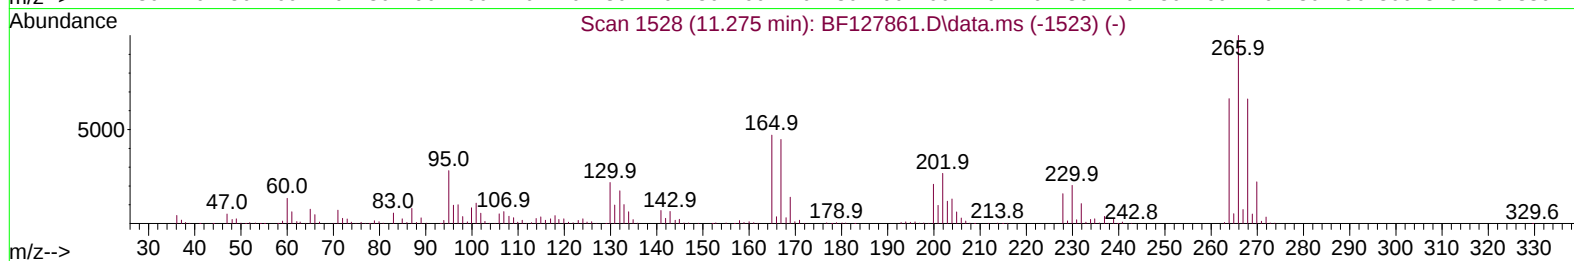
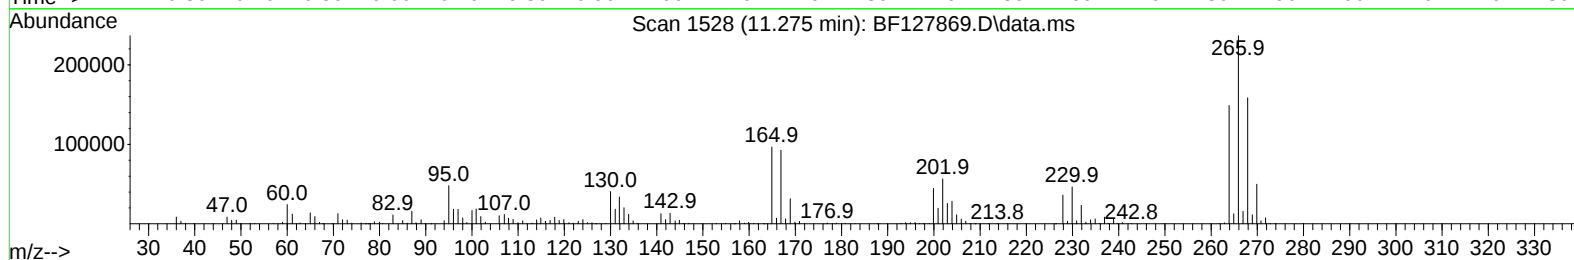


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127869.D
Acq On : 25 Apr 2022 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 17:09:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

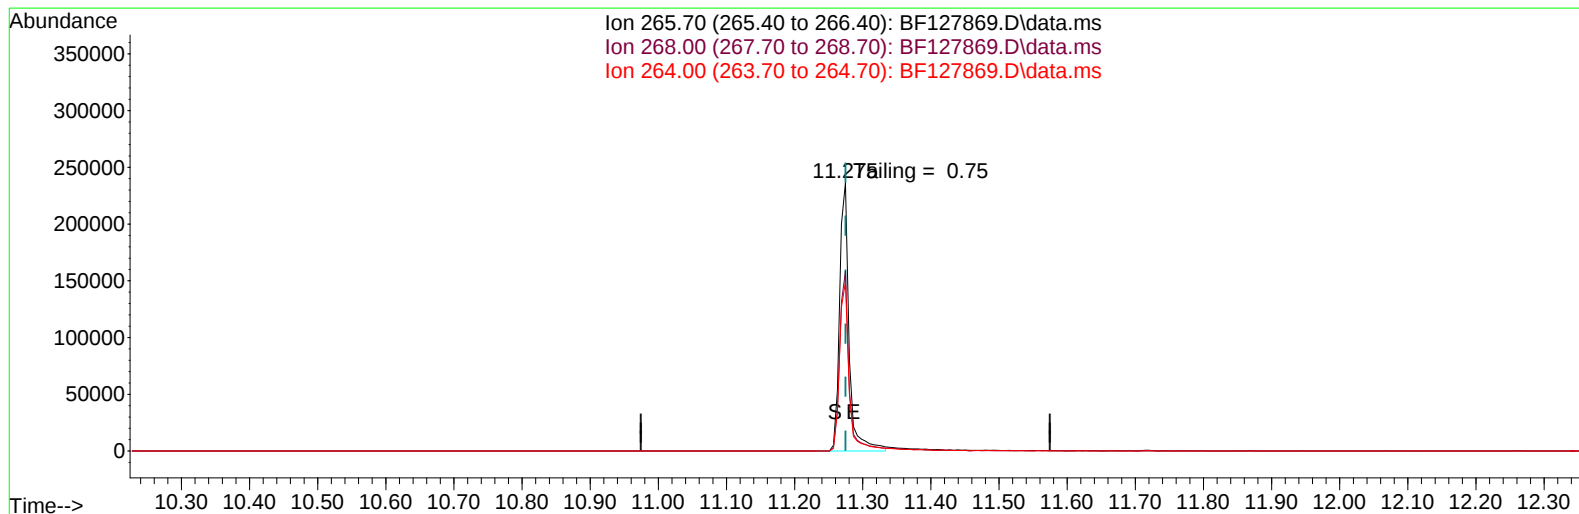

TIC: BF127869.D\data.ms

(70) Pentachlorophenol (C)




11.275min (-0.000) 473855.03 ng

response 234427

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	67.02
264.00	66.40	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127869.D
 Acq On : 25 Apr 2022 09:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 17:09:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

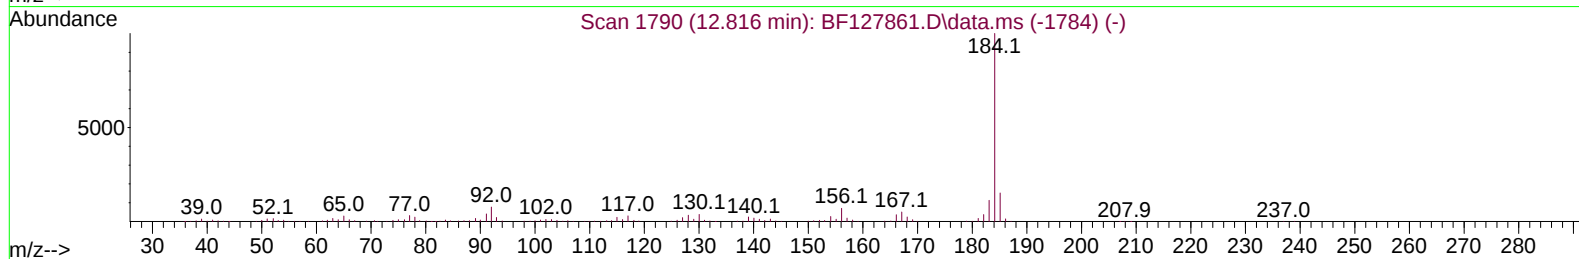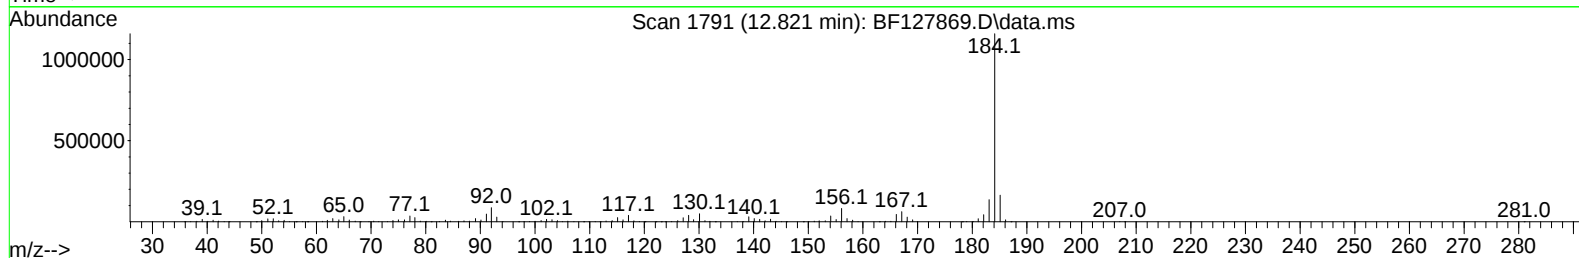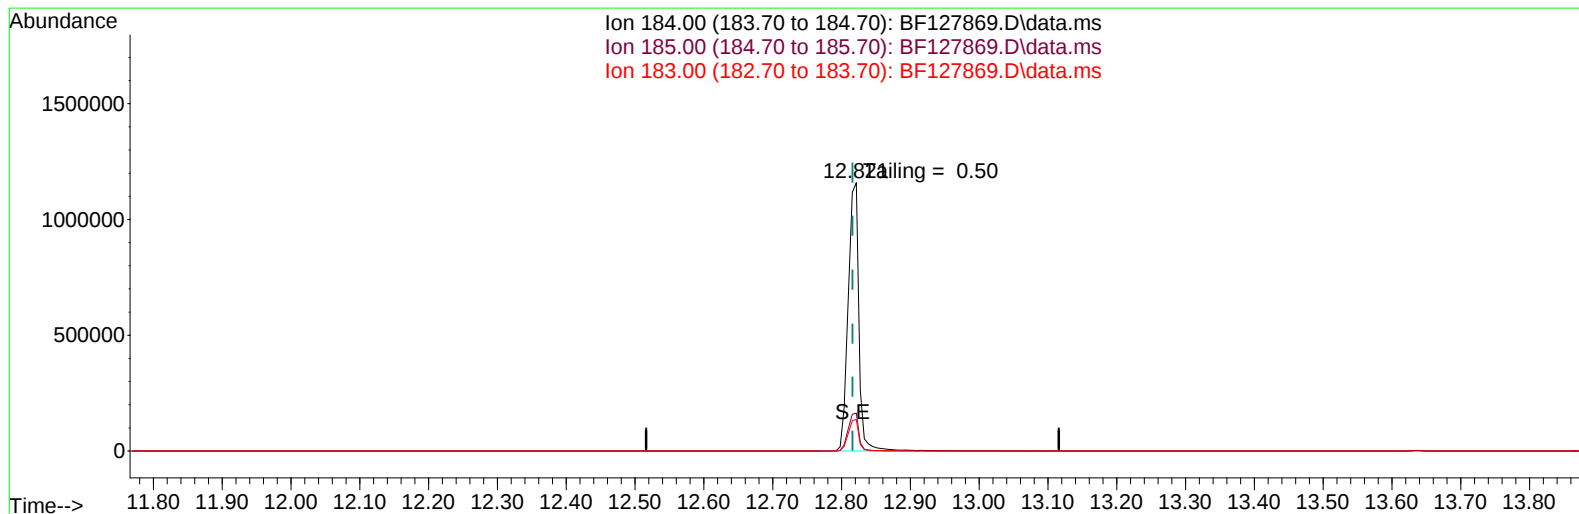

TIC: BF127869.D\data.ms

(77) Benzidine

12.821min (+ 0.005) 7454.68 ng m

response 1250860

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.13
183.00	11.20	11.77
0.00	0.00	0.00