
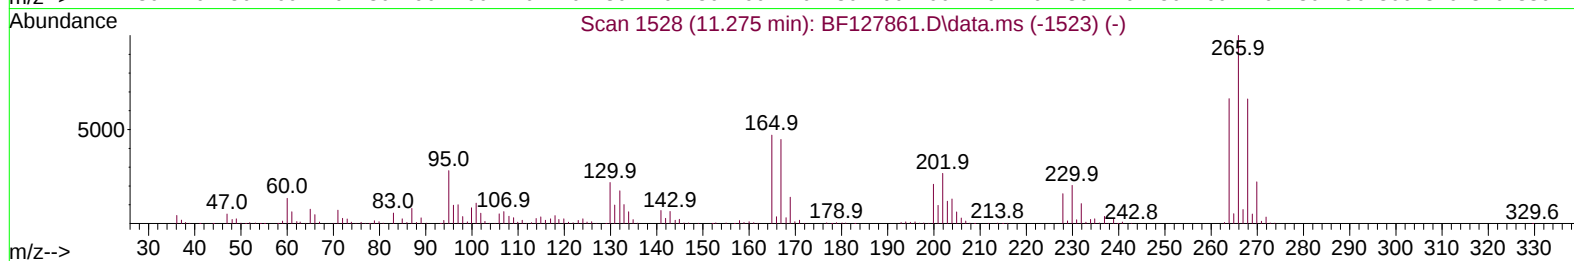
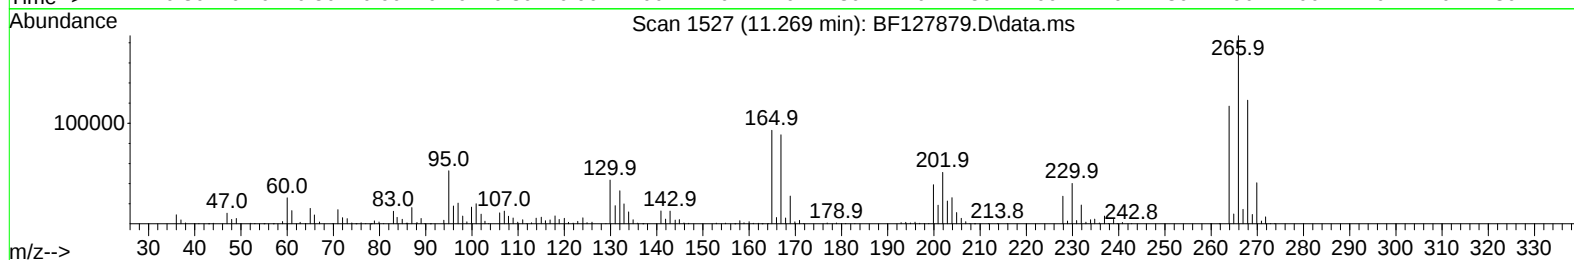


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\  
Data File : BF127879.D  
Acq On    : 25 Apr 2022  14:36  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 25 17:11:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 00:43:03 2022
Response via : Initial Calibration

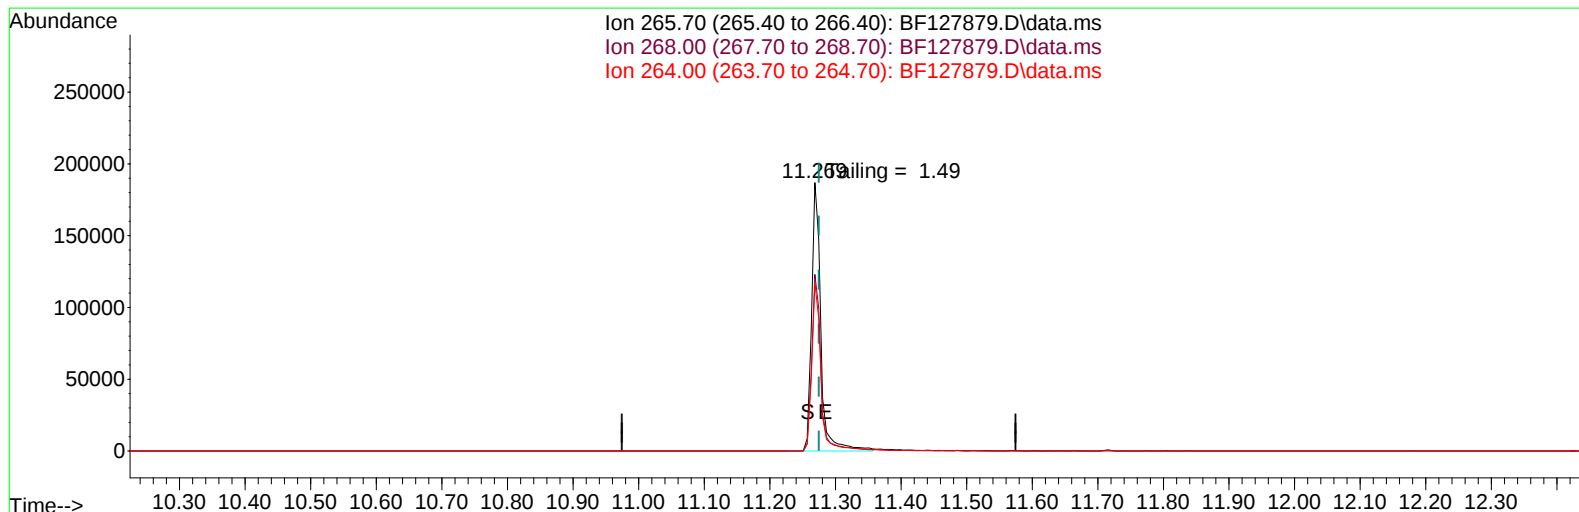

TIC: BF127879.D\data.ms

(70) Pentachlorophenol (C)




11.269min (-0.006) 26641.07 ng

response	186899
----------	--------

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.77
264.00	66.40	62.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127879.D
 Acq On : 25 Apr 2022 14:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 17:11:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 00:43:03 2022
 Response via : Initial Calibration

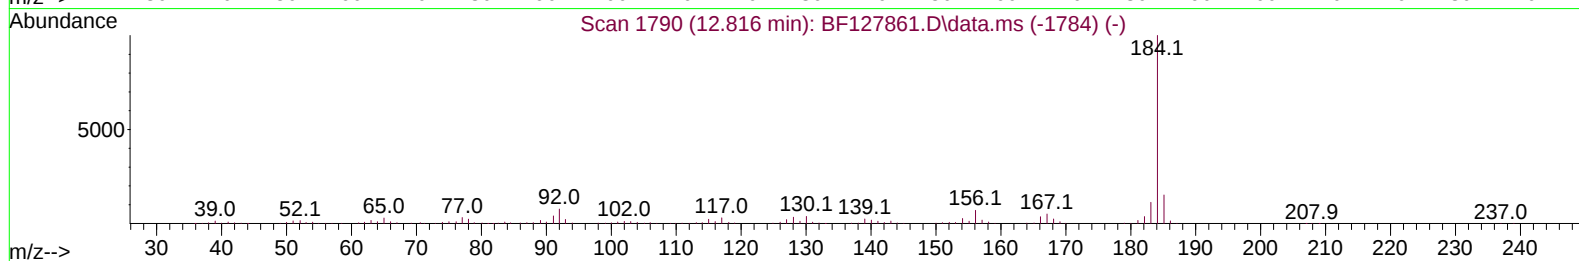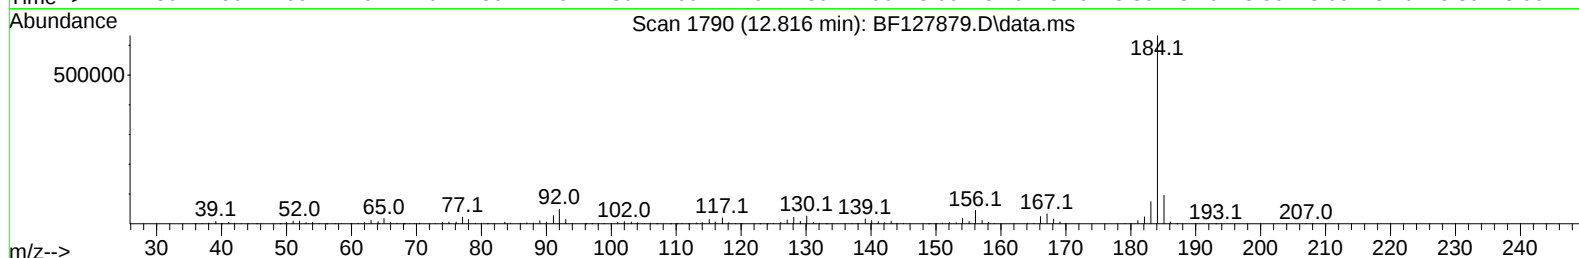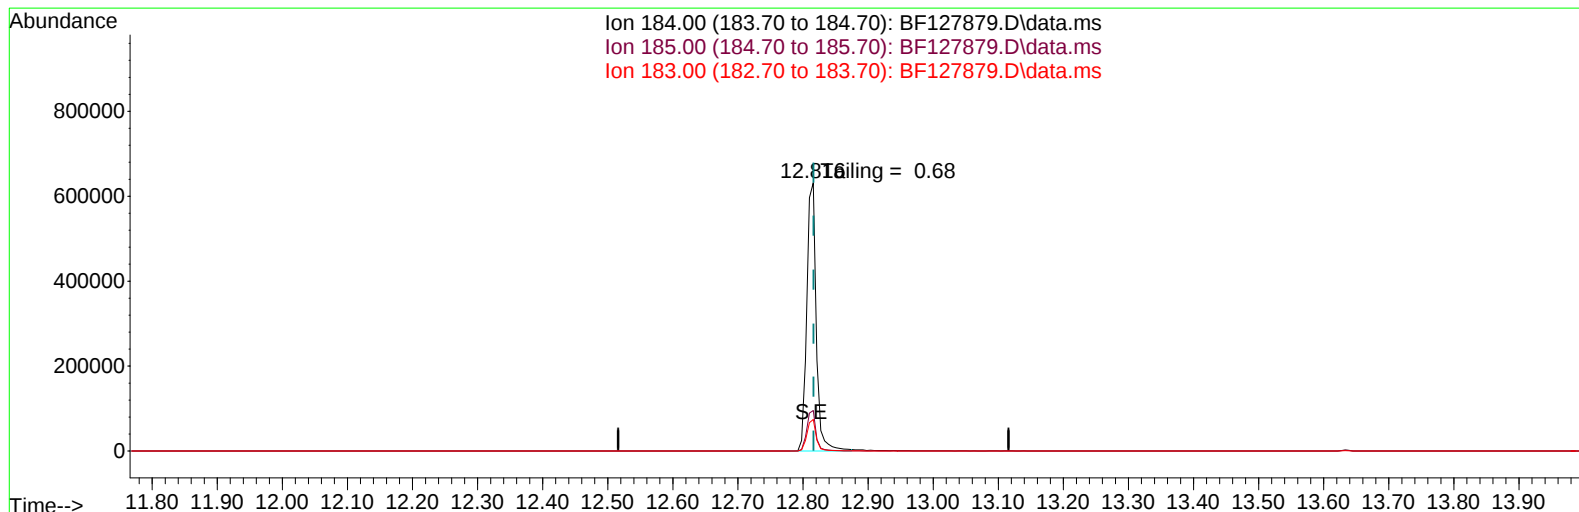

TIC: BF127879.D\data.ms

(77) Benzidine

12.816min (-0.000) 0.00 ng

response 645568

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	15.12
183.00	11.20	11.76
0.00	0.00	0.00