

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127871.D
 Acq On : 25 Apr 2022 10:45
 Operator : CG\JU
 Sample : PB144283BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144283BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.569	553	558	561	rBV	4186733	4709497	78.94%	13.137%
2	6.563	721	727	730	rBV	3953067	4833457	81.02%	13.483%
3	6.940	787	791	794	rBV	1200665	957083	16.04%	2.670%
4	7.504	881	887	890	rBV	3097060	3340775	56.00%	9.319%
5	8.222	1004	1009	1013	rBV	1386140	1271162	21.31%	3.546%
6	9.298	1186	1192	1196	rBV	5188852	5666894	94.99%	15.808%
7	9.981	1303	1308	1312	rBV	1708517	1472706	24.69%	4.108%
8	10.775	1438	1443	1446	rBV	3599963	3458515	57.97%	9.648%
9	11.475	1558	1562	1570	rBV	1805167	1547729	25.94%	4.317%
10	13.069	1827	1833	1836	rBV	5519086	5965811	100.00%	16.642%
11	14.116	2007	2011	2021	rBV	1360180	1318417	22.10%	3.678%
12	15.633	2263	2269	2278	rBV	828712	1090187	18.27%	3.041%
13	17.627	2600	2608	2623	rVB3	51682	216370	3.63%	0.604%


Sum of corrected areas: 35848603

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127871.D
Acq On : 25 Apr 2022 10:45
Operator : CG\JU
Sample : PB144283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144283BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

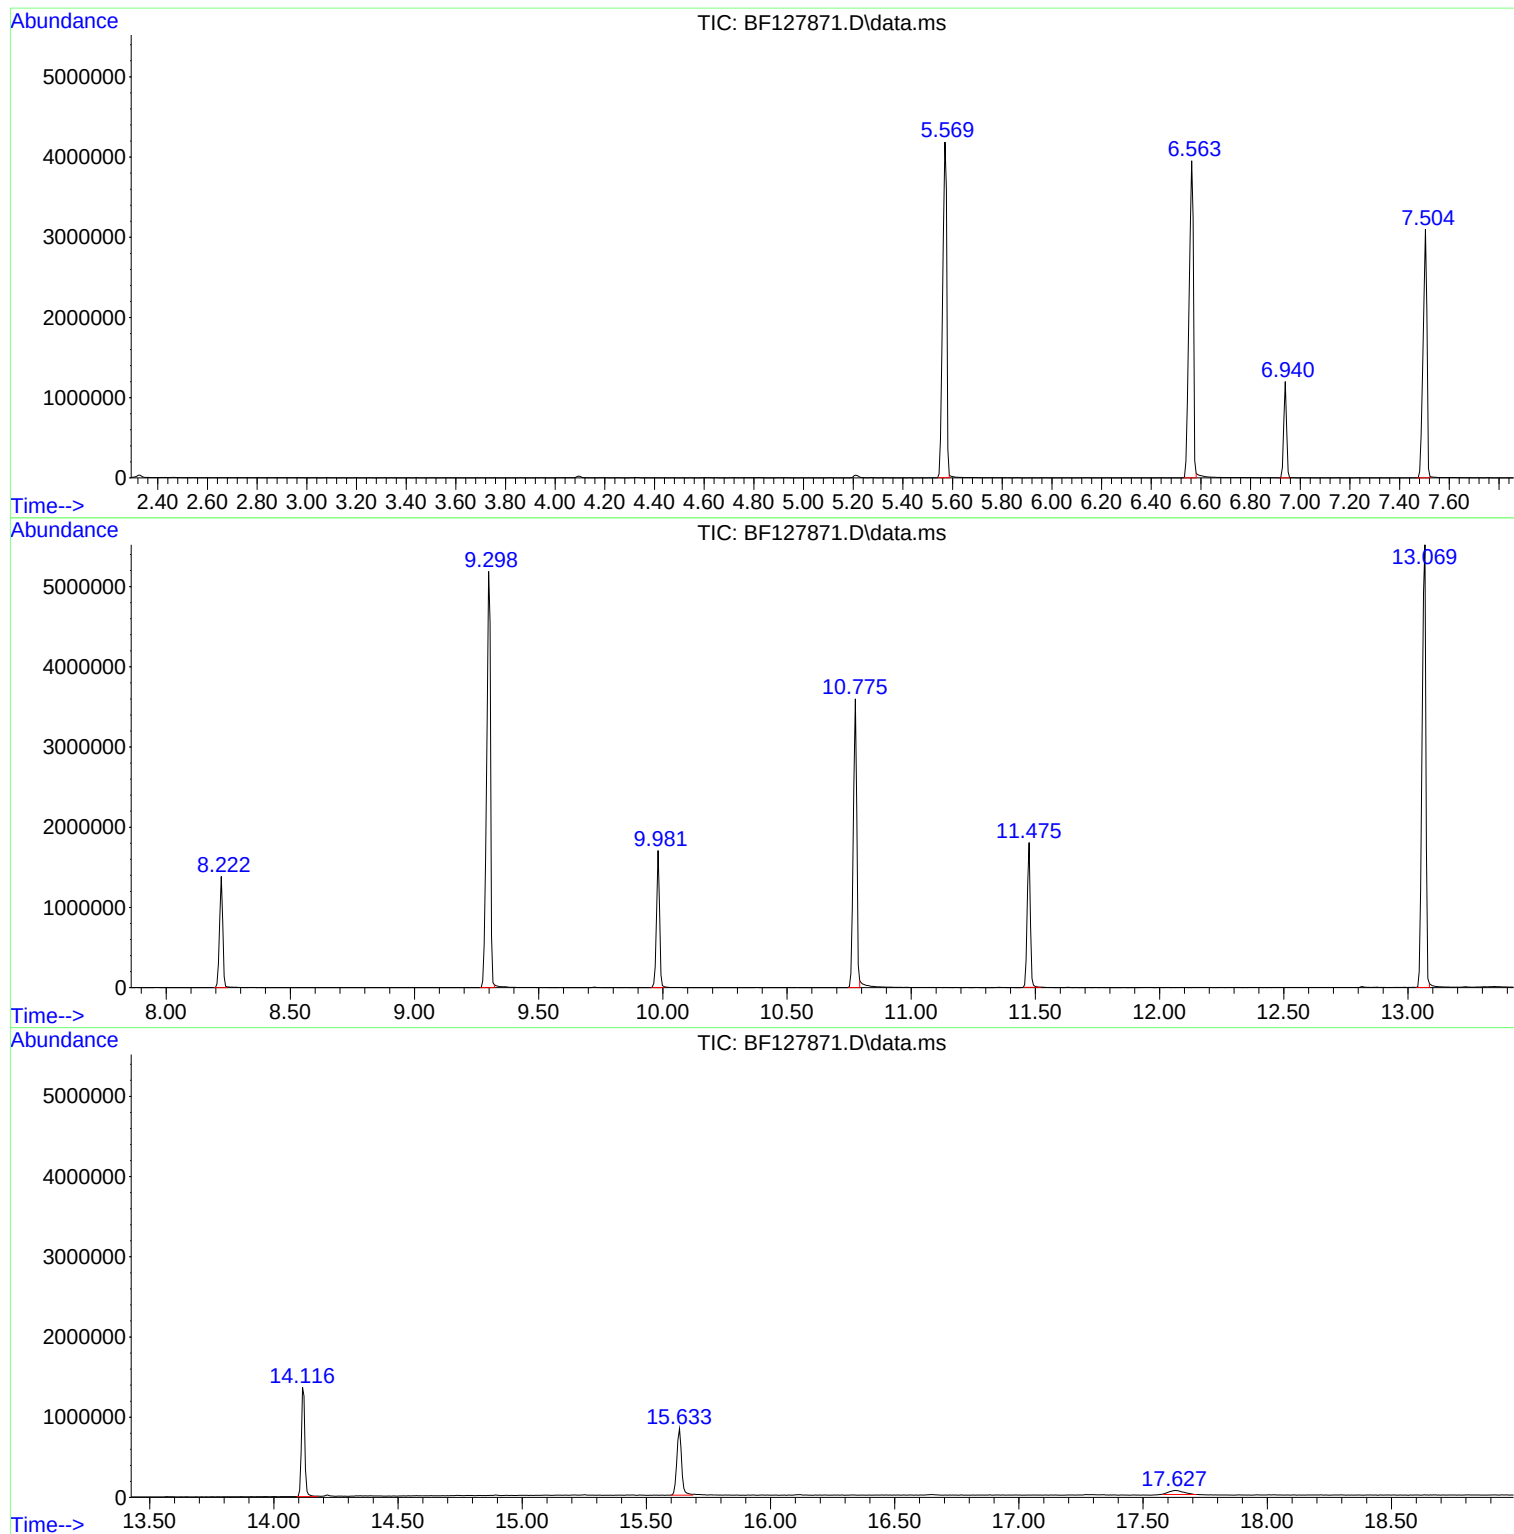

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127871.D
Acq On : 25 Apr 2022 10:45
Operator : CG\JU
Sample : PB144283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB144283BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (1,1'-Biphenyl)-4,4'-diamin... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
17.627	3.97 ng	216370	Perylene-d12	15.633	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	(1,1'-Biphenyl)-4,4'-diamine, N,...	360	C26H20N2	006311-48-4	87
2	1,10-Phenanthroline, 2,9-dimethy...	360	C26H20N2	004733-39-5	47
3	Benzaldehyde, 4-hydroxy-3,5-dime...	360	C18H20N2O6	014414-32-5	47
4	1,3,2-Dioxaborolane, bis(spiro[4...	360	C20H13BO6	1000150-23-7	43
5	N,N'-di-2-Naphthyl-p-phenylenedi...	360	C26H20N2	000093-46-9	43

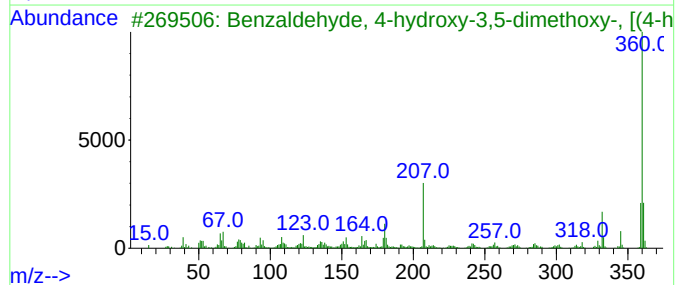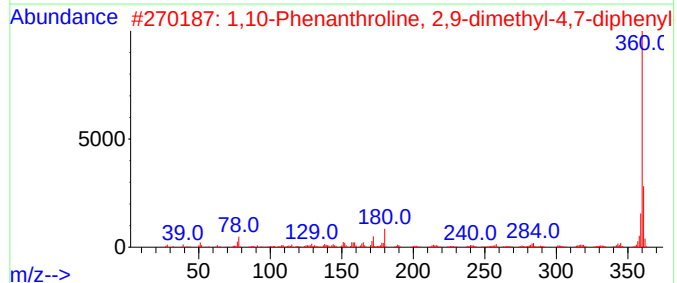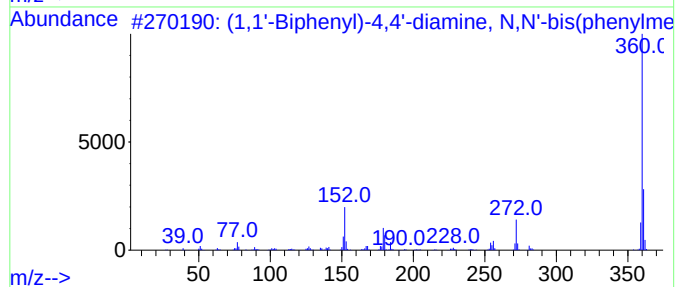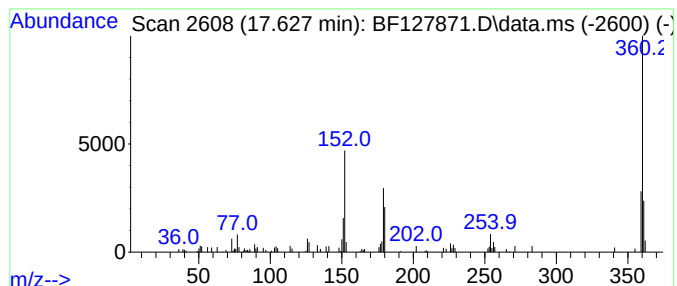

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127871.D
Acq On : 25 Apr 2022 10:45
Operator : CG\JU
Sample : PB144283BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144283BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(1,1'-Biphenyl)...	17.627	4.0	ng	216370	6	15.633	1090190	20.0