

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
 Data File : BF127874.D
 Acq On : 25 Apr 2022 12:12
 Operator : CG\JU
 Sample : N2494-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 2

Instrument :
 BNA_F
 ClientSampleId :
 MH-1S

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.181	487	492	499	rVB	76547	97795	2.46%	0.311%
2	5.563	552	557	560	rBV	3183364	3044770	76.56%	9.694%
3	6.563	721	727	730	rBV	2911338	3168329	79.67%	10.087%
4	6.939	787	791	795	rBV	2035457	1641372	41.27%	5.226%
5	7.504	881	887	890	rBV	2268433	2153034	54.14%	6.855%
6	7.675	912	916	919	rVB	50961	45984	1.16%	0.146%
7	8.222	1005	1009	1013	rBV	2344276	2125946	53.46%	6.769%
8	9.298	1187	1192	1195	rBV	4200366	3868812	97.28%	12.318%
9	9.980	1303	1308	1312	rBV	2555929	2474718	62.23%	7.879%
10	10.769	1438	1442	1446	rBV	2180981	2242105	56.38%	7.138%
11	11.474	1558	1562	1565	rBV	3000130	2590834	65.15%	8.249%
12	13.063	1827	1832	1835	rBV	4343581	3976788	100.00%	12.661%
13	14.121	2003	2012	2015	rBV	2242937	2131227	53.59%	6.785%
14	14.215	2024	2028	2034	rVB	67592	77081	1.94%	0.245%
15	15.633	2263	2269	2278	rBV	1262864	1770037	44.51%	5.635%




Sum of corrected areas: 31408832

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127874.D
Acq On : 25 Apr 2022 12:12
Operator : CG\JU
Sample : N2494-01
Misc :
ALS Vial : 6 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
MH-1S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

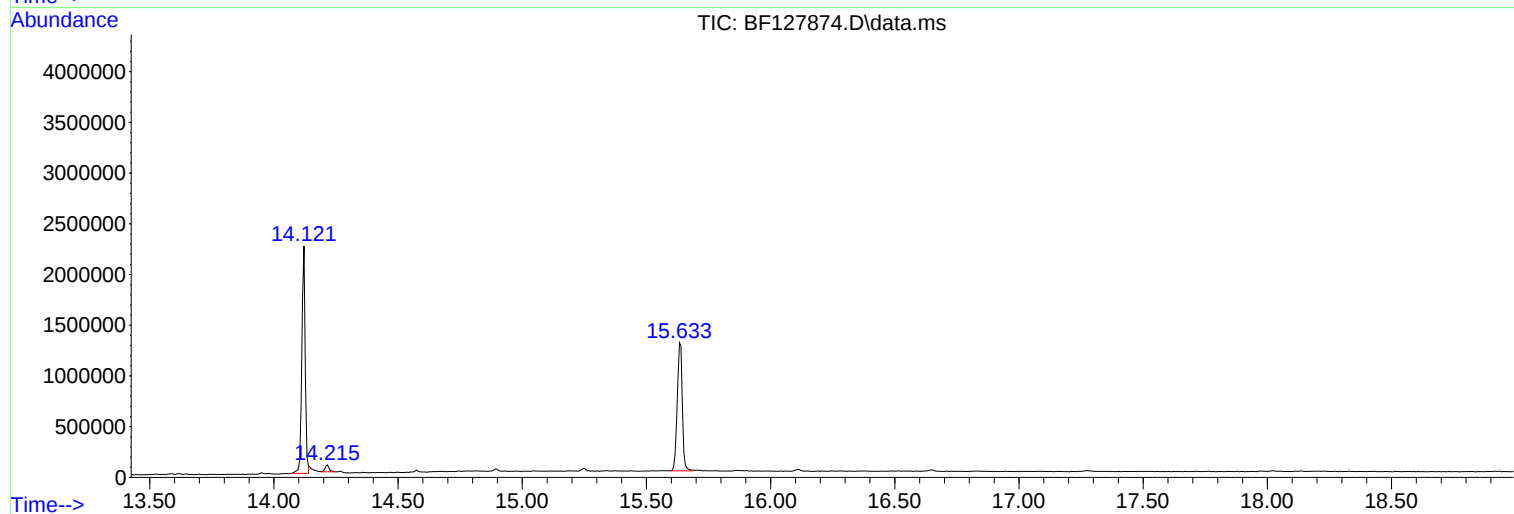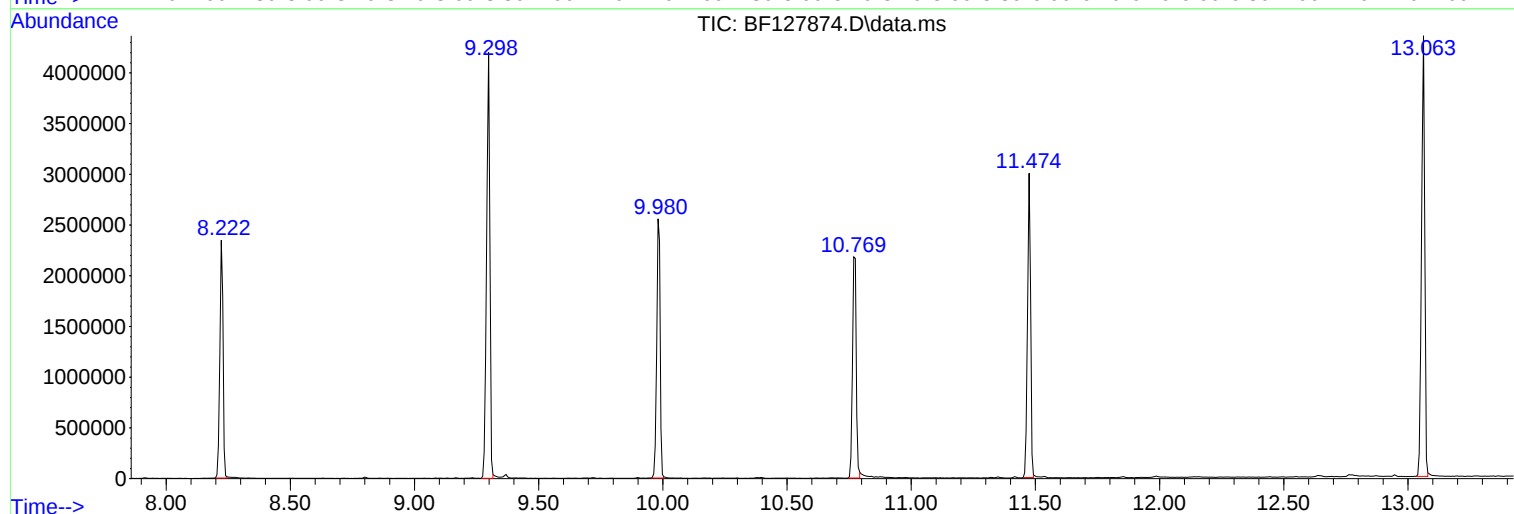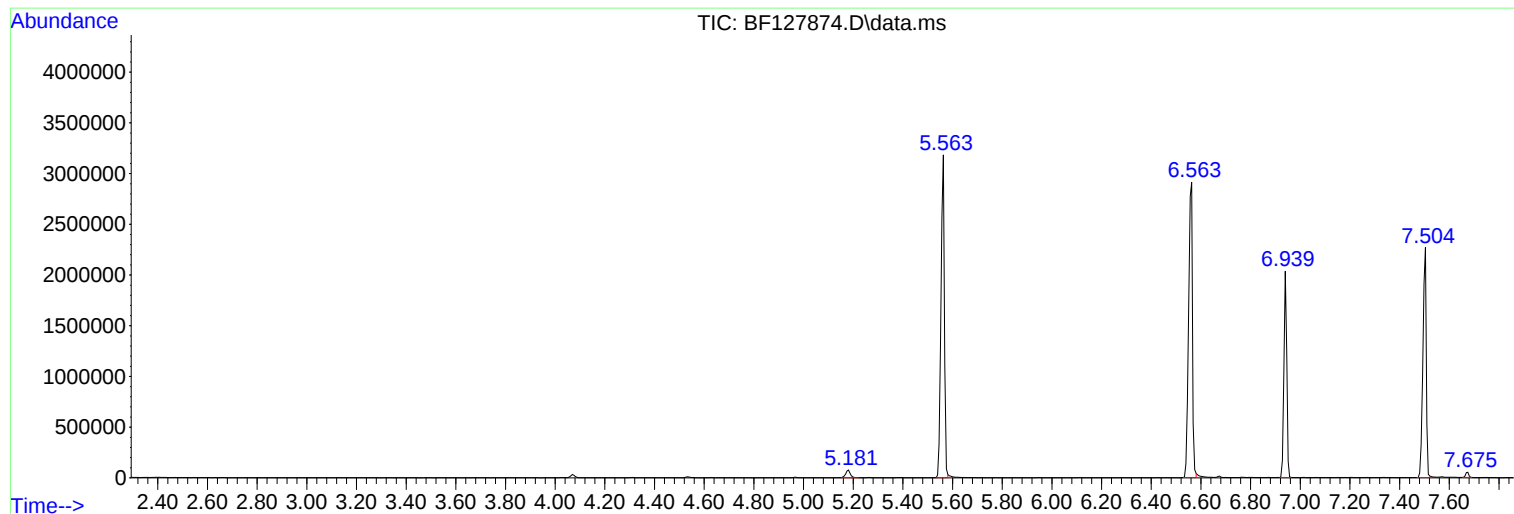

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127874.D
Acq On : 25 Apr 2022 12:12
Operator : CG\JU
Sample : N2494-01
Misc :
ALS Vial : 6 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
MH-1S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF042522\
Data File : BF127874.D
Acq On : 25 Apr 2022 12:12
Operator : CG\JU
Sample : N2494-01
Misc :
ALS Vial : 6 Sample Multiplier: 2

Instrument :
BNA_F
ClientSampleId :
MH-1S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------